

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003304.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 15:58
 Operator : AJ\SJ
 Sample : K1173-05
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:55:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	2128633	14.877 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	1707934	10.460 ug/ml
5) N-HEXADECANE	9.773	774048	4.714 ug/ml
8) N-DOCOSANE	13.703	118313	0.728 ug/ml
10) N-TETRACOSANE	14.809	262044	1.634 ug/ml
11) N-HEXACOSANE	15.833	339151	2.144 ug/ml
12) N-OCTACOSANE	16.785	446045	2.832 ug/ml
13) N-TRIACONTANE	17.676	473640	3.017 ug/ml
14) N-DOTRIACONTANE	18.510	372214	2.560 ug/ml
15) N-TETRATRIACONTANE	19.298	104164	0.788 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003304.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 15:58
 Operator : AJ\SJ
 Sample : K1173-05
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampled :

Integration File: autoint1.e
 Quant Time: Jan 18 20:55:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

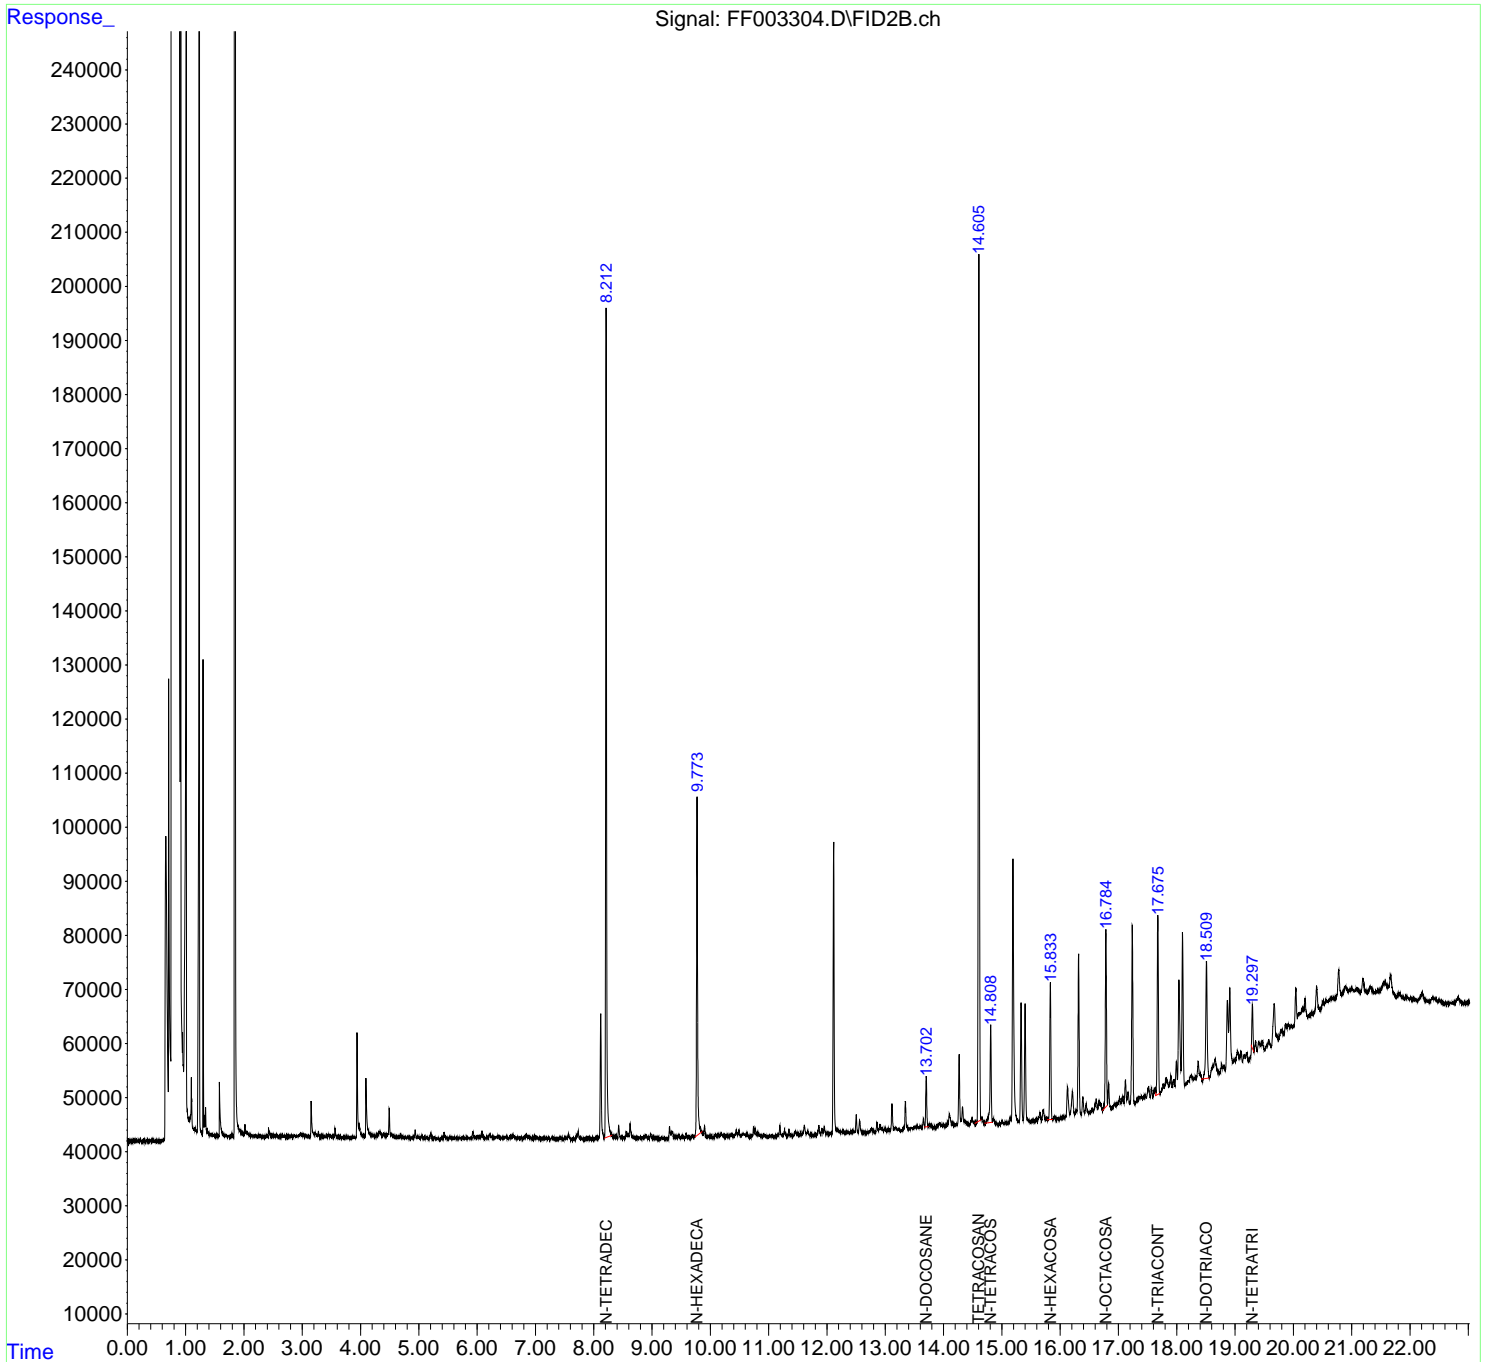

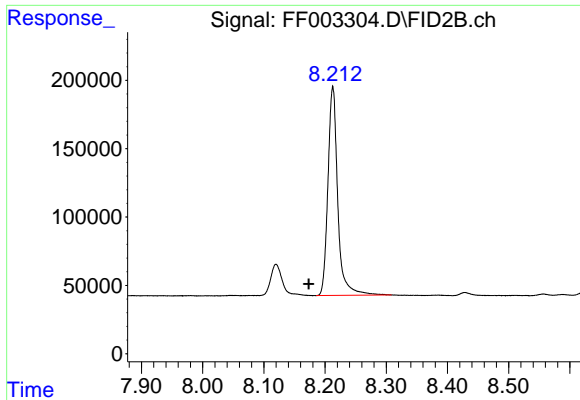


#4 N-TETRADECANE
 R.T.: 8.213 min
 Delta R.T.: 0.039 min
 Response: 1707934
 Conc: 10.46 ug/ml


Instrument :
 FID_F
 ClientSampled :

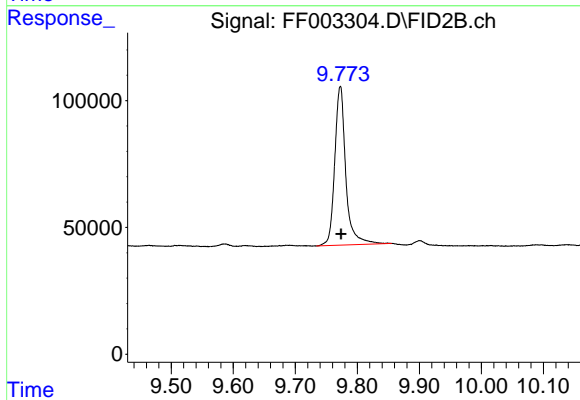


#5 N-HEXADECANE
 R.T.: 9.773 min
 Delta R.T.: 0.000 min
 Response: 774048
 Conc: 4.71 ug/ml

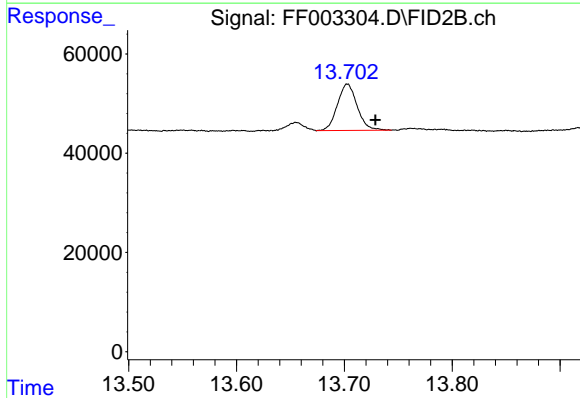

#8 N-DOCOSANE
 R.T.: 13.703 min
 Delta R.T.: -0.026 min
 Response: 118313
 Conc: 0.73 ug/ml

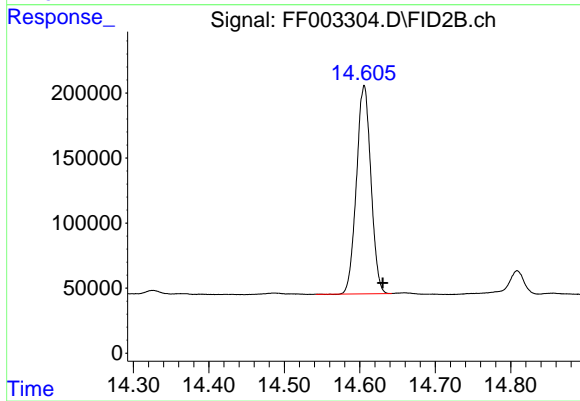


#9 TETRACOSANE-d50 (SURROGATE)
 R.T.: 14.606 min
 Delta R.T.: -0.025 min
 Response: 2128633
 Conc: 14.88 ug/ml

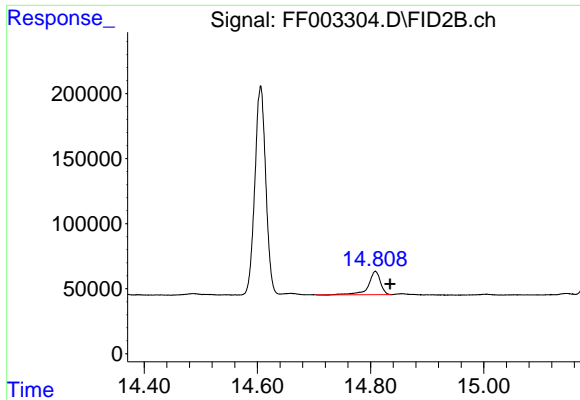


#10 N-TETRACOSANE
 R.T.: 14.809 min
 Delta R.T.: -0.026 min
 Response: 262044
 Conc: 1.63 ug/ml


Instrument :
 FID_F
 ClientSampleId :

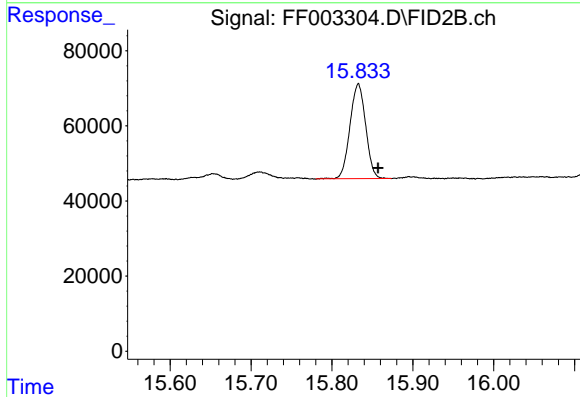


#11 N-HEXACOSANE
 R.T.: 15.833 min
 Delta R.T.: -0.025 min
 Response: 339151
 Conc: 2.14 ug/ml

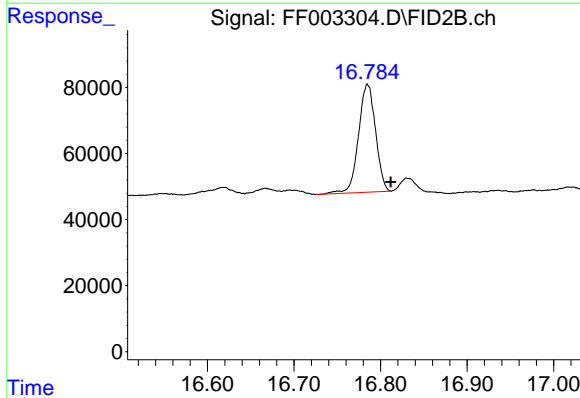

#12 N-OCTACOSANE
 R.T.: 16.785 min
 Delta R.T.: -0.027 min
 Response: 446045
 Conc: 2.83 ug/ml

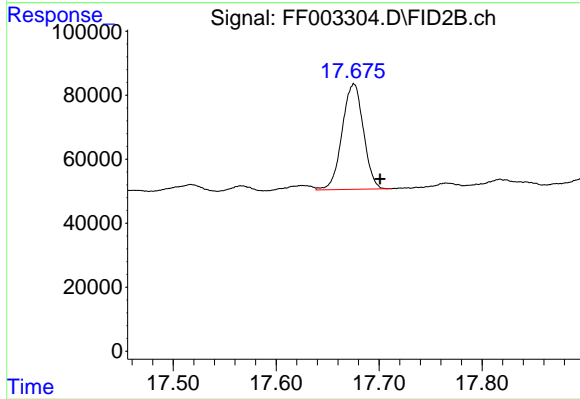


#13 N-TRIACONTANE
 R.T.: 17.676 min
 Delta R.T.: -0.025 min
 Response: 473640
 Conc: 3.02 ug/ml

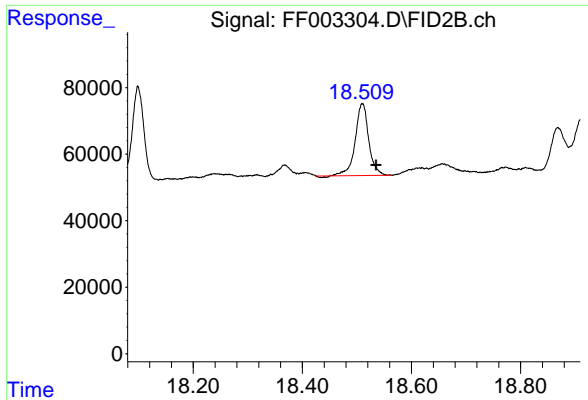

#14 N-DOTRIACONTANE

R.T.: 18.510 min
Delta R.T.: -0.025 min
Response: 372214
Conc: 2.56 ug/ml

Instrument :
FID_F
ClientSampleId :

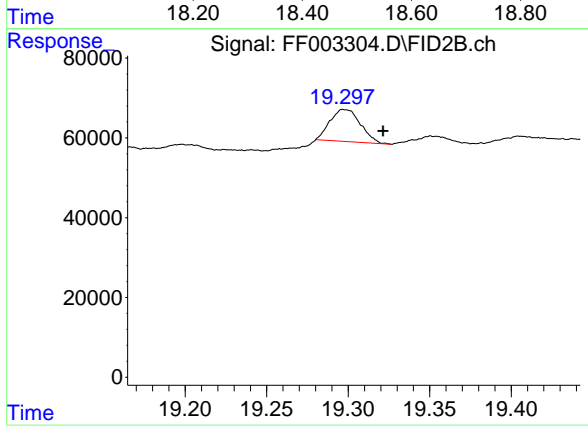

#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.024 min
Response: 104164
Conc: 0.79 ug/ml