

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003306.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 16:58
 Operator : AJ\SJ
 Sample : K1011-05 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:56:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	170760	1.193 ug/ml
Target Compounds			
7) N-EICOSANE	12.557	431459	2.628 ug/ml
10) N-TETRACOSANE	14.780f	140914	0.879 ug/ml
11) N-HEXACOSANE	15.836	199195	1.259 ug/ml
12) N-OCTACOSANE	16.789	393442	2.498 ug/ml
13) N-TRIACONTANE	17.679	402209	2.562 ug/ml
14) N-DOTRIACONTANE	18.514	316233	2.175 ug/ml
15) N-TETRATRIACONTANE	19.312	207586	1.570 ug/ml
16) N-HEXATRIACONTANE	20.112	45786	0.388 ug/ml
17) N-OCTATRIACONTANE	20.786	289107	2.767 ug/ml
18) N-TETRACONTANE	21.674	121040	1.137 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003306.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 16:58
Operator : AJ\SJ
Sample : K1011-05 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 18 20:56:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

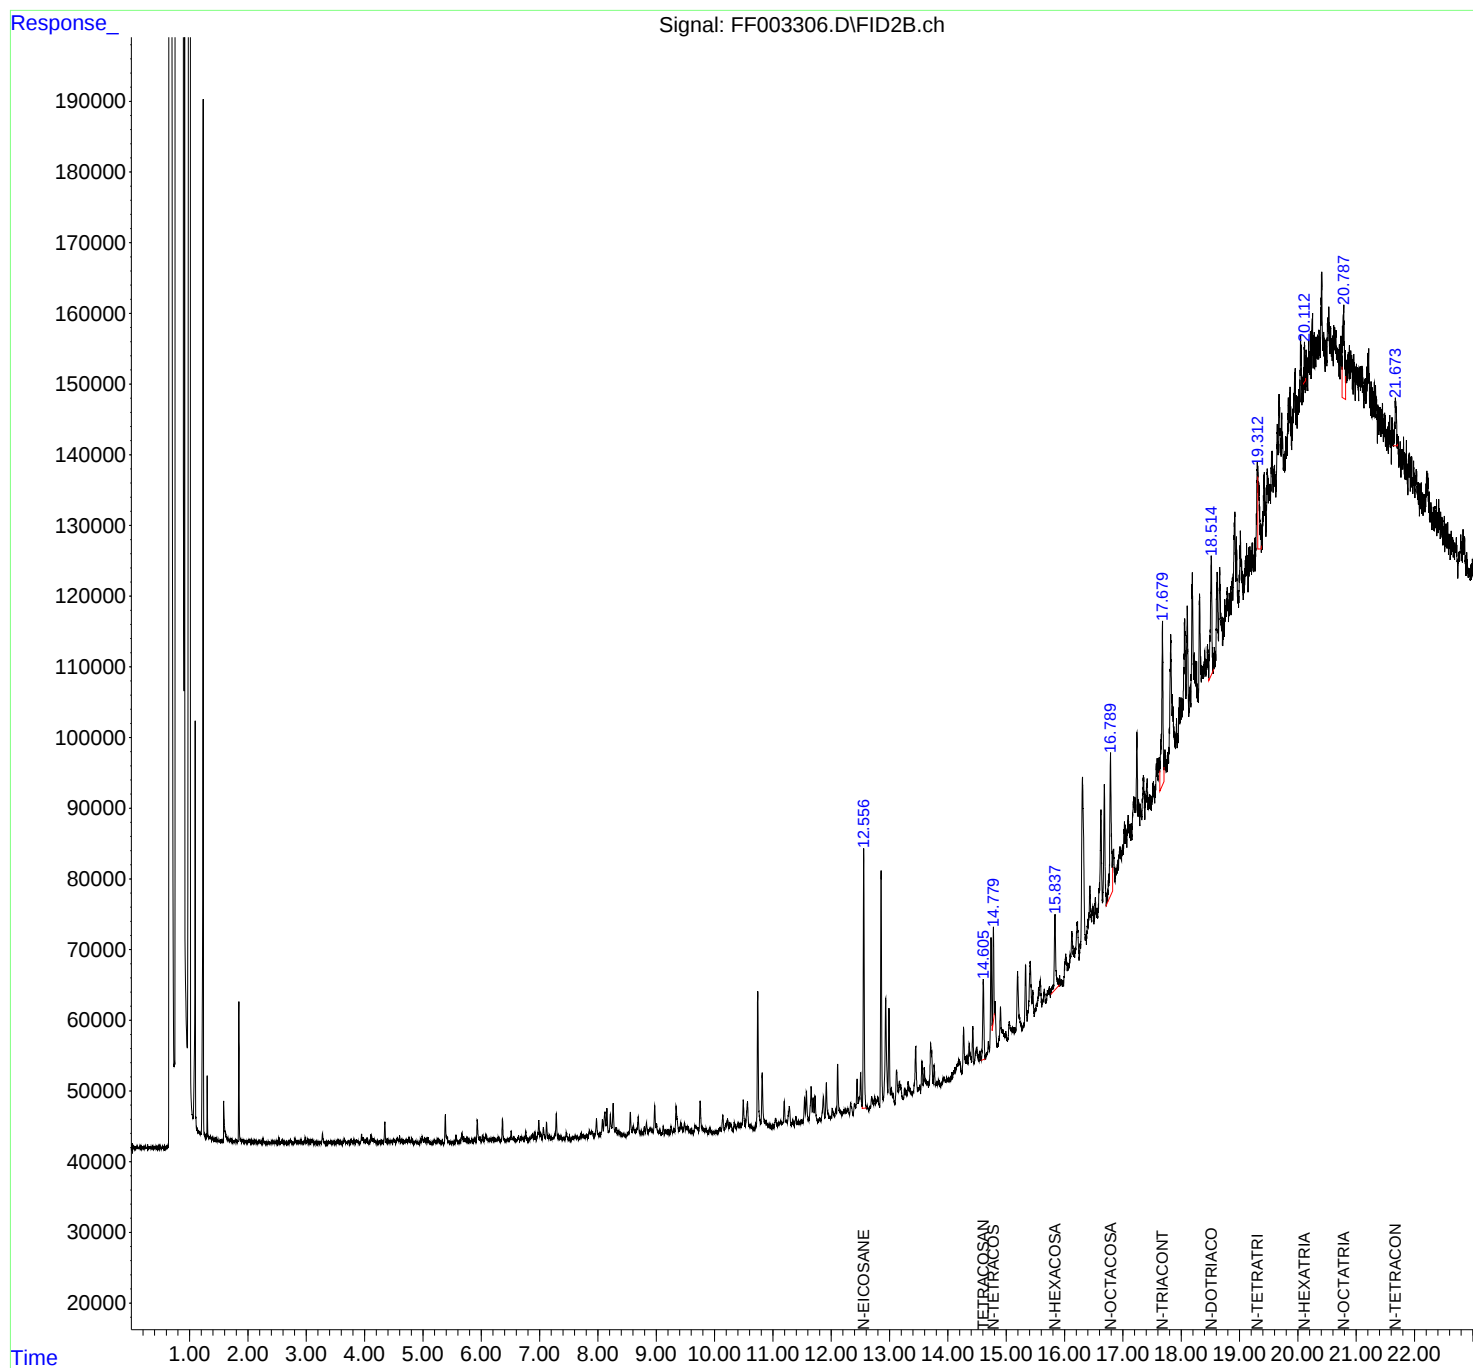


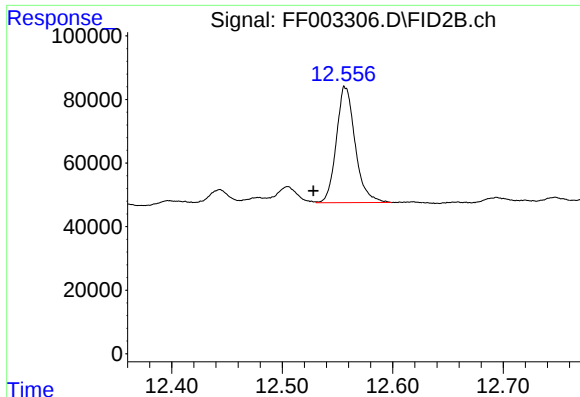

#7 N-EICOSANE


R.T.: 12.557 min
Delta R.T.: 0.029 min
Response: 431459
Conc: 2.63 ug/ml

Instrument :
FID_F
ClientSampleId :

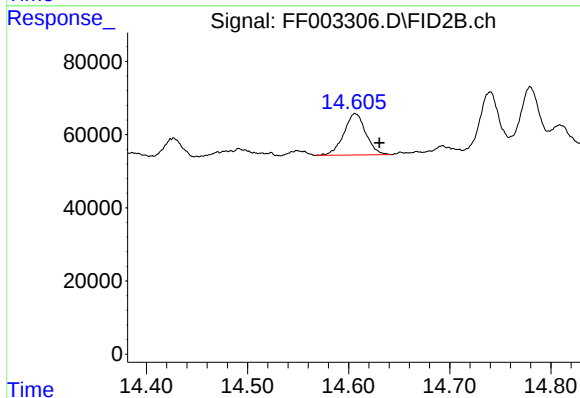


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.606 min
Delta R.T.: -0.024 min
Response: 170760
Conc: 1.19 ug/ml

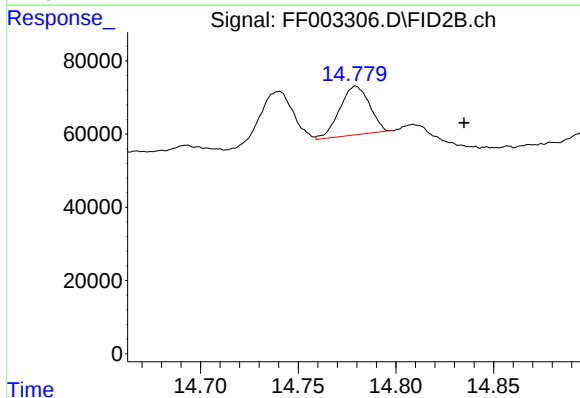


#10 N-TETRACOSANE

R.T.: 14.780 min
Delta R.T.: -0.055 min
Response: 140914
Conc: 0.88 ug/ml

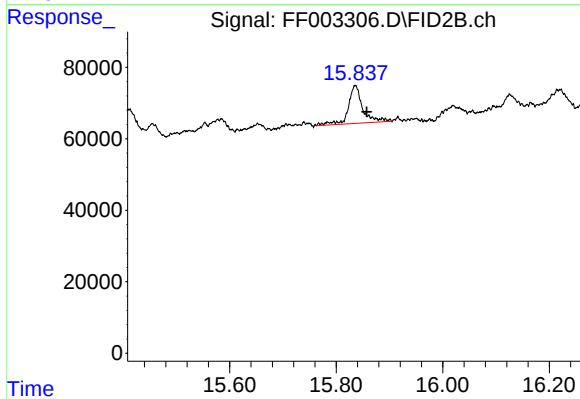

#11 N-HEXACOSANE


R.T.: 15.836 min
Delta R.T.: -0.021 min
Response: 199195
Conc: 1.26 ug/ml

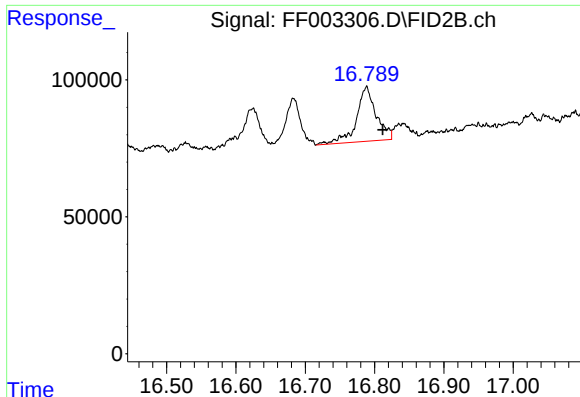

#12 N-OCTACOSANE


R.T.: 16.789 min
Delta R.T.: -0.023 min
Response: 393442
Conc: 2.50 ug/ml

Instrument :
FID_F
ClientSampleId :

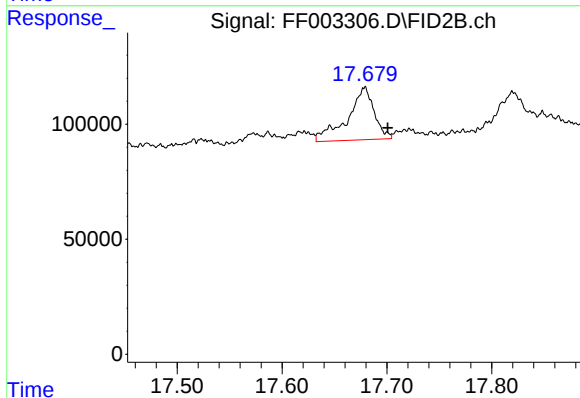


#13 N-TRIACONTANE

R.T.: 17.679 min
Delta R.T.: -0.022 min
Response: 402209
Conc: 2.56 ug/ml

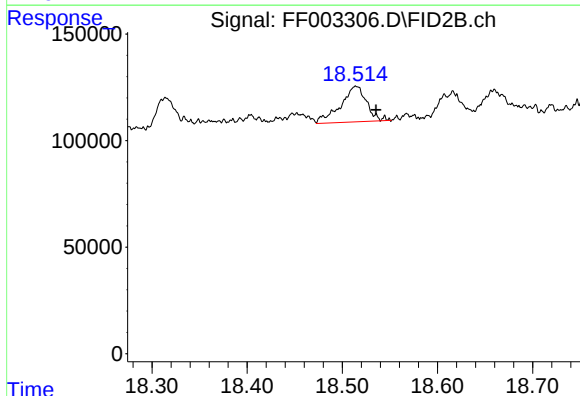


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.021 min
Response: 316233
Conc: 2.17 ug/ml

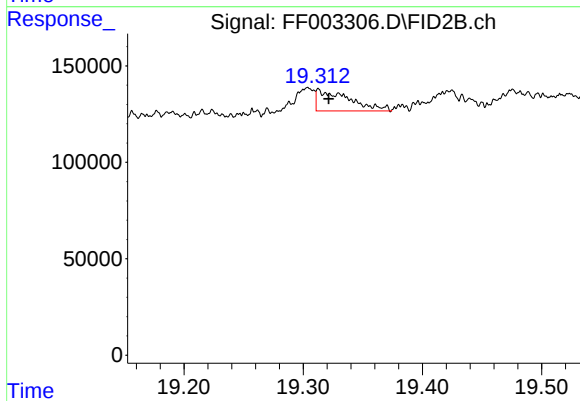

#15 N-TETRATRIACONTANE


R.T.: 19.312 min
Delta R.T.: -0.009 min
Response: 207586
Conc: 1.57 ug/ml

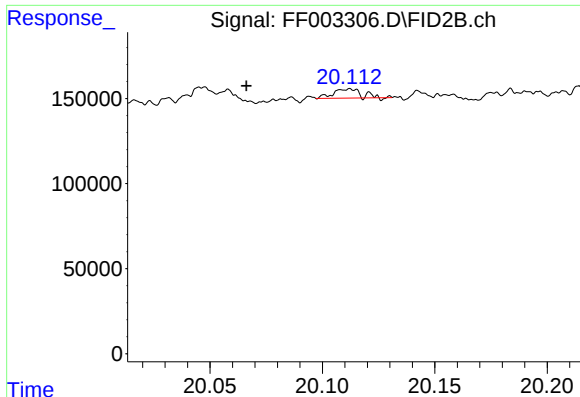

#16 N-HEXATRIACONTANE


R.T.: 20.112 min
Delta R.T.: 0.046 min
Response: 45786
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

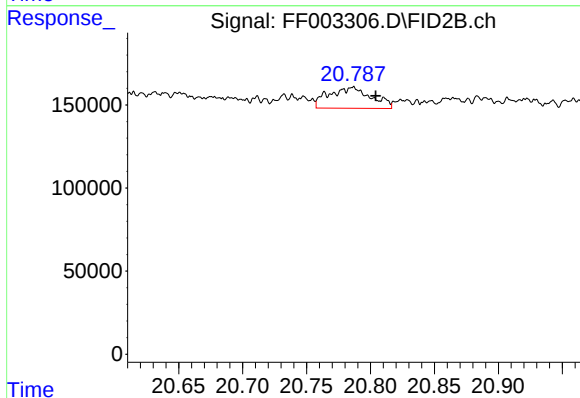

#17 N-OCTATRIACONTANE

R.T.: 20.786 min
Delta R.T.: -0.018 min
Response: 289107
Conc: 2.77 ug/ml

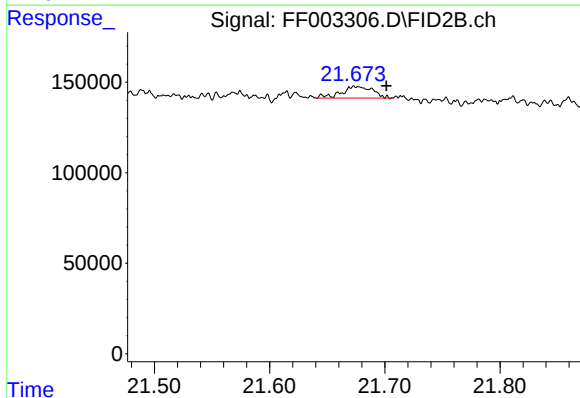

#18 N-TETRACONTANE

R.T.: 21.674 min
Delta R.T.: -0.027 min
Response: 121040
Conc: 1.14 ug/ml