

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003307.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 17:28
 Operator : AJ\SJ
 Sample : K1015-09 10X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:56:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.608	232495	1.625 ug/ml
Target Compounds				
3)	N-DODECANE	6.364	144765	0.892 ug/ml
4)	N-TETRADECANE	8.154	274653	1.682 ug/ml
5)	N-HEXADECANE	9.753	241691	1.472 ug/ml
6)	N-OCTADECANE	11.195	185974	1.125 ug/ml
7)	N-EICOSANE	12.505	196220	1.195 ug/ml
8)	N-DOCOSANE	13.707	209731	1.291 ug/ml
10)	N-TETRACOSANE	14.781f	689431	4.299 ug/ml
11)	N-HEXACOSANE	15.836	217894	1.378 ug/ml
12)	N-OCTACOSANE	16.788	387381	2.459 ug/ml
13)	N-TRIACONTANE	17.680	479046	3.051 ug/ml
14)	N-DOTRIACONTANE	18.517	355547	2.445 ug/ml
15)	N-TETRATRIACONTANE	19.315	302955	2.292 ug/ml
16)	N-HEXATRIACONTANE	20.047	145220	1.230 ug/ml
17)	N-OCTATRIACONTANE	20.822	174973	1.675 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003307.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 17:28
Operator : AJ\SJ
Sample : K1015-09 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:56:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

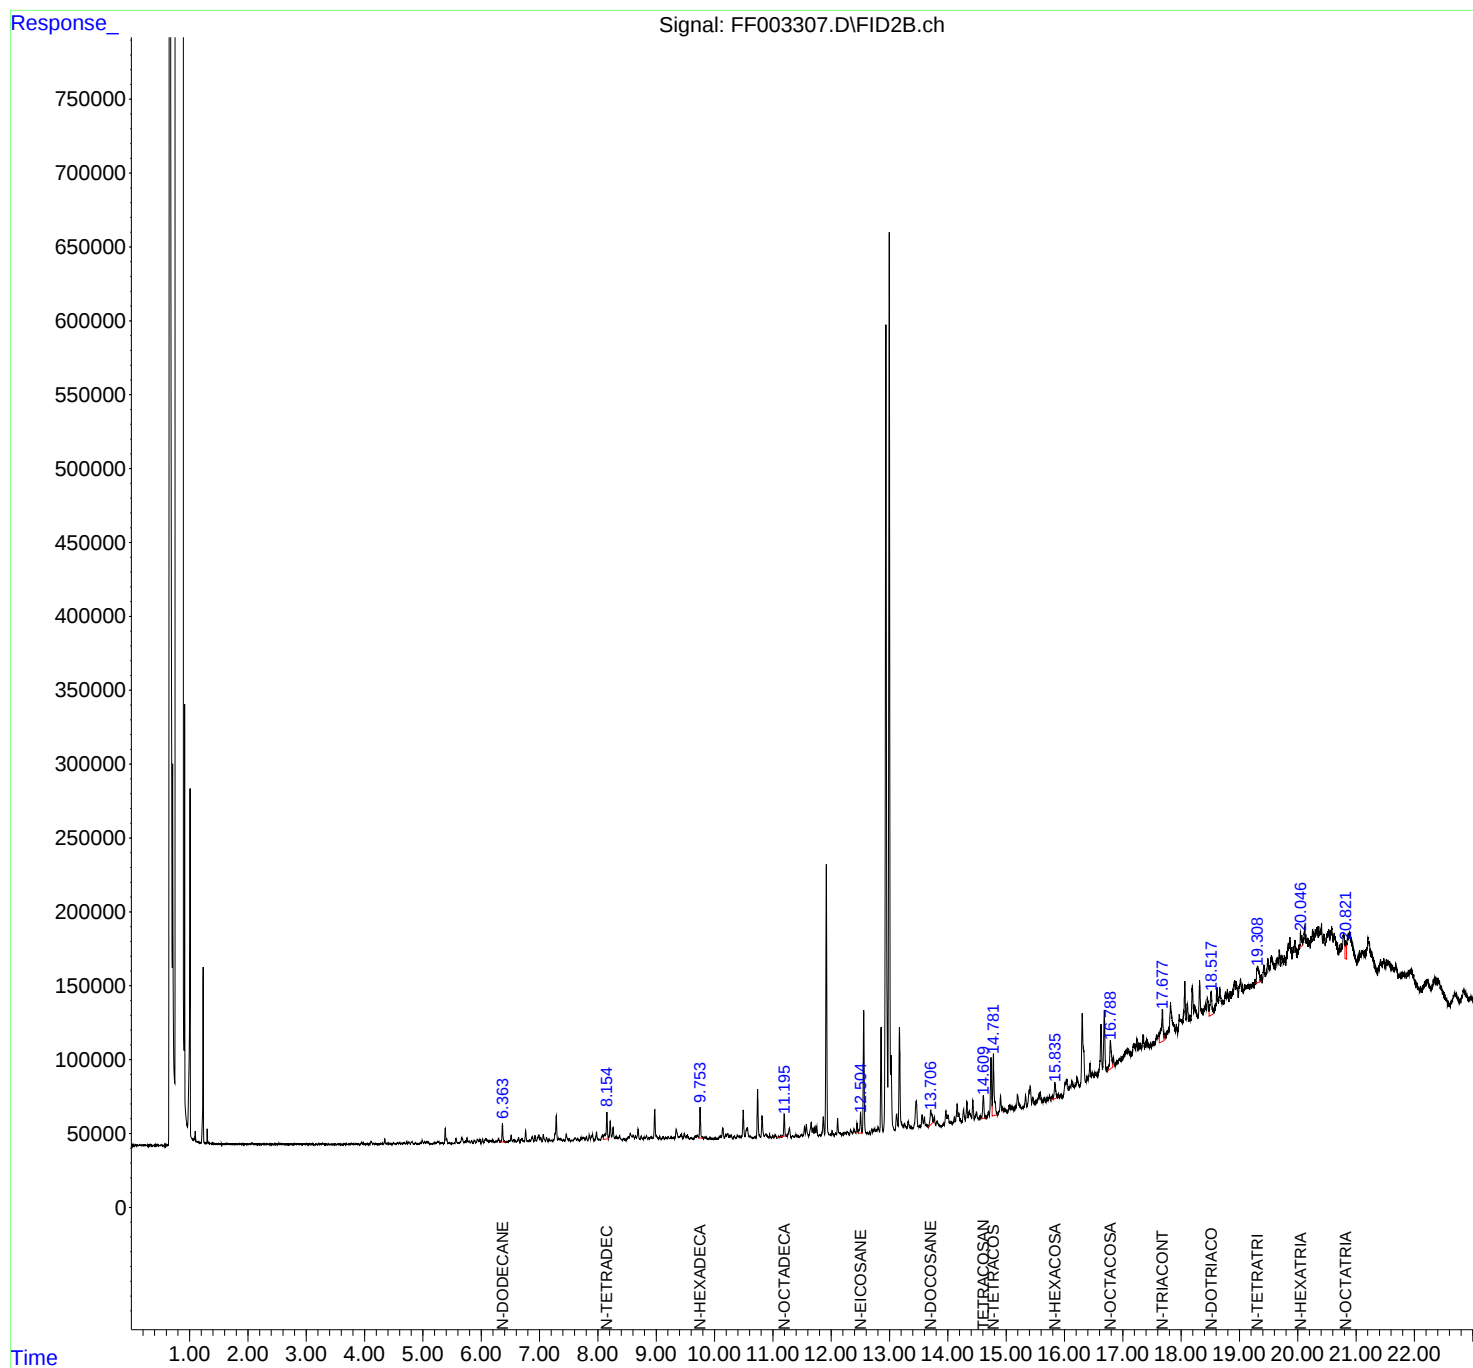


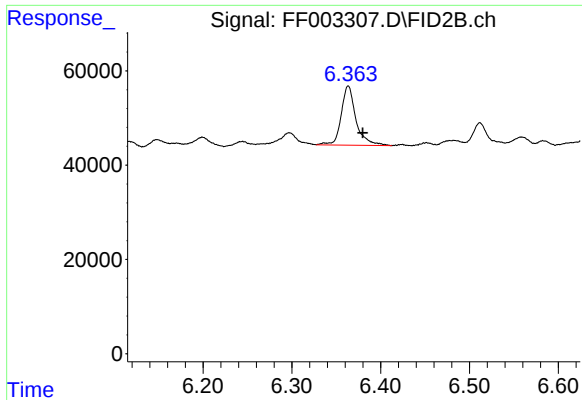

#3 N-DODECANE


R.T.: 6.364 min
Delta R.T.: -0.016 min
Response: 144765
Conc: 0.89 ug/ml

Instrument :
FID_F
ClientSampleId :

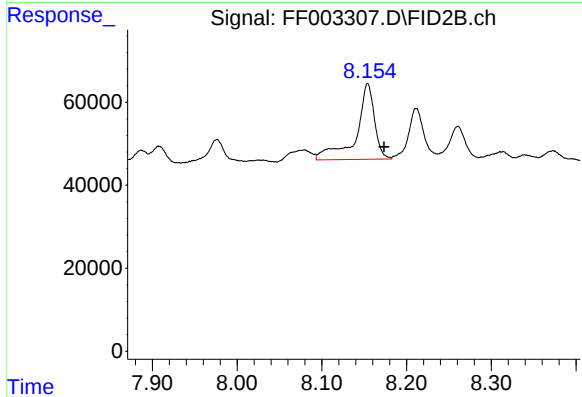


#4 N-TETRADECANE

R.T.: 8.154 min
Delta R.T.: -0.019 min
Response: 274653
Conc: 1.68 ug/ml

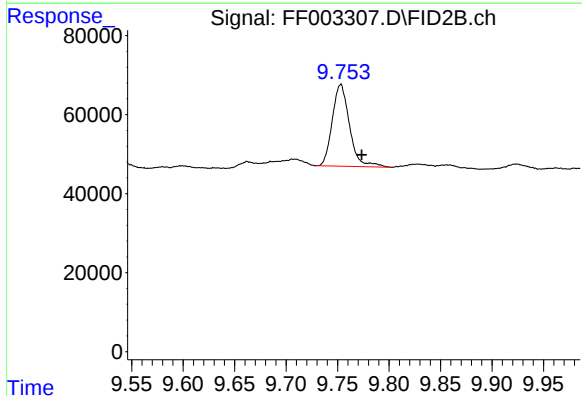


#5 N-HEXADECANE

R.T.: 9.753 min
Delta R.T.: -0.021 min
Response: 241691
Conc: 1.47 ug/ml

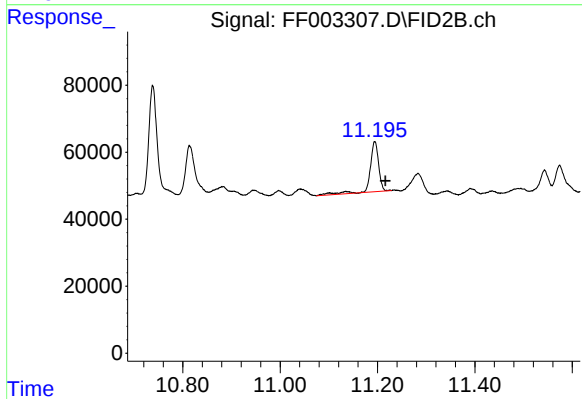

#6 N-OCTADECANE


R.T.: 11.195 min
Delta R.T.: -0.022 min
Response: 185974
Conc: 1.12 ug/ml

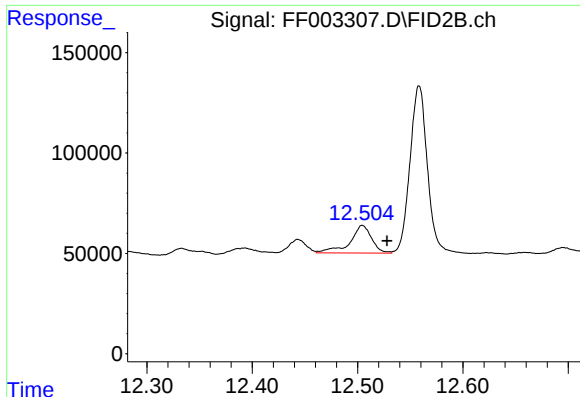

#7 N-EICOSANE


R.T.: 12.505 min
Delta R.T.: -0.023 min
Response: 196220
Conc: 1.20 ug/ml

Instrument :
FID_F
ClientSampleId :

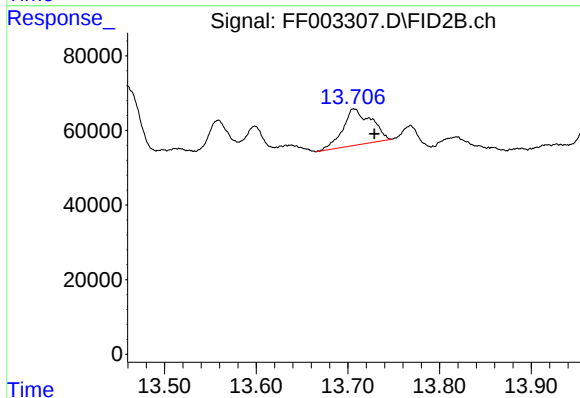


#8 N-DOCOSANE

R.T.: 13.707 min
Delta R.T.: -0.022 min
Response: 209731
Conc: 1.29 ug/ml

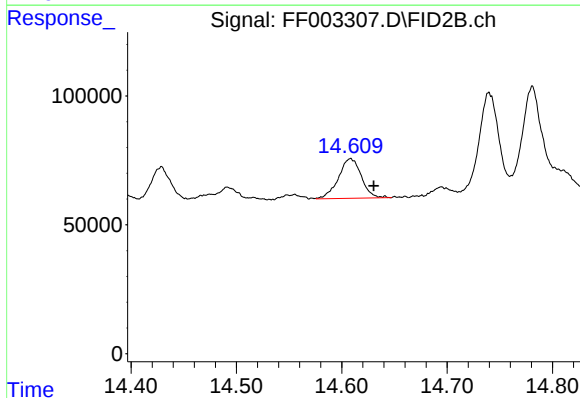


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 232495
Conc: 1.62 ug/ml

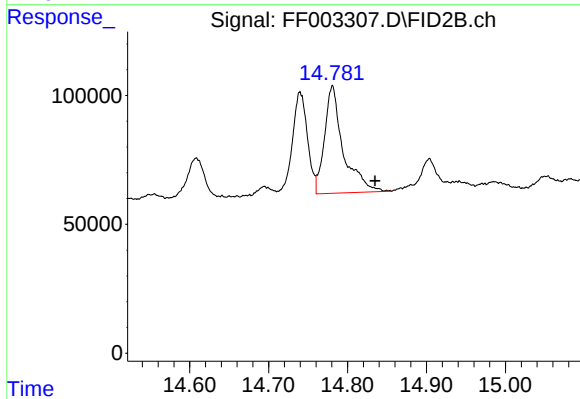

#10 N-TETRACOSANE


R.T.: 14.781 min
Delta R.T.: -0.054 min
Response: 689431
Conc: 4.30 ug/ml

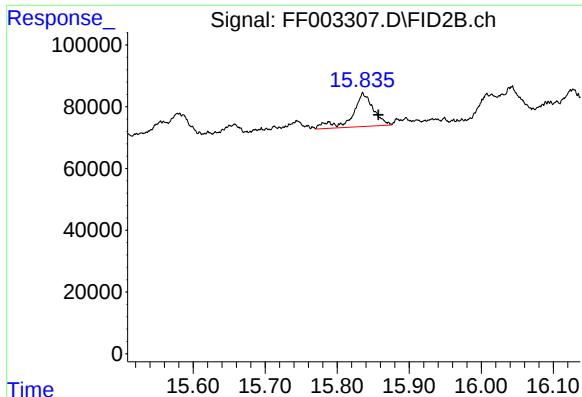

#11 N-HEXACOSANE


R.T.: 15.836 min
Delta R.T.: -0.022 min
Response: 217894
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :

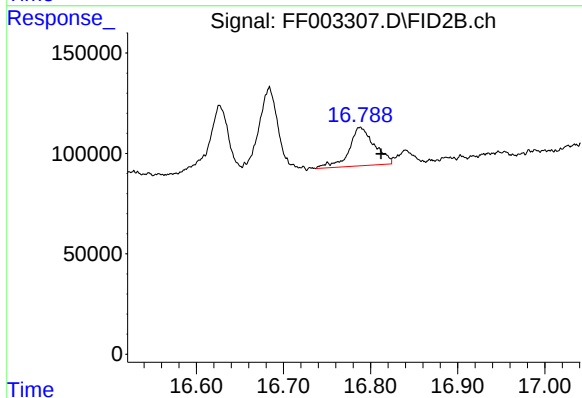


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.024 min
Response: 387381
Conc: 2.46 ug/ml

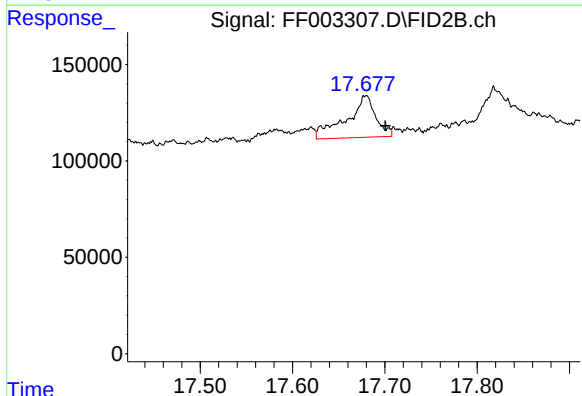


#13 N-TRIACONTANE

R.T.: 17.680 min
Delta R.T.: -0.021 min
Response: 479046
Conc: 3.05 ug/ml

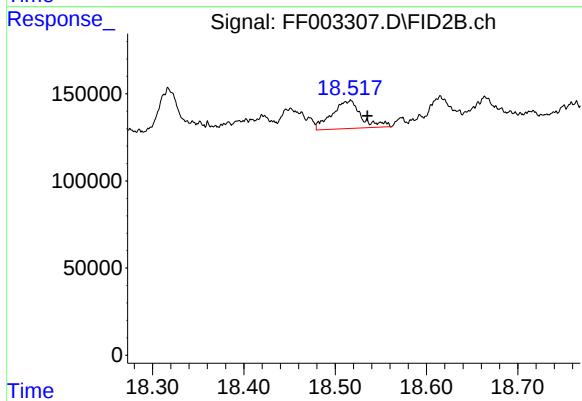

#14 N-DOTRIACONTANE


R.T.: 18.517 min
Delta R.T.: -0.018 min
Response: 355547
Conc: 2.44 ug/ml

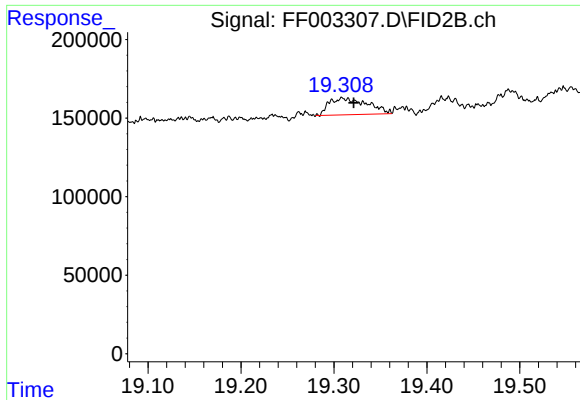

#15 N-TETRATRIACONTANE


R.T.: 19.315 min
Delta R.T.: -0.006 min
Response: 302955
Conc: 2.29 ug/ml

Instrument :
FID_F
ClientSampleId :

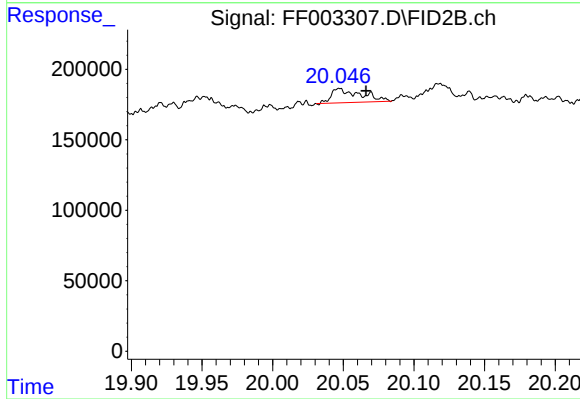

#16 N-HEXATRIACONTANE

R.T.: 20.047 min
Delta R.T.: -0.019 min
Response: 145220
Conc: 1.23 ug/ml

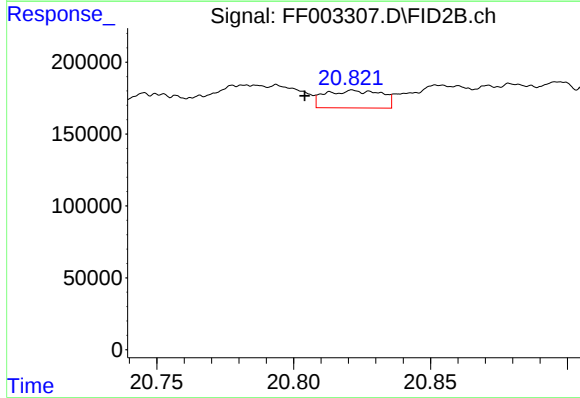

#17 N-OCTATRIACONTANE

R.T.: 20.822 min
Delta R.T.: 0.018 min
Response: 174973
Conc: 1.67 ug/ml