

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003309.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 18:27
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jan 18 20:57:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.611	6305803	44.070 ug/ml
Target Compounds			
2) N-DECANE	4.349	8804777	54.444 ug/ml
3) N-DODECANE	6.367	8602223	53.029 ug/ml
4) N-TETRADECANE	8.159	8349693	51.136 ug/ml
5) N-HEXADECANE	9.757	8097266	49.313 ug/ml
6) N-OCTADECANE	11.200	7874825	47.622 ug/ml
7) N-EICOSANE	12.511	7565564	46.077 ug/ml
8) N-DOCOSANE	13.710	7336242	45.149 ug/ml
10) N-TETRACOSANE	14.816	7199844	44.892 ug/ml
11) N-HEXACOSANE	15.840	7165909	45.305 ug/ml
12) N-OCTACOSANE	16.793	7363044	46.747 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003309.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 18:27
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jan 18 20:57:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

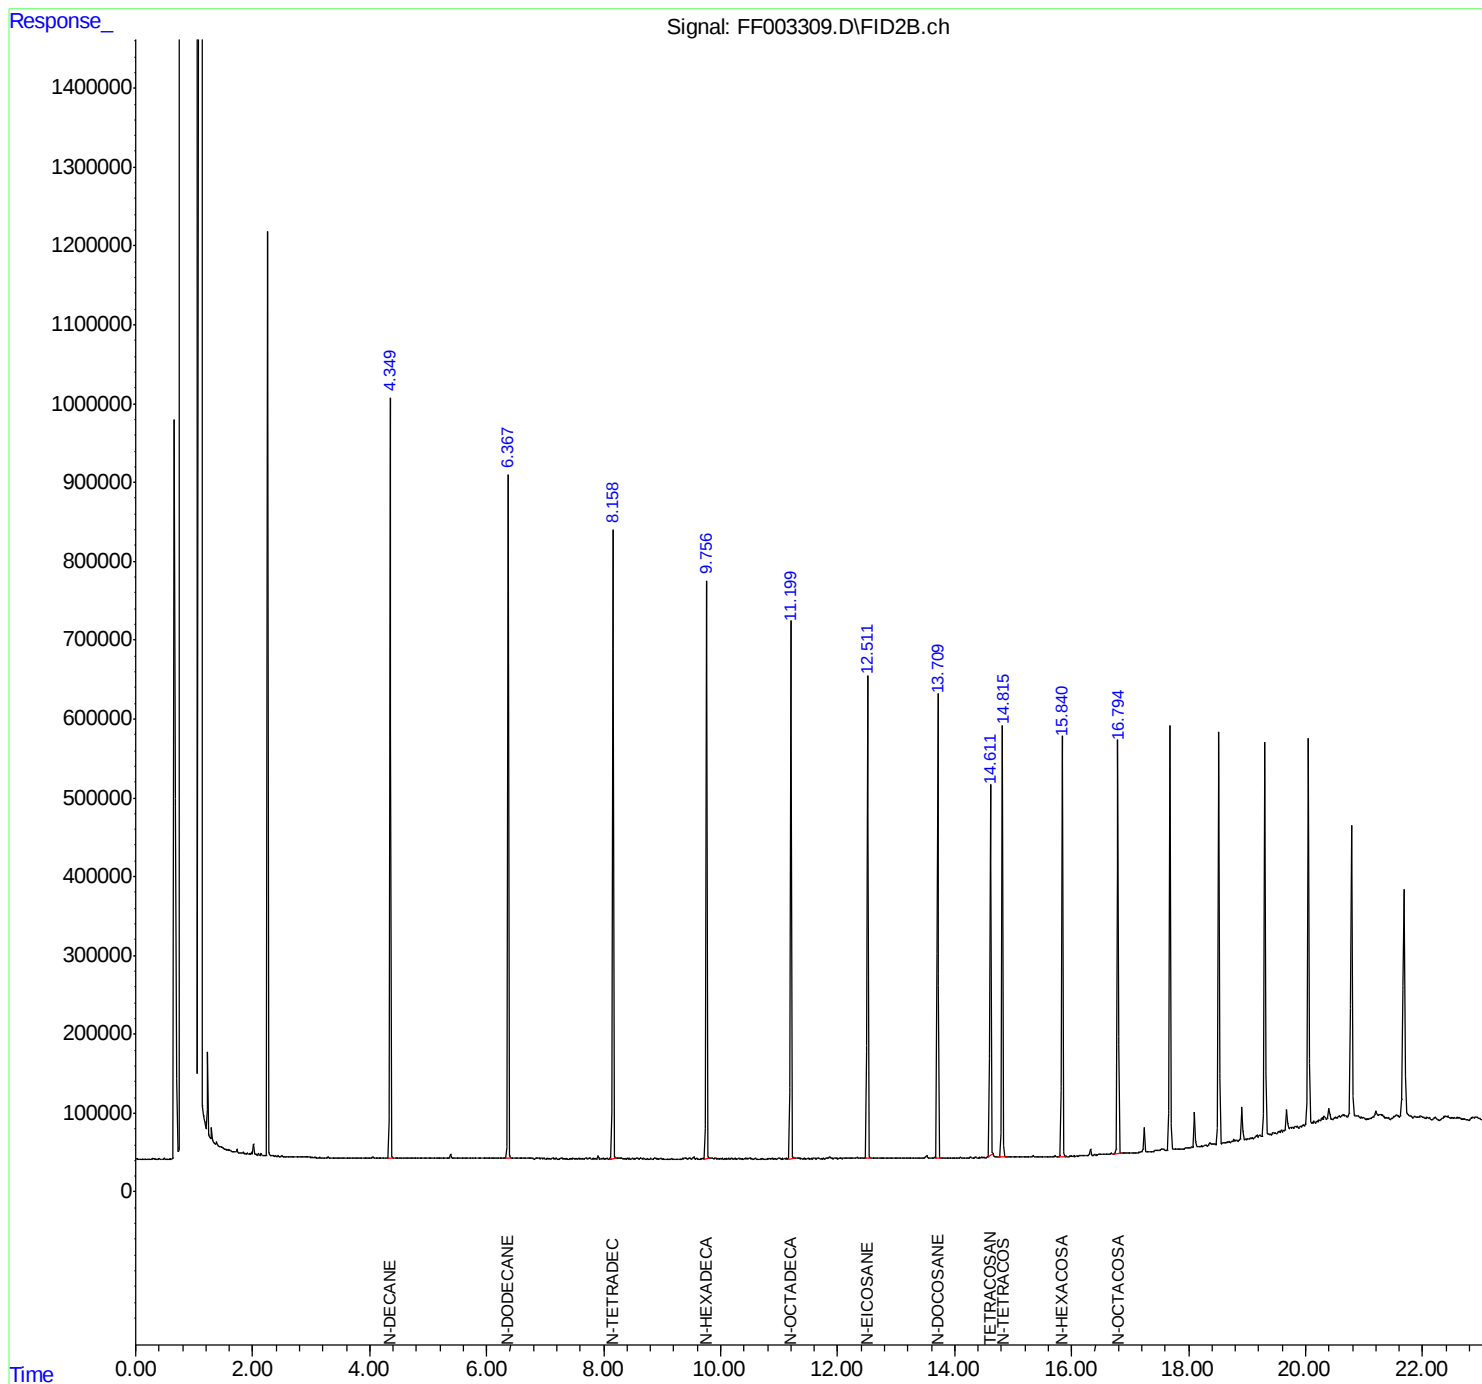


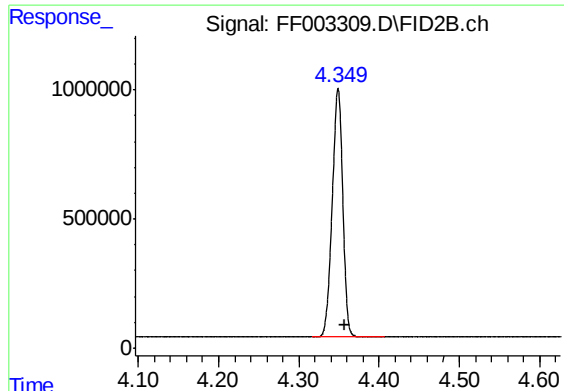

#2 N-DECANE


R.T.: 4.349 min
Delta R.T.: -0.009 min
Response: 8804777
Conc: 54.44 ug/ml

Instrument :
FID_F
ClientSampleId :

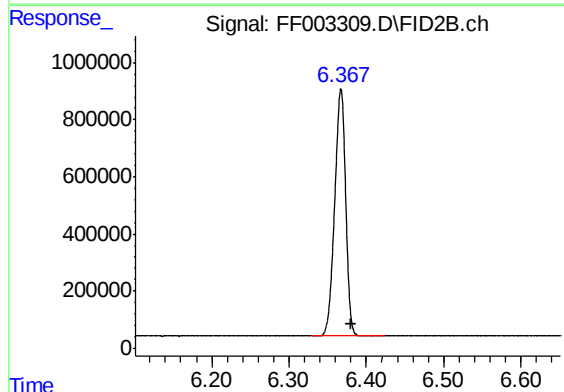


#3 N-DODECANE

R.T.: 6.367 min
Delta R.T.: -0.013 min
Response: 8602223
Conc: 53.03 ug/ml

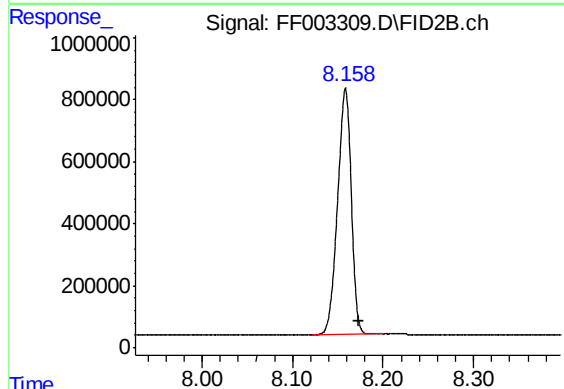


#4 N-TETRADECANE

R.T.: 8.159 min
Delta R.T.: -0.015 min
Response: 8349693
Conc: 51.14 ug/ml

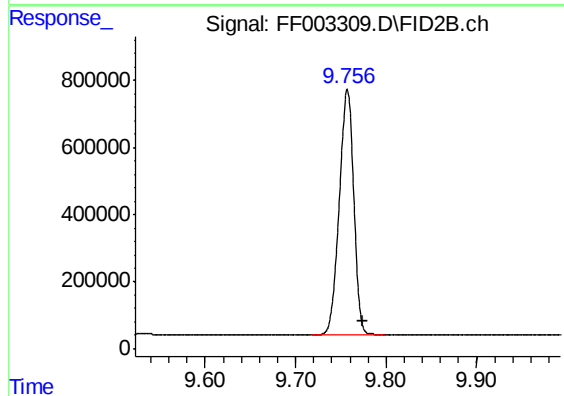

#5 N-HEXADECANE


R.T.: 9.757 min
Delta R.T.: -0.016 min
Response: 8097266
Conc: 49.31 ug/ml

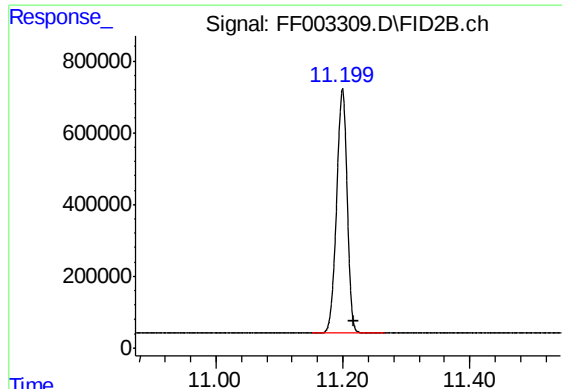

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.017 min
Response: 7874825
Conc: 47.62 ug/ml

Instrument :
FID_F
ClientSampleId :

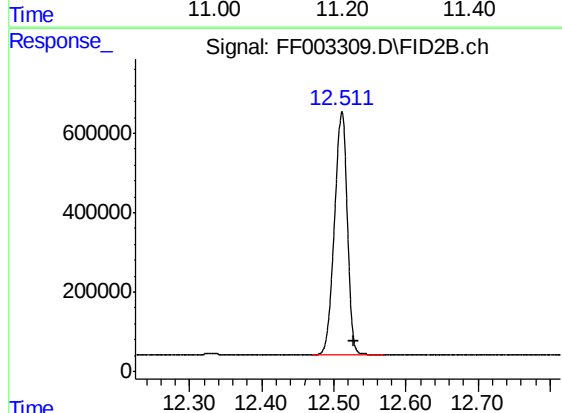


#7 N-EICOSANE

R.T.: 12.511 min
Delta R.T.: -0.017 min
Response: 7565564
Conc: 46.08 ug/ml

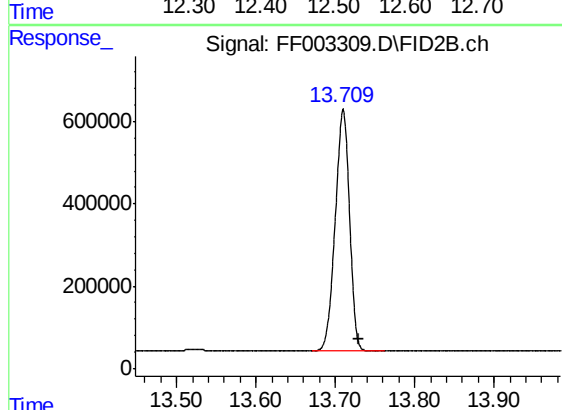


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 7336242
Conc: 45.15 ug/ml

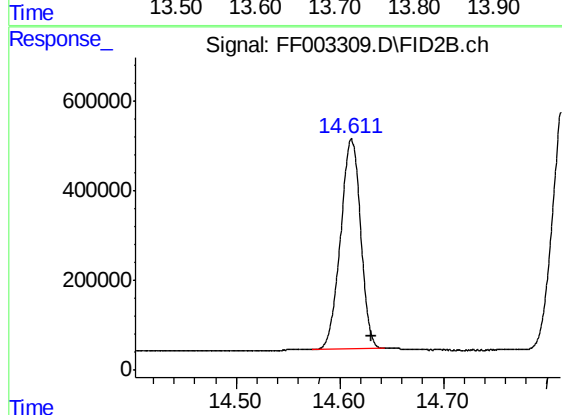

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.611 min
Delta R.T.: -0.019 min
Response: 6305803
Conc: 44.07 ug/ml

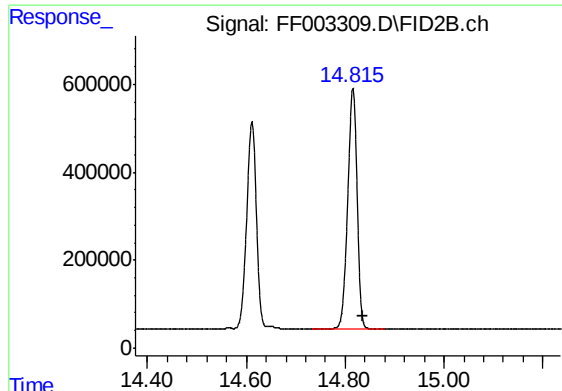

#10 N-TETRACOSANE


R.T.: 14.816 min
Delta R.T.: -0.019 min
Response: 7199844
Conc: 44.89 ug/ml

Instrument :
FID_F
ClientSampleId :

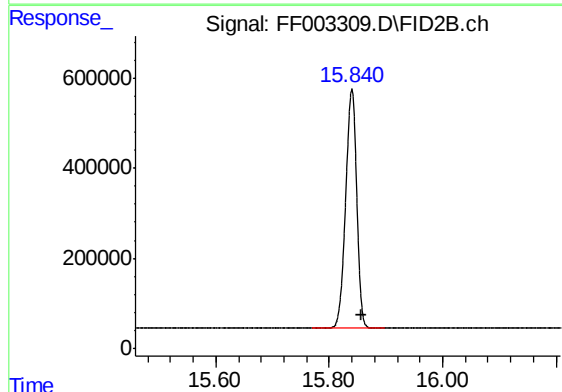

#11 N-HEXACOSANE

R.T.: 15.840 min
Delta R.T.: -0.017 min
Response: 7165909
Conc: 45.31 ug/ml

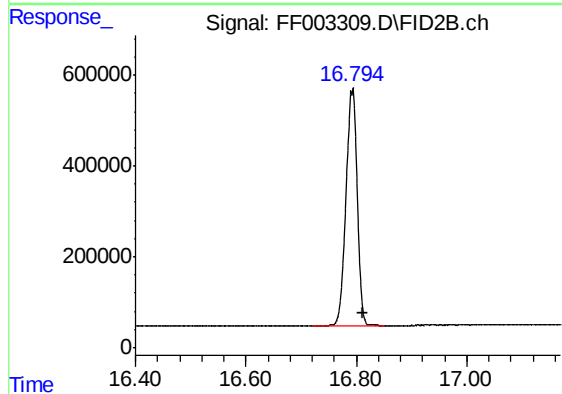

#12 N-OCTACOSANE

R.T.: 16.793 min
Delta R.T.: -0.019 min
Response: 7363044
Conc: 46.75 ug/ml