

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011822\
 Data File : FF009685.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2022 11:05
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 00:15:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.242	3570142	24.949 ug/ml
12)	N-OCTACOSANE	16.614	3464239	23.864 ug/ml
13)	N-TRIACONTANE	17.498	67774	0.474 ug/ml
14)	N-DOTRIACONTANE	18.344	158855	1.167 ug/ml
15)	N-TETRATRIACONTANE	19.105	68247	0.575 ug/ml
16)	N-HEXATRIACONTANE	19.892	200121	1.941 ug/ml
18)	N-TETRACONTANE	21.406	204397	2.250 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011822\
Data File : FF009685.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2022 11:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 00:15:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

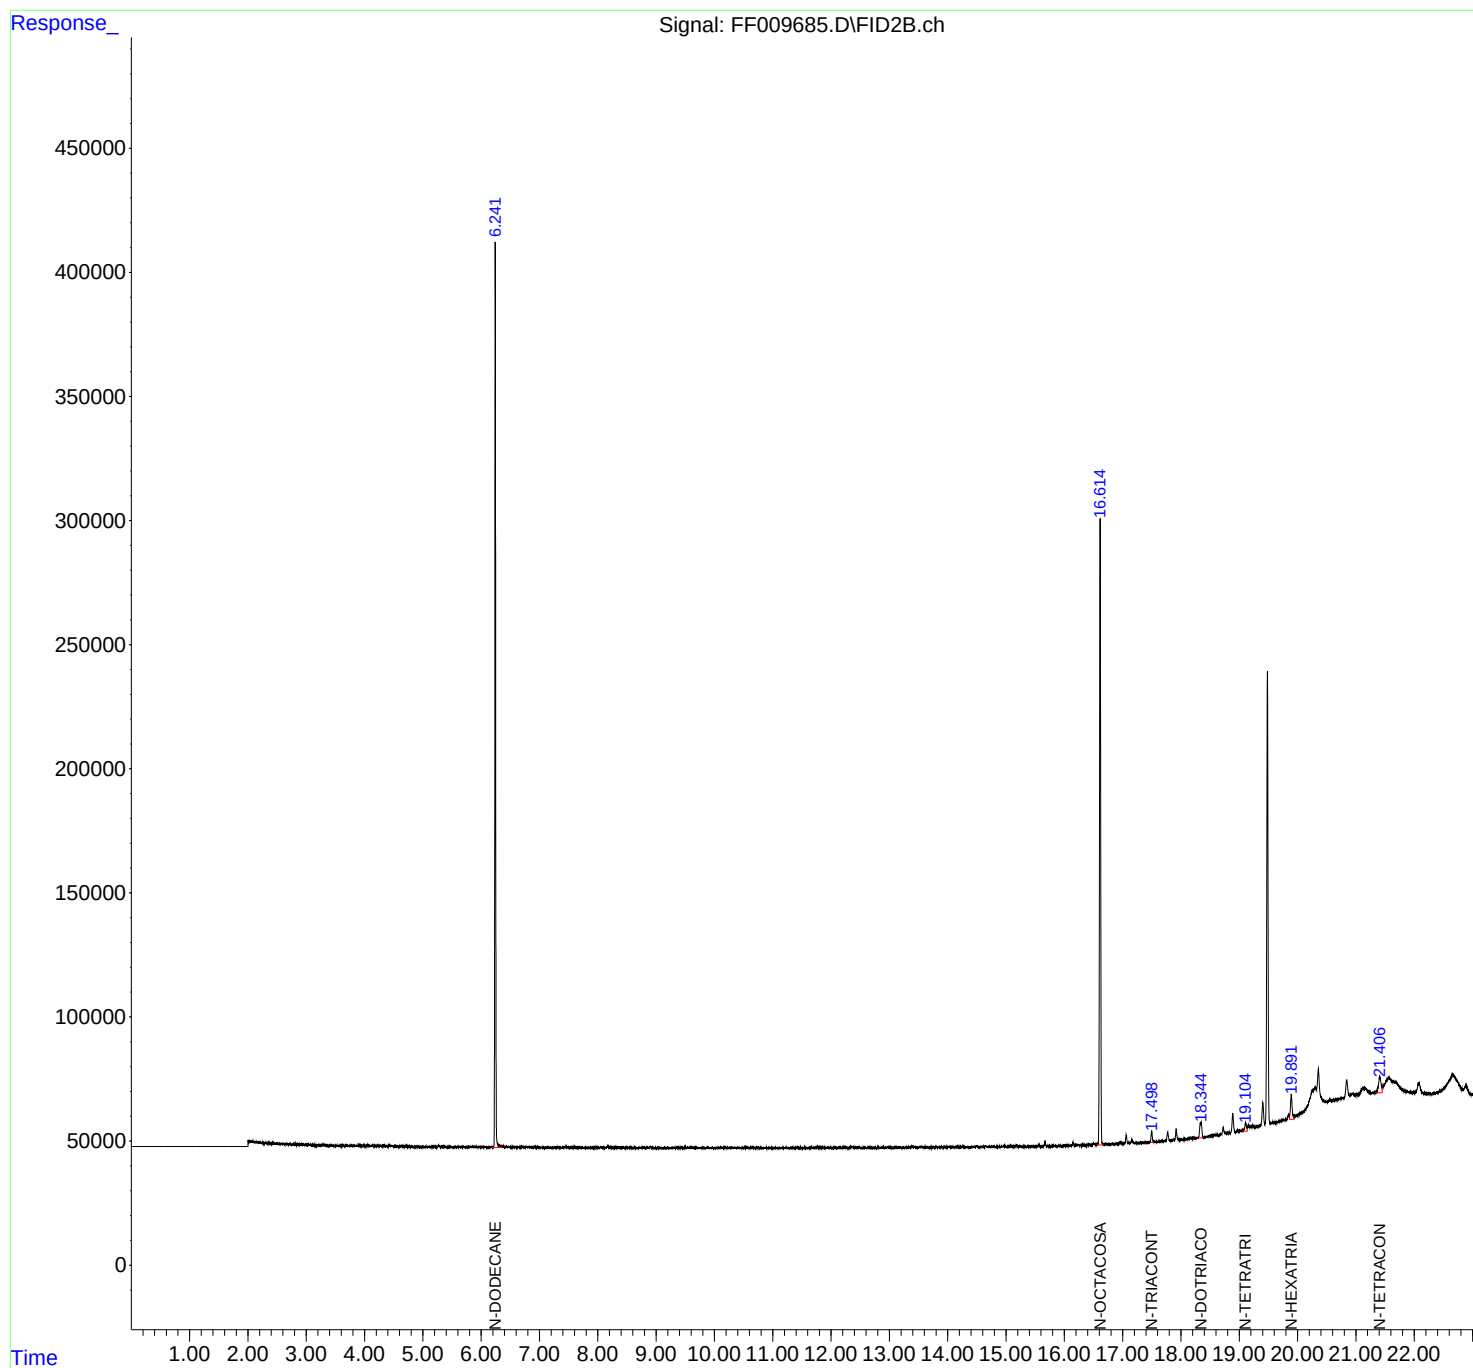


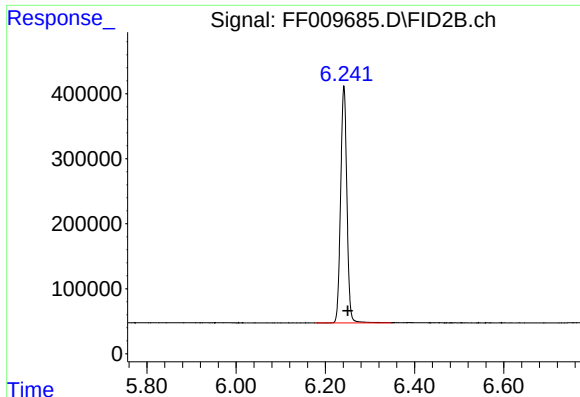

#3 N-DODECANE


R.T.: 6.242 min
Delta R.T.: -0.008 min
Response: 3570142
Conc: 24.95 ug/ml

Instrument :
FID_F
ClientSampleId :

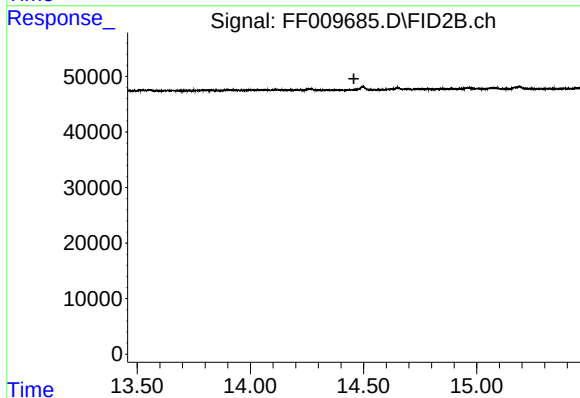


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

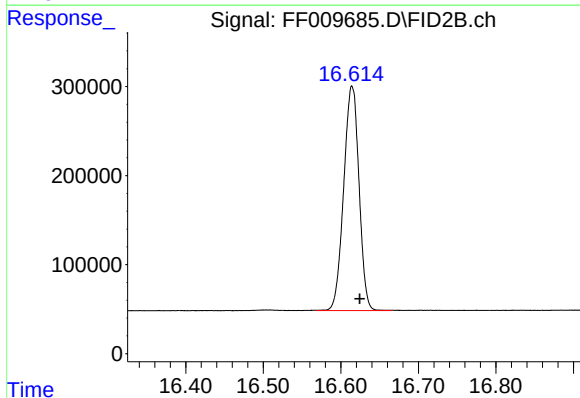


#12 N-OCTACOSANE

R.T.: 16.614 min
Delta R.T.: -0.010 min
Response: 3464239
Conc: 23.86 ug/ml

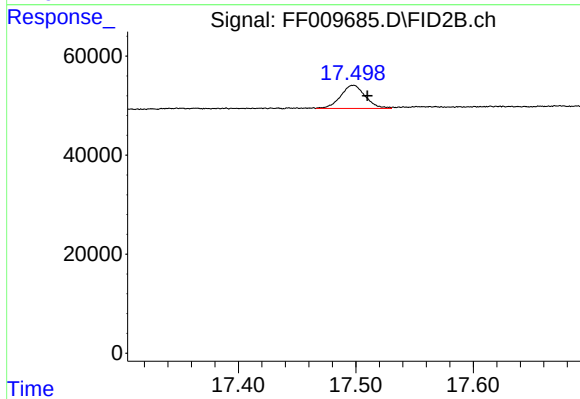

#13 N-TRIACONTANE


R.T.: 17.498 min
Delta R.T.: -0.012 min
Response: 67774
Conc: 0.47 ug/ml

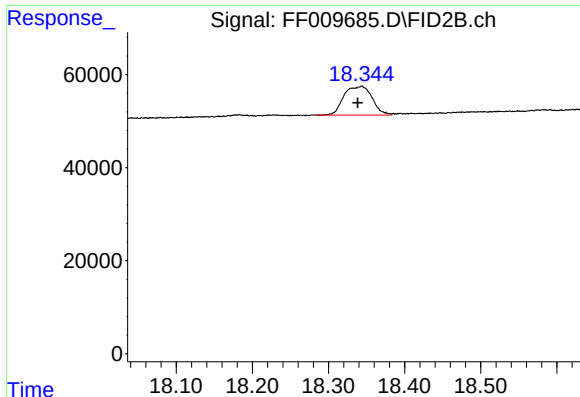

#14 N-DOTRIACONTANE


R.T.: 18.344 min
Delta R.T.: 0.006 min
Response: 158855
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :

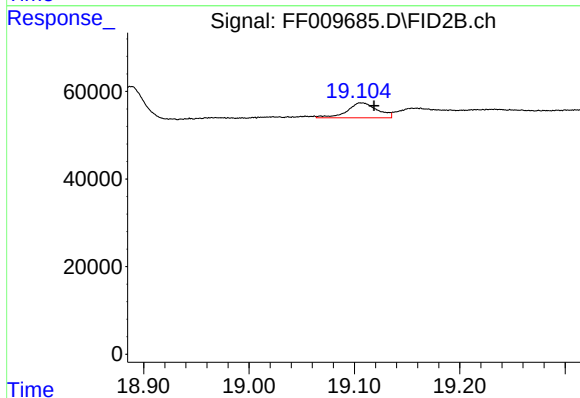


#15 N-TETRATRIACONTANE

R.T.: 19.105 min
Delta R.T.: -0.014 min
Response: 68247
Conc: 0.57 ug/ml

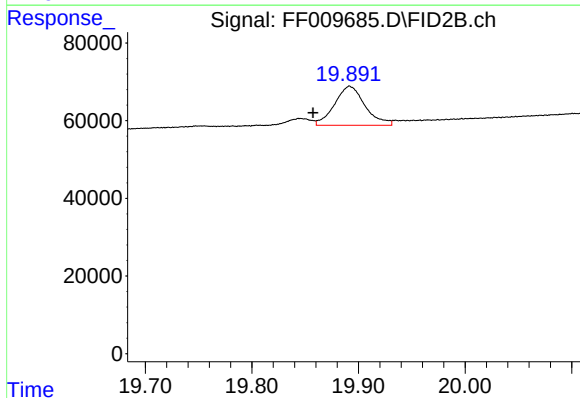

#16 N-HEXATRIACONTANE

R.T.: 19.892 min
Delta R.T.: 0.034 min
Response: 200121
Conc: 1.94 ug/ml

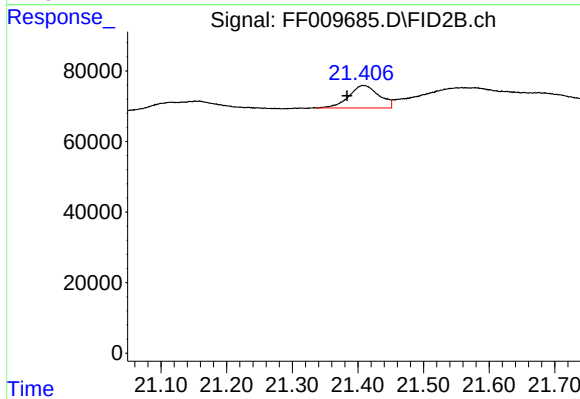

#18 N-TETRACONTANE

R.T.: 21.406 min
Delta R.T.: 0.023 min
Response: 204397
Conc: 2.25 ug/ml