

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011822\
 Data File : FF009695.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2022 16:16
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 00:18:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.244	3582601	25.036 ug/ml
12) N-OCTACOSANE	16.615	3573139	24.614 ug/ml
13) N-TRIACONTANE	17.500	69277	0.484 ug/ml
14) N-DOTRIACONTANE	18.328	100111	0.736 ug/ml
15) N-TETRATRIACONTANE	19.107	59738	0.503 ug/ml
16) N-HEXATRIACONTANE	19.892	80123	0.777 ug/ml
18) N-TETRACONTANE	21.406	106918	1.177 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011822\
Data File : FF009695.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2022 16:16
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 00:18:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

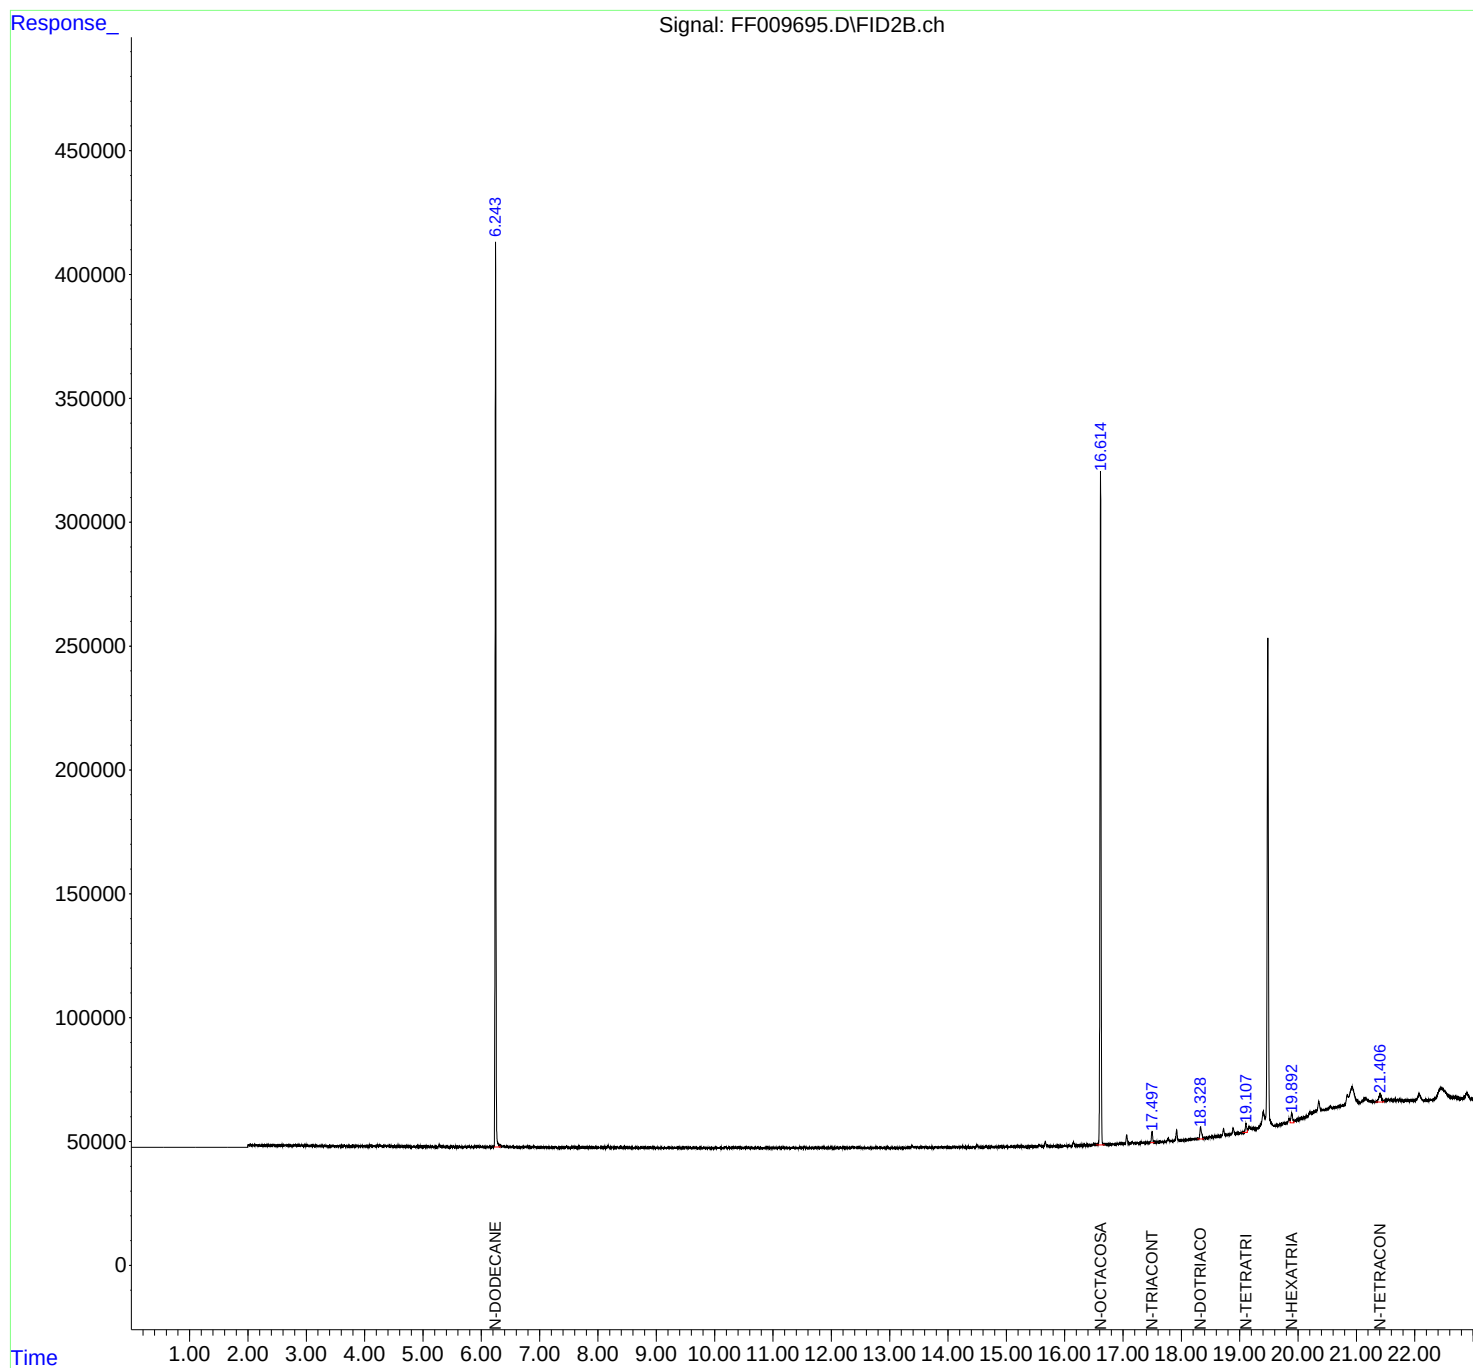


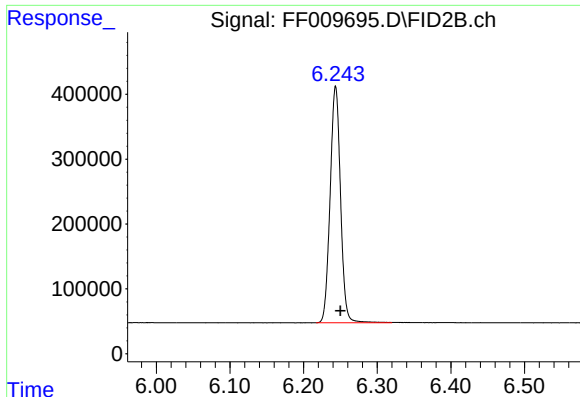

#3 N-DODECANE


R.T.: 6.244 min
Delta R.T.: -0.006 min
Response: 3582601
Conc: 25.04 ug/ml

Instrument :
FID_F
ClientSampleId :

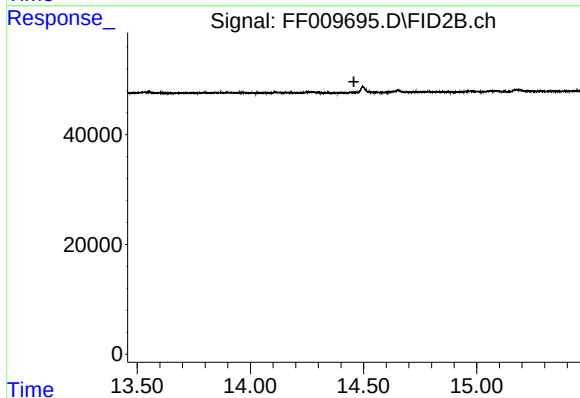


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

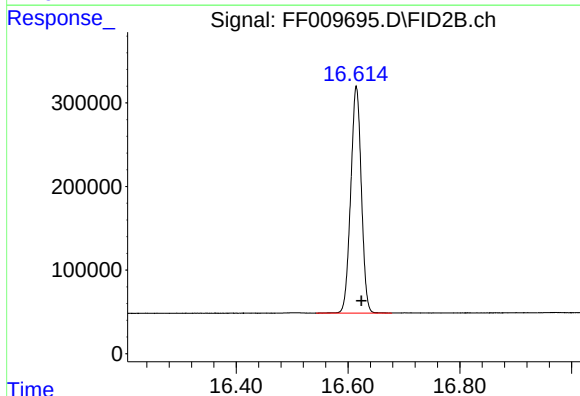


#12 N-OCTACOSANE

R.T.: 16.615 min
Delta R.T.: -0.010 min
Response: 3573139
Conc: 24.61 ug/ml

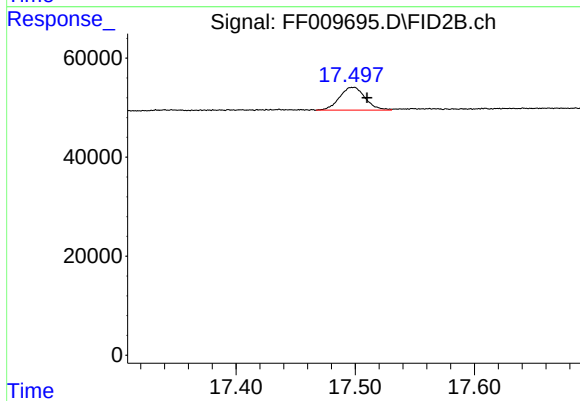

#13 N-TRIACONTANE


R.T.: 17.500 min
Delta R.T.: -0.010 min
Response: 69277
Conc: 0.48 ug/ml

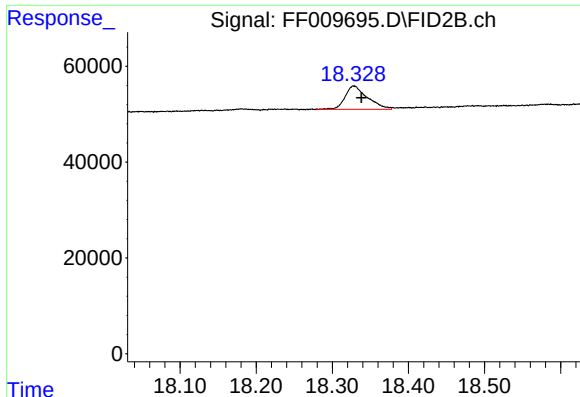

#14 N-DOTRIACONTANE


R.T.: 18.328 min
Delta R.T.: -0.011 min
Response: 100111
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

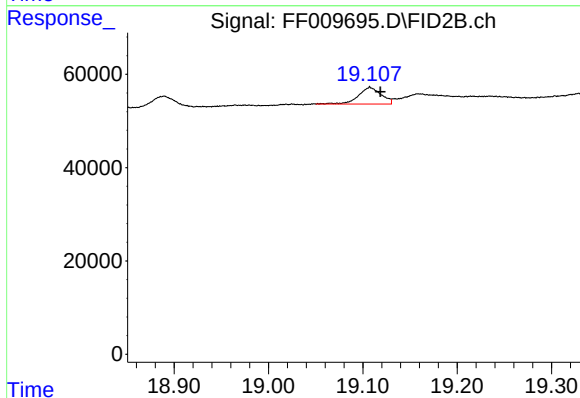


#15 N-TETRATRIACONTANE

R.T.: 19.107 min
Delta R.T.: -0.011 min
Response: 59738
Conc: 0.50 ug/ml

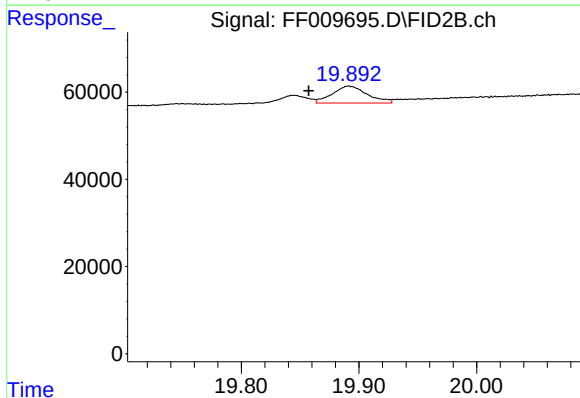

#16 N-HEXATRIACONTANE

R.T.: 19.892 min
Delta R.T.: 0.034 min
Response: 80123
Conc: 0.78 ug/ml

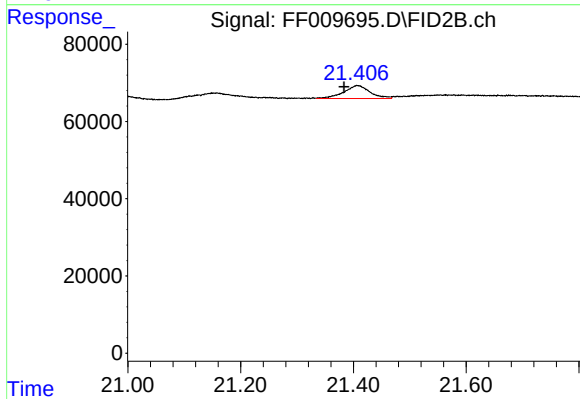

#18 N-TETRACONTANE

R.T.: 21.406 min
Delta R.T.: 0.023 min
Response: 106918
Conc: 1.18 ug/ml