

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011922\
Data File : FF009701.D
Signal(s) : FID2B.ch
Acq On : 19 Jan 2022 08:55
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 00:15:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.311f	50883	0.337 ug/ml
10)	N-TETRACOSANE	14.649	77319	0.521 ug/ml
11)	N-HEXACOSANE	15.662	94933	0.649 ug/ml
12)	N-OCTACOSANE	16.609	320454	2.208 ug/ml
13)	N-TRIACONTANE	17.493	359295	2.511 ug/ml
14)	N-DOTRIACONTANE	18.341	458869	3.372 ug/ml
15)	N-TETRATRIACONTANE	19.103	116496	0.981 ug/ml
16)	N-HEXATRIACONTANE	19.887	645742	6.263 ug/ml
18)	N-TETRACONTANE	21.406	588463	6.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011922\
Data File : FF009701.D
Signal(s) : FID2B.ch
Acq On : 19 Jan 2022 08:55
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 00:15:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

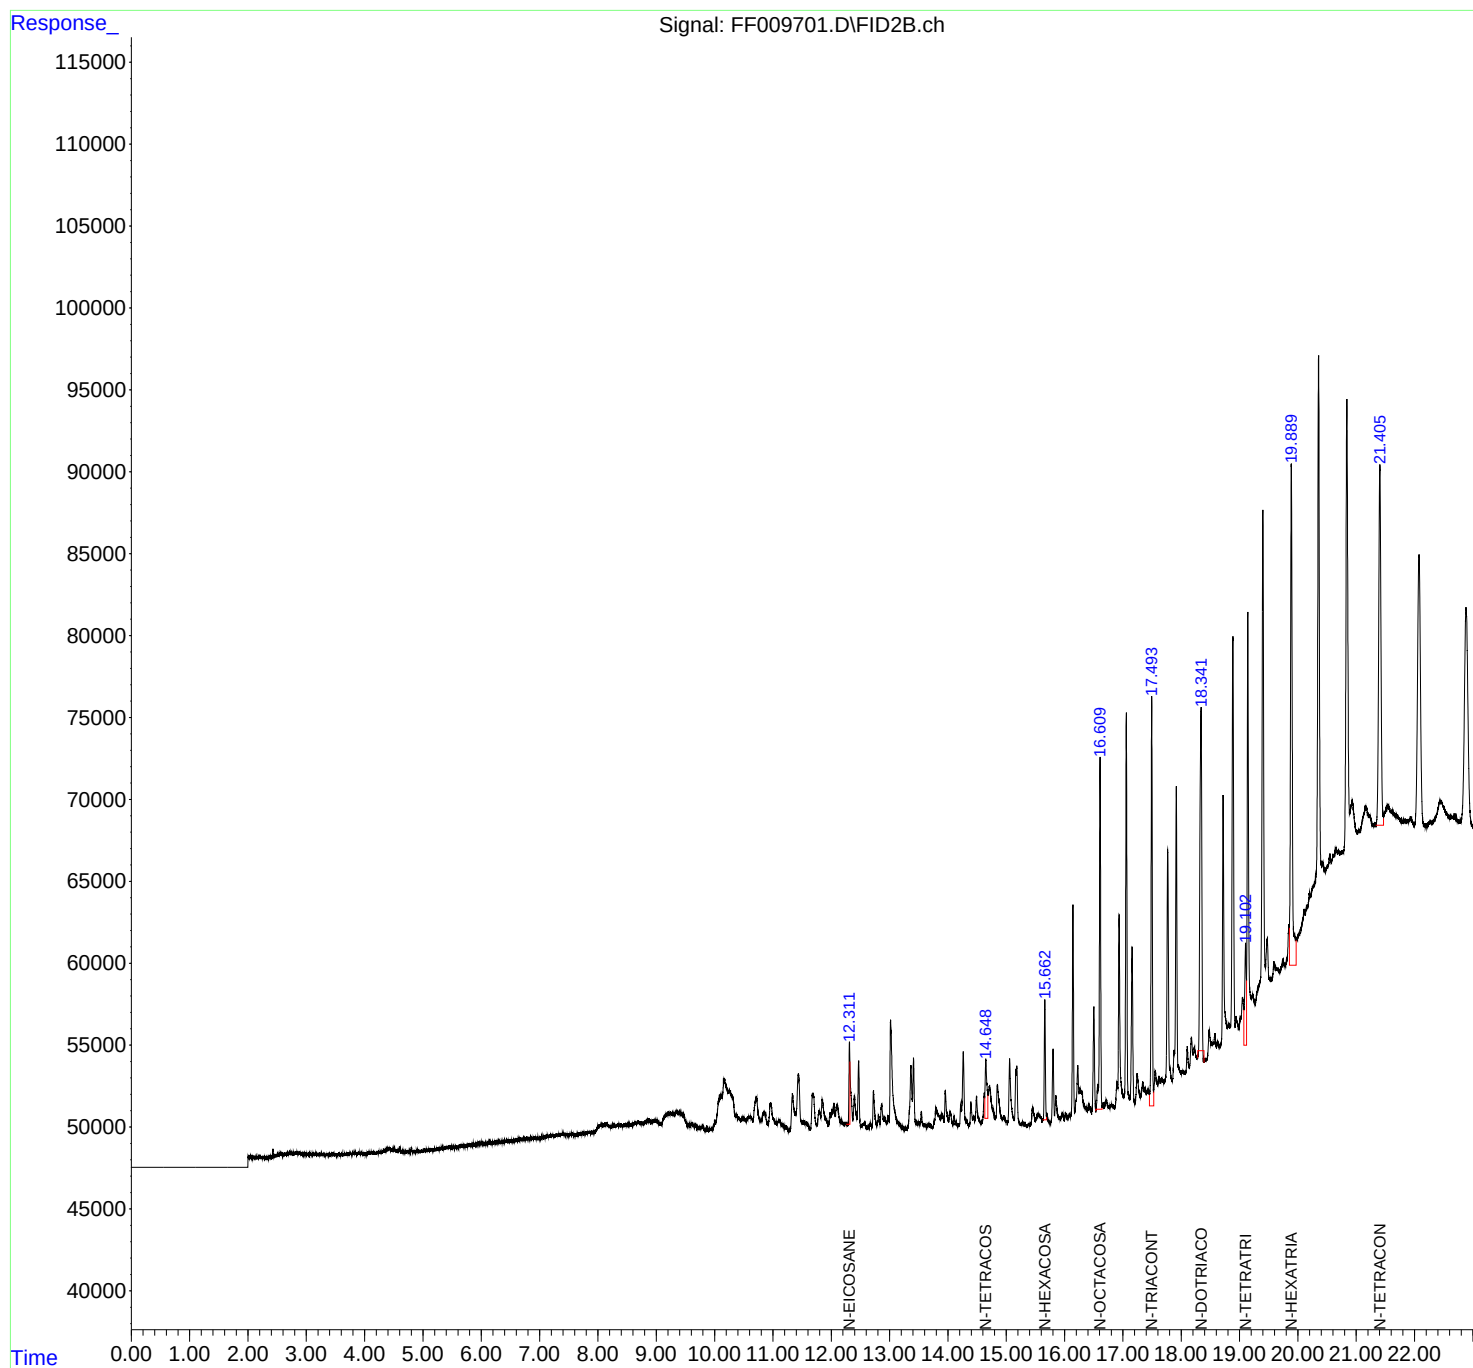


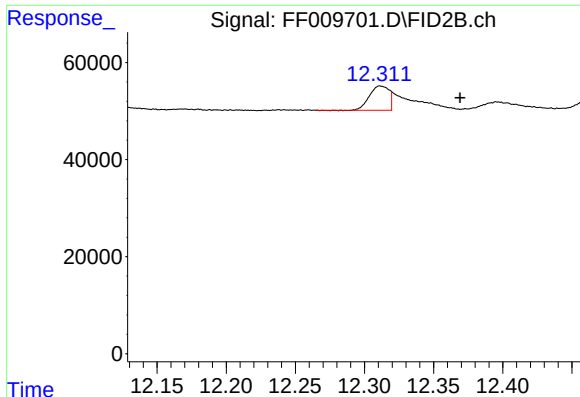

#7 N-EICOSANE


R.T.: 12.311 min
Delta R.T.: -0.058 min
Response: 50883
Conc: 0.34 ug/ml

Instrument :
FID_F
ClientSampleId :

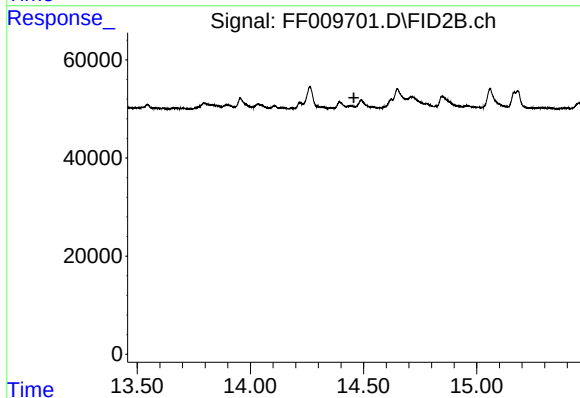


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

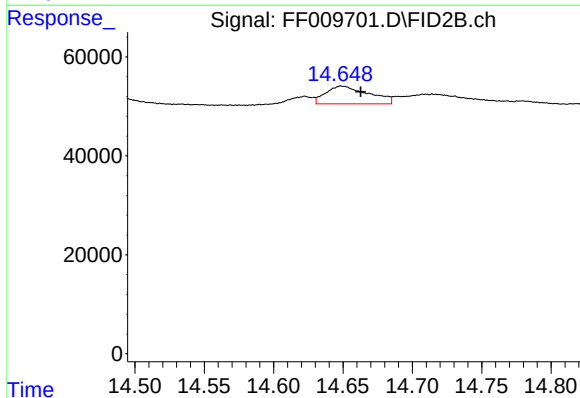


#10 N-TETRACOSANE

R.T.: 14.649 min
Delta R.T.: -0.014 min
Response: 77319
Conc: 0.52 ug/ml

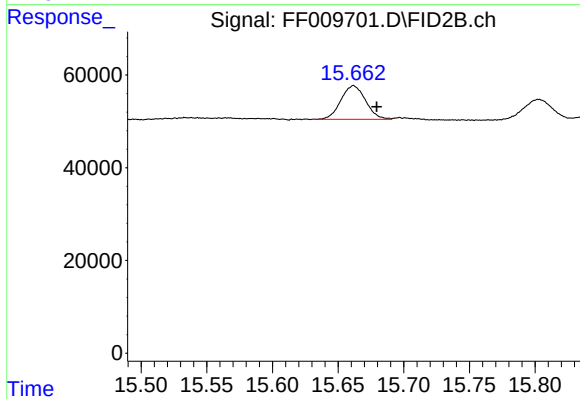

#11 N-HEXACOSANE


R.T.: 15.662 min
Delta R.T.: -0.018 min
Response: 94933
Conc: 0.65 ug/ml

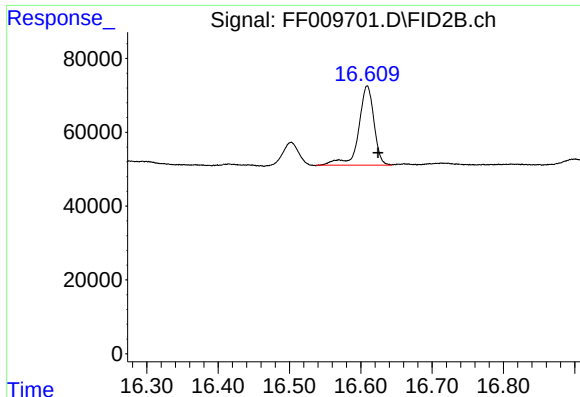

#12 N-OCTACOSANE


R.T.: 16.609 min
Delta R.T.: -0.015 min
Response: 320454
Conc: 2.21 ug/ml

Instrument :
FID_F
ClientSampleId :

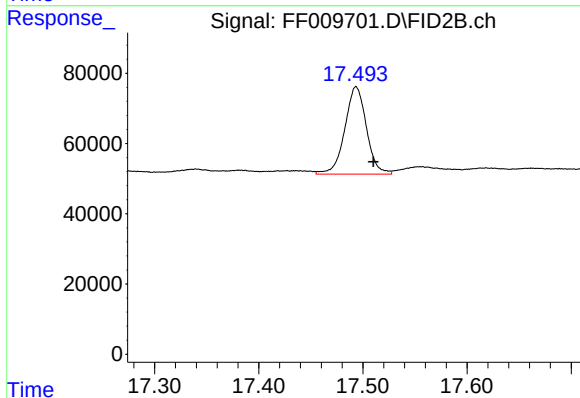


#13 N-TRIACONTANE

R.T.: 17.493 min
Delta R.T.: -0.016 min
Response: 359295
Conc: 2.51 ug/ml

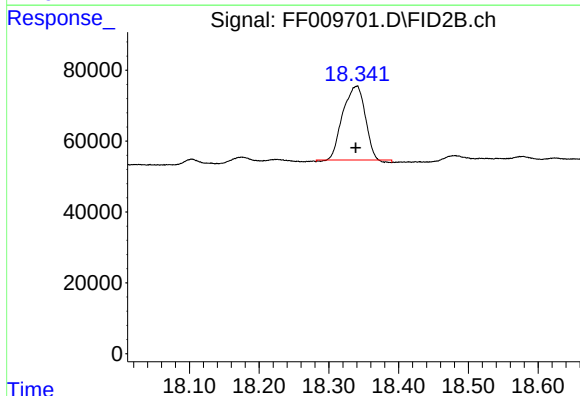


#14 N-DOTRIACONTANE

R.T.: 18.341 min
Delta R.T.: 0.003 min
Response: 458869
Conc: 3.37 ug/ml

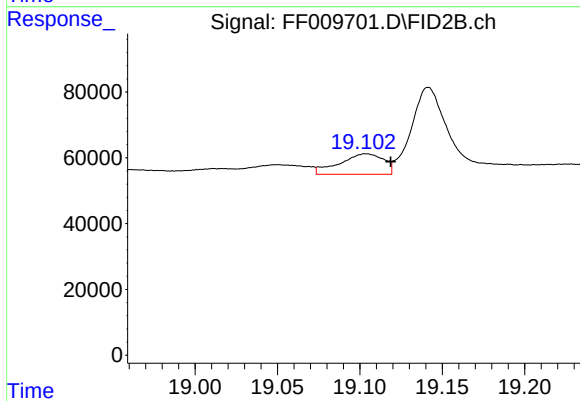

#15 N-TETRATRIACONTANE


R.T.: 19.103 min
Delta R.T.: -0.016 min
Response: 116496
Conc: 0.98 ug/ml

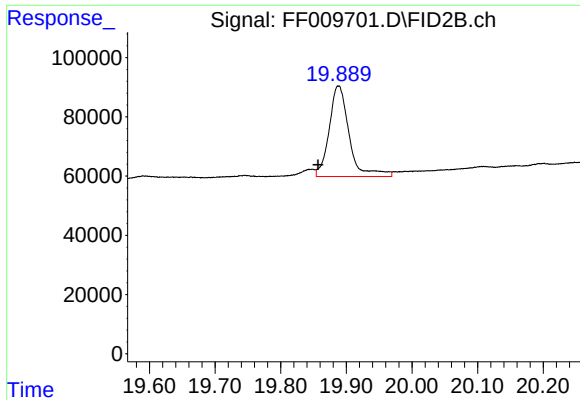

#16 N-HEXATRIACONTANE

R.T.: 19.887 min
Delta R.T.: 0.030 min
Response: 645742
Conc: 6.26 ug/ml

Instrument :
FID_F
ClientSampleId :

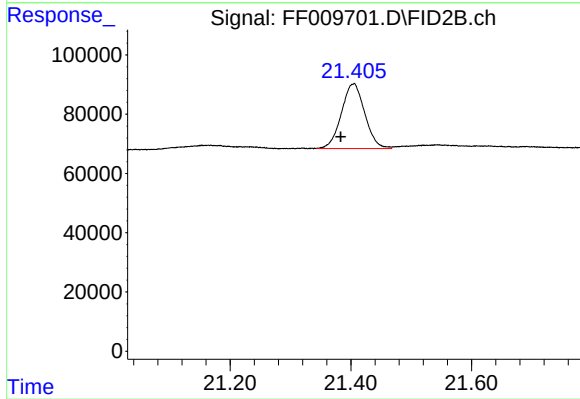

#18 N-TETRACONTANE

R.T.: 21.406 min
Delta R.T.: 0.023 min
Response: 588463
Conc: 6.48 ug/ml