

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011922\
Data File : FF009704.D
Signal(s) : FID2B.ch
Acq On : 19 Jan 2022 13:04
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 00:16:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.243	3494332	24.419 ug/ml
12)	N-OCTACOSANE	16.614	3323438	22.894 ug/ml
13)	N-TRIACONTANE	17.496	48093	0.336 ug/ml
14)	N-DOTRIACONTANE	18.328	93966	0.691 ug/ml
16)	N-HEXATRIACONTANE	19.891	102066	0.990 ug/ml
18)	N-TETRACONTANE	21.407	107171	1.180 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011922\
Data File : FF009704.D
Signal(s) : FID2B.ch
Acq On : 19 Jan 2022 13:04
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 00:16:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

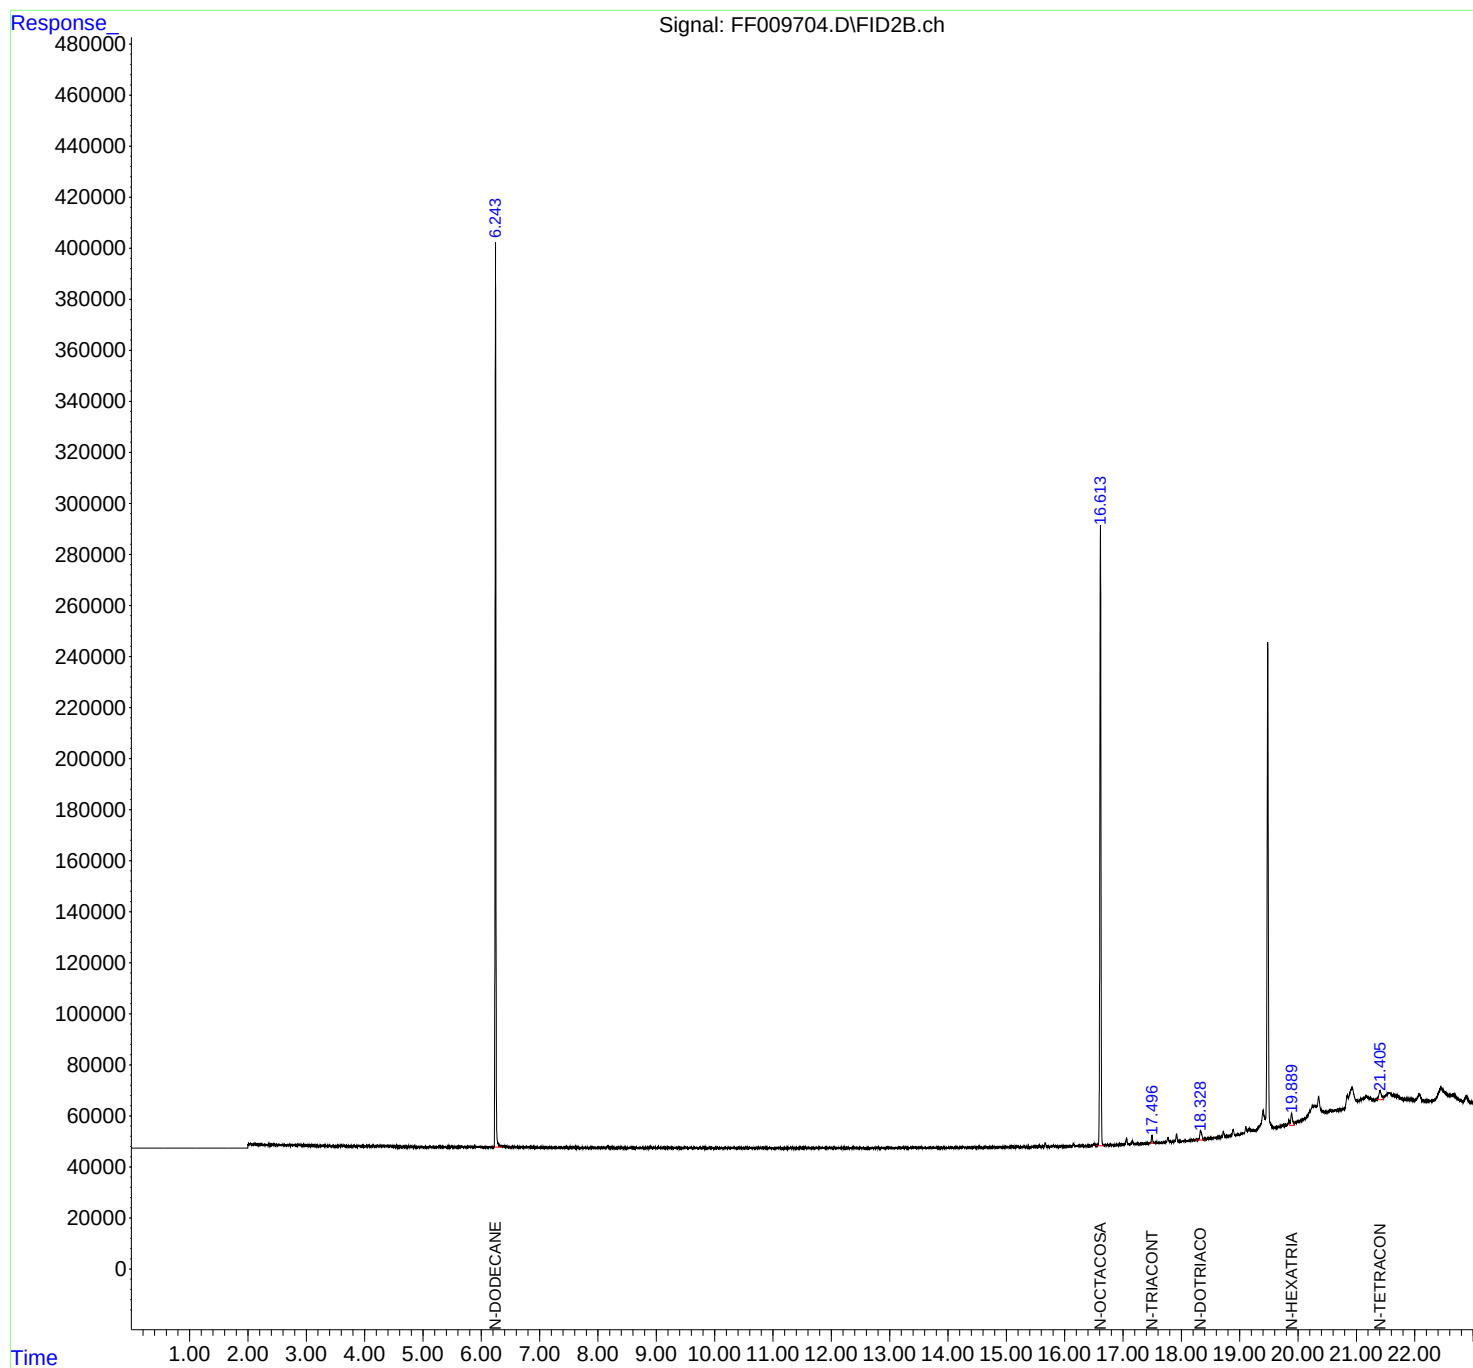


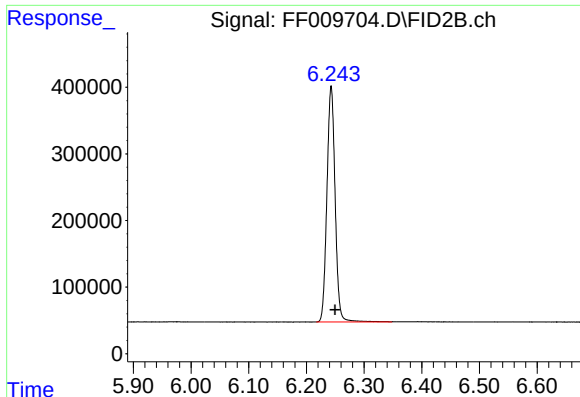

#3 N-DODECANE


R.T.: 6.243 min
Delta R.T.: -0.007 min
Response: 3494332
Conc: 24.42 ug/ml

Instrument :
FID_F
ClientSampleId :

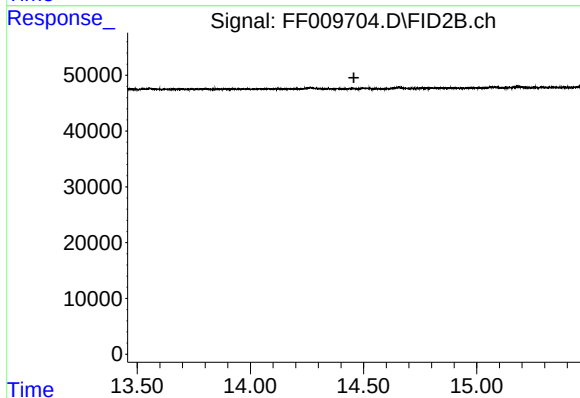


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

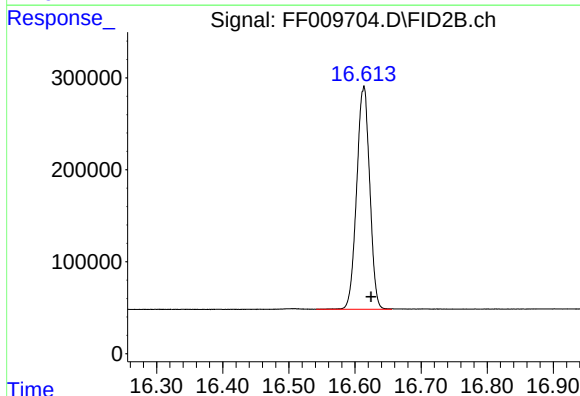


#12 N-OCTACOSANE

R.T.: 16.614 min
Delta R.T.: -0.011 min
Response: 3323438
Conc: 22.89 ug/ml

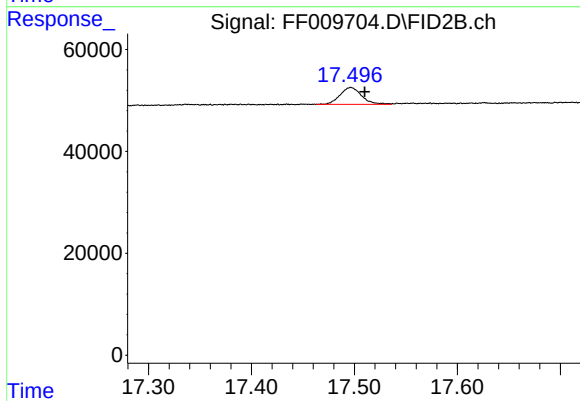

#13 N-TRIACONTANE


R.T.: 17.496 min
Delta R.T.: -0.013 min
Response: 48093
Conc: 0.34 ug/ml

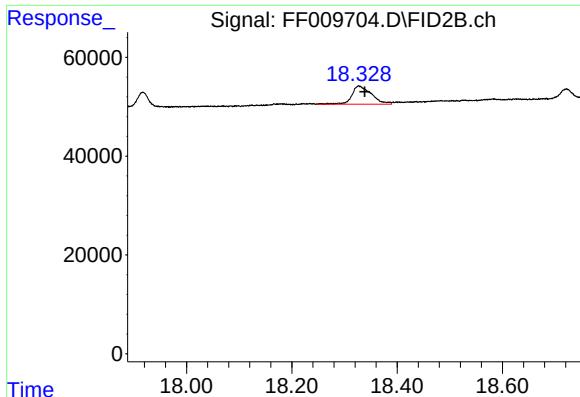

#14 N-DOTRIACONTANE


R.T.: 18.328 min
Delta R.T.: -0.011 min
Response: 93966
Conc: 0.69 ug/ml

Instrument :
FID_F
ClientSampleId :

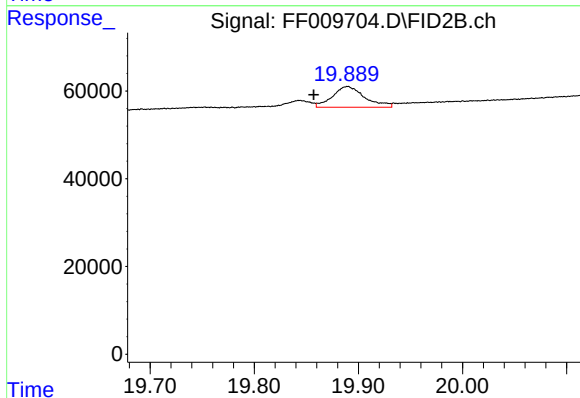

#16 N-HEXATRIACONTANE

R.T.: 19.891 min
Delta R.T.: 0.034 min
Response: 102066
Conc: 0.99 ug/ml

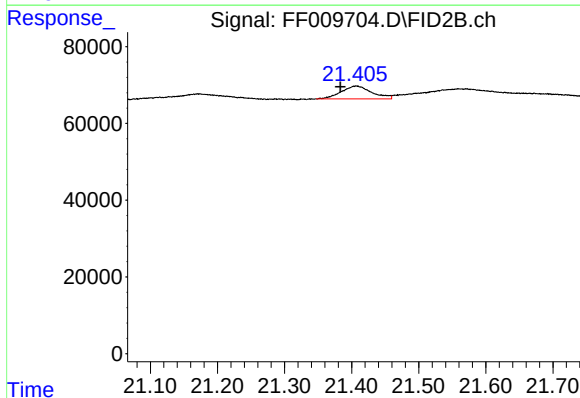

#18 N-TETRACONTANE

R.T.: 21.407 min
Delta R.T.: 0.023 min
Response: 107171
Conc: 1.18 ug/ml