

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006234.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 08:53
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:29:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.516	248460	2.150 ug/ml
15)	N-TETRATRIACONTANE	19.300	76741	0.681 ug/ml
16)	N-HEXATRIACONTANE	20.053	611755	5.721 ug/ml
17)	N-OCTATRIACONTANE	20.715	220129	2.379 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006234.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 08:53
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:29:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

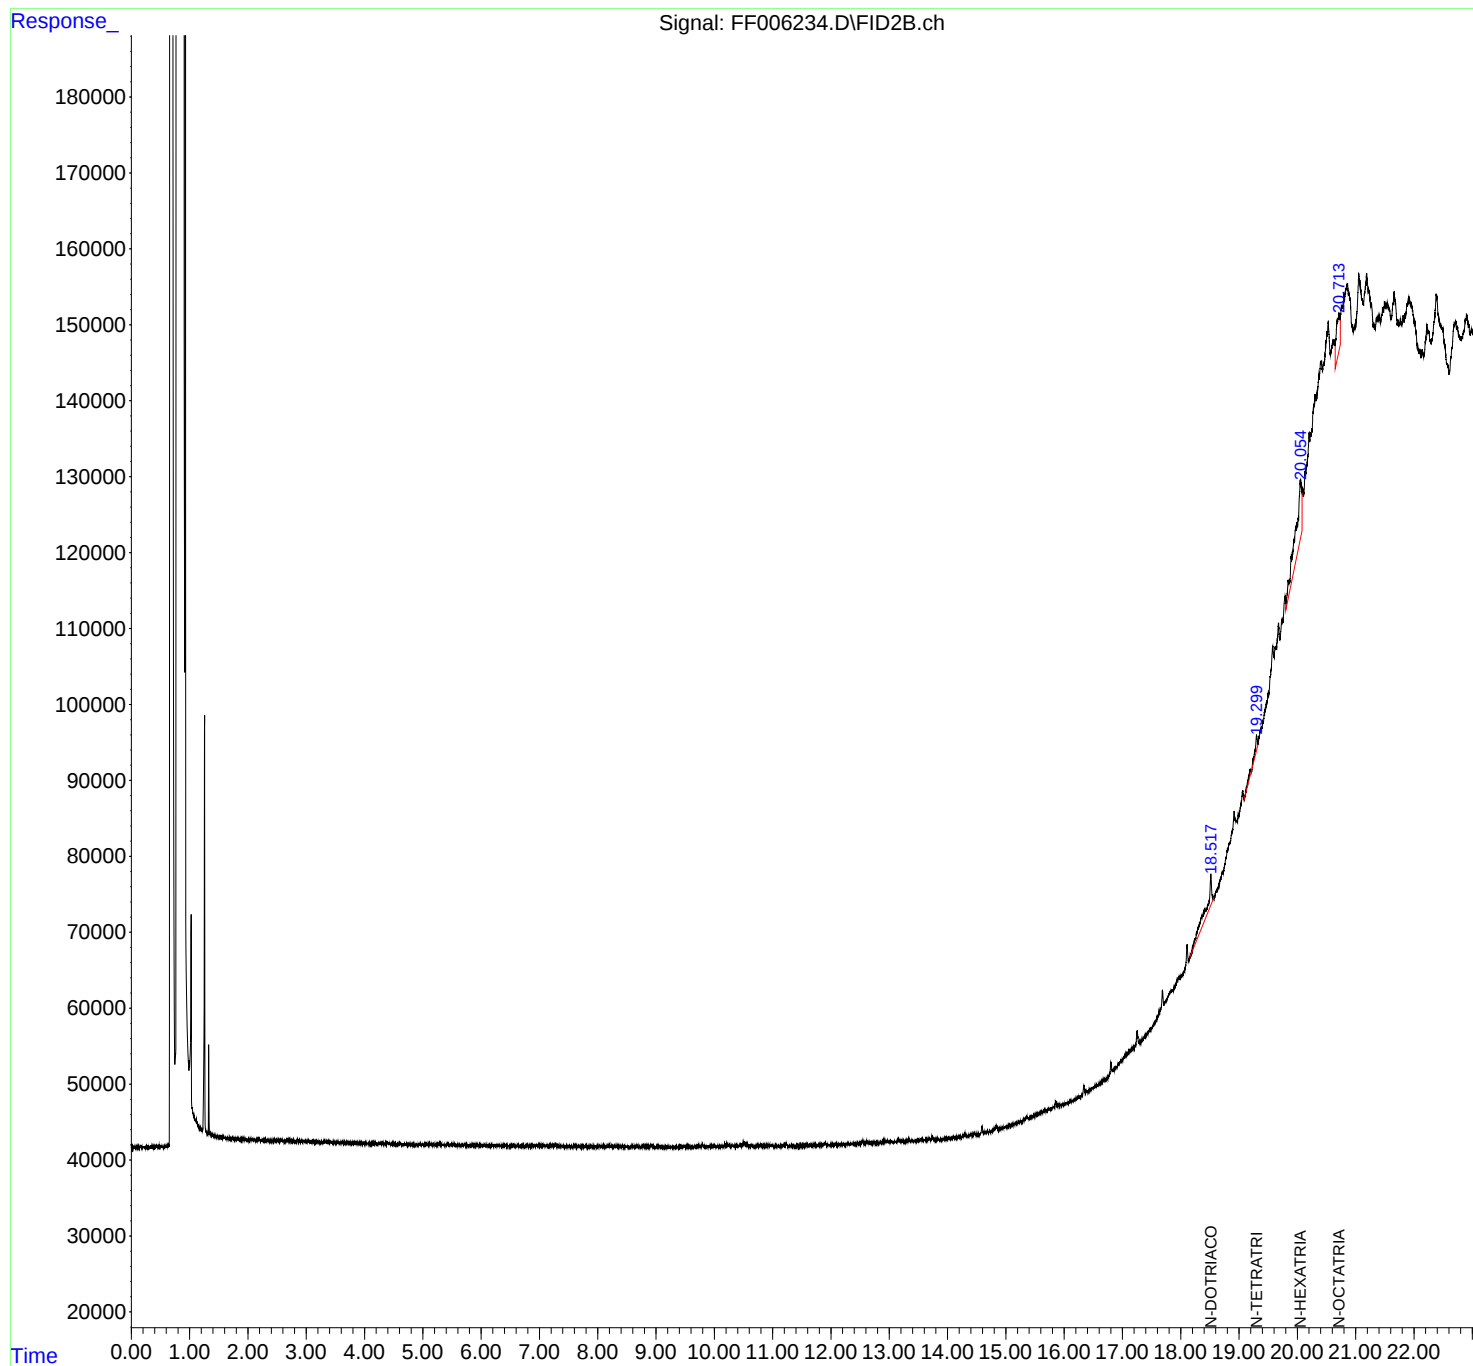


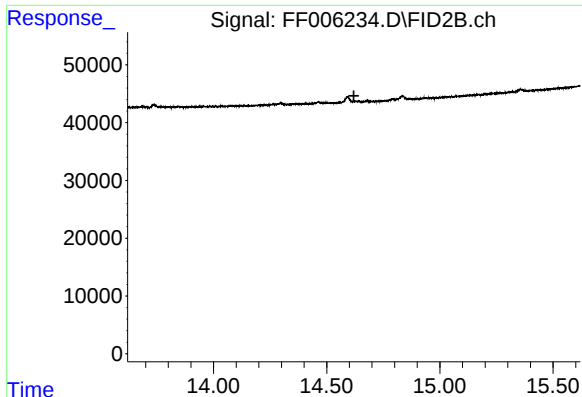

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.620 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

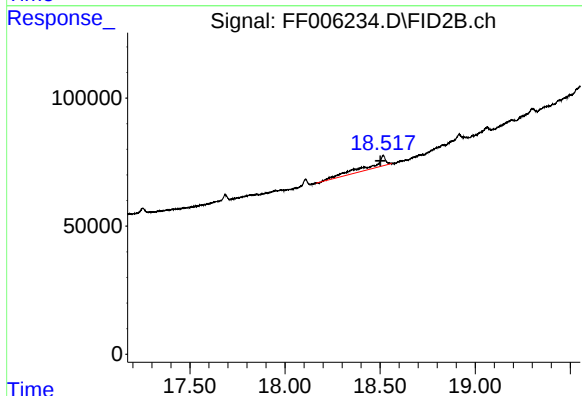


#14 N-DOTRIACONTANE

R.T.: 18.516 min
Delta R.T.: 0.015 min
Response: 248460
Conc: 2.15 ug/ml

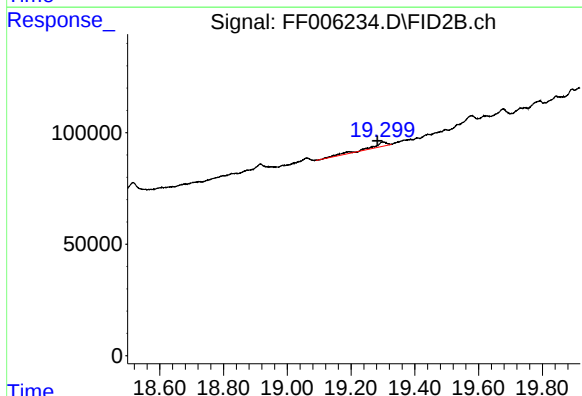


#15 N-TETRATRIACONTANE

R.T.: 19.300 min
Delta R.T.: 0.017 min
Response: 76741
Conc: 0.68 ug/ml

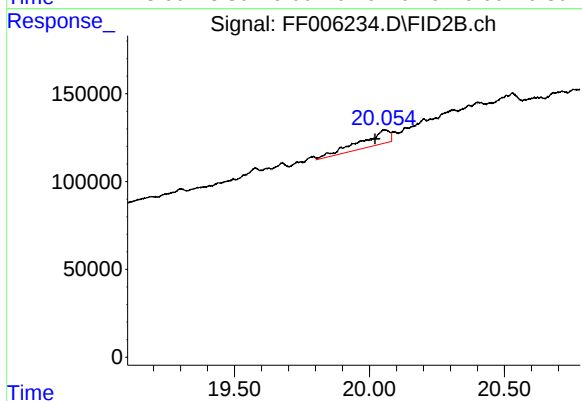

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: 0.031 min
Response: 611755
Conc: 5.72 ug/ml

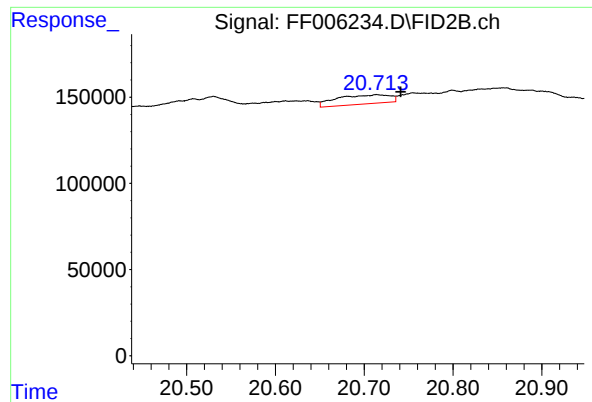

#17 N-OCTATRIACONTANE

R.T.: 20.715 min
Delta R.T.: -0.027 min
Response: 220129
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :