

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
 Data File : FF006237.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2020 12:44
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 01:29:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	254891	2.352 ug/ml
Target Compounds			
3) N-DODECANE	6.400	2892914	22.908 ug/ml
12) N-OCTACOSANE	16.803	2756144	22.672 ug/ml
13) N-TRIACONTANE	17.686	146234	1.220 ug/ml
14) N-DOTRIACONTANE	18.517	133576	1.156 ug/ml
15) N-TETRATRIACONTANE	19.301	160293	1.423 ug/ml
16) N-HEXATRIACONTANE	20.041	444072	4.153 ug/ml
17) N-OCTATRIACONTANE	20.768	548395	5.928 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006237.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 12:44
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:29:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

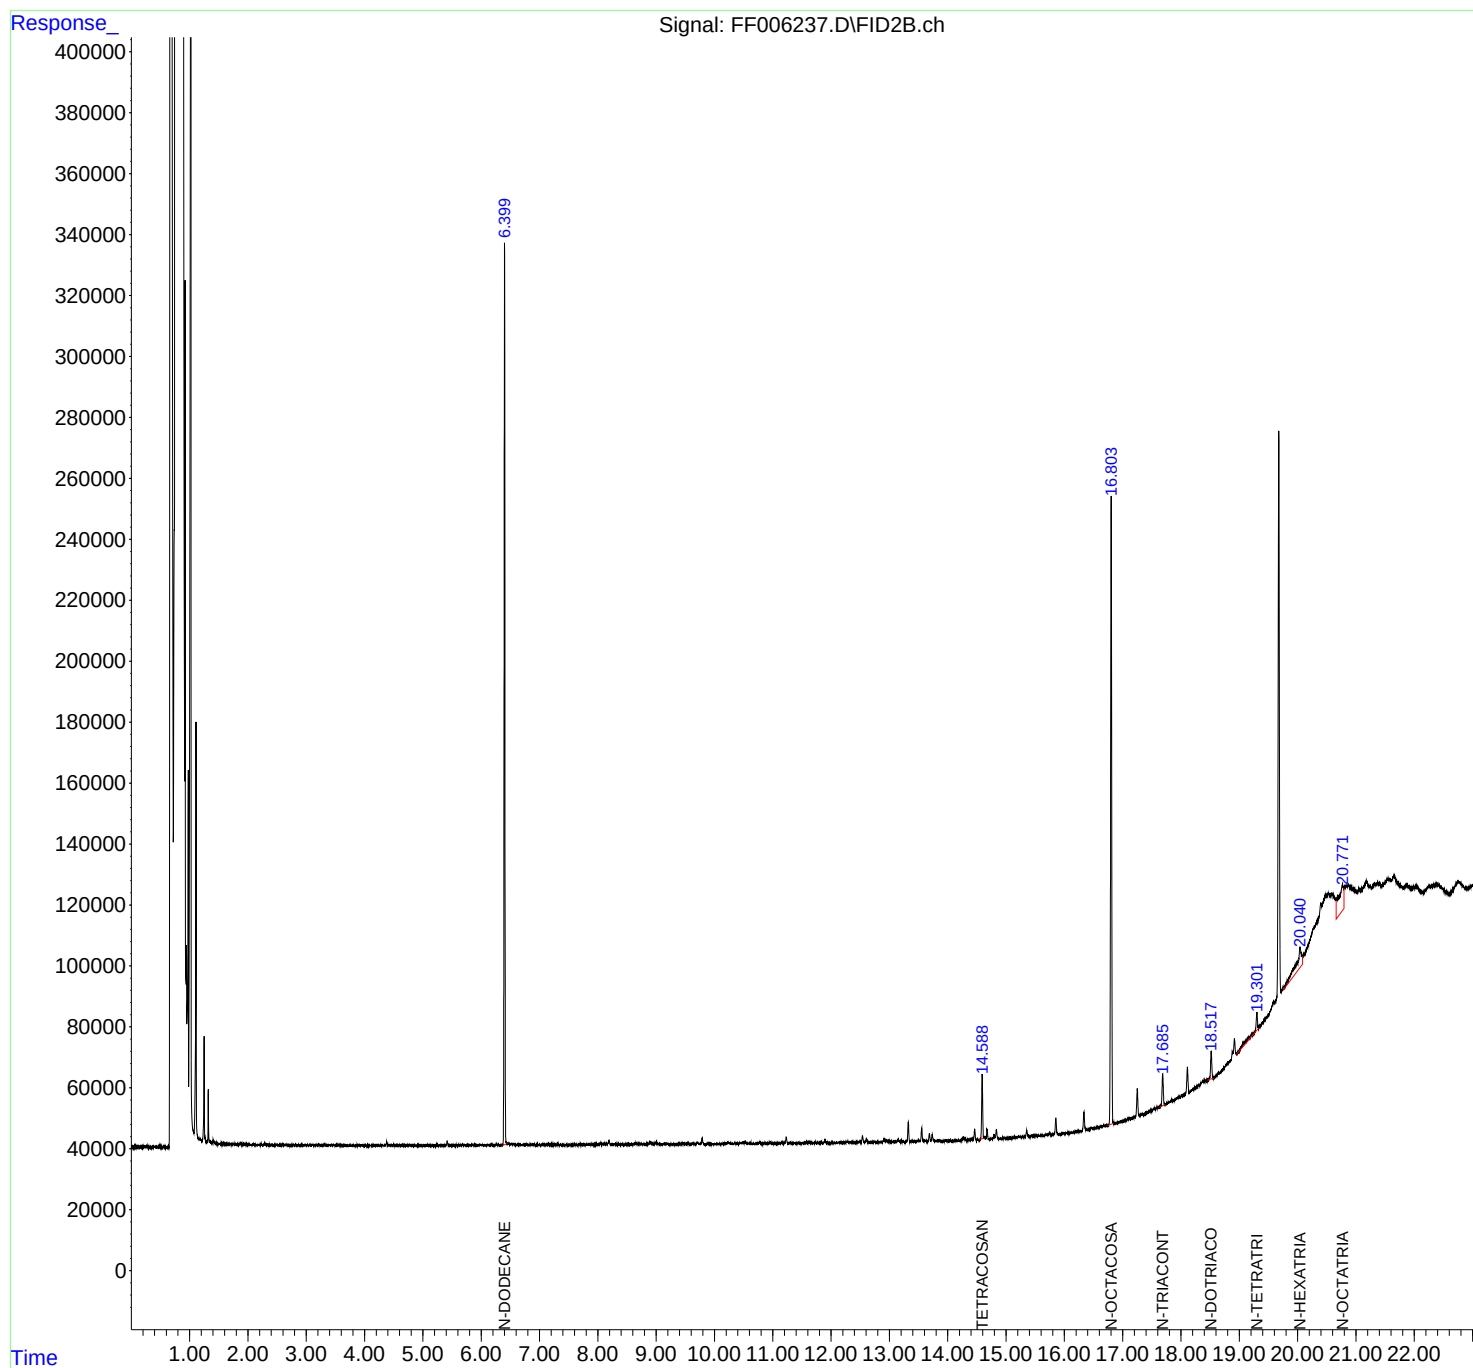


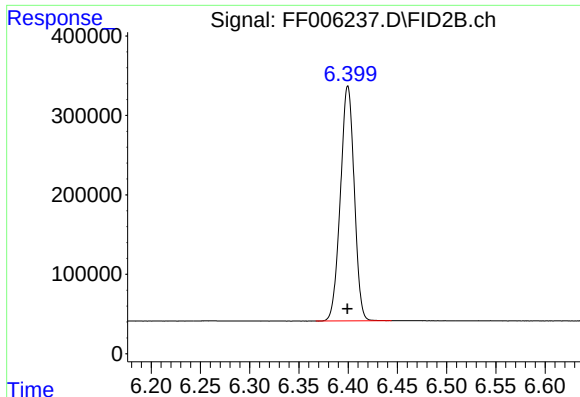

#3 N-DODECANE


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 2892914
Conc: 22.91 ug/ml

Instrument :
FID_F
ClientSampleId :

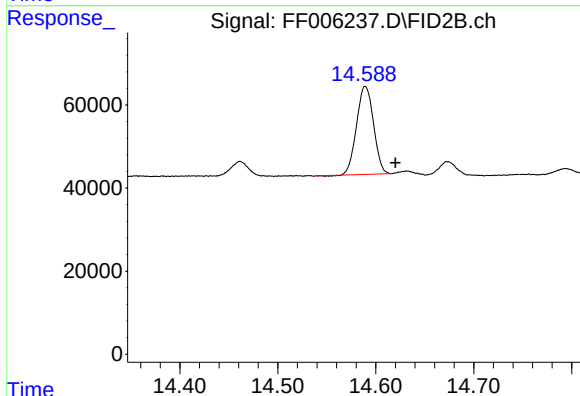


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.589 min
Delta R.T.: -0.031 min
Response: 254891
Conc: 2.35 ug/ml

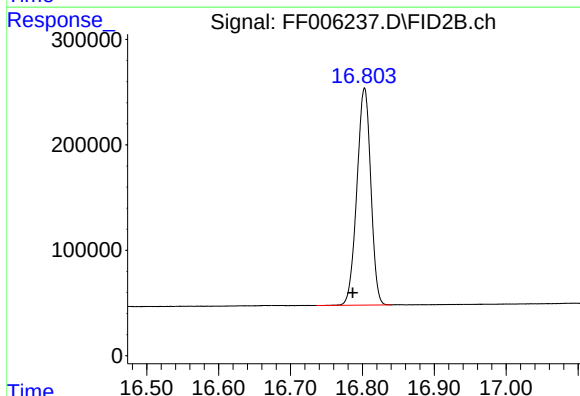


#12 N-OCTACOSANE

R.T.: 16.803 min
Delta R.T.: 0.017 min
Response: 2756144
Conc: 22.67 ug/ml

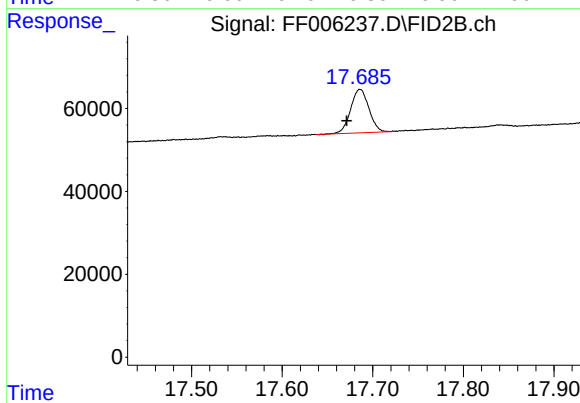

#13 N-TRIACONTANE


R.T.: 17.686 min
Delta R.T.: 0.015 min
Response: 146234
Conc: 1.22 ug/ml

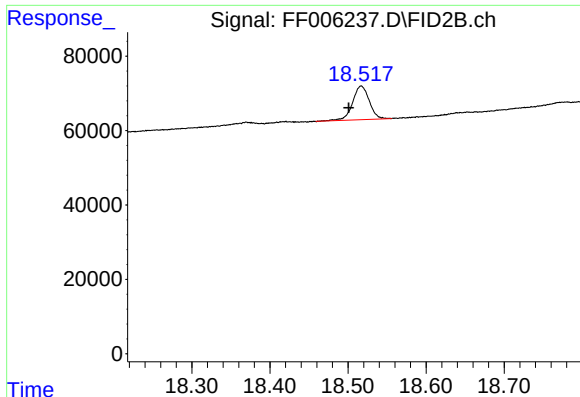

#14 N-DOTRIACONTANE


R.T.: 18.517 min
Delta R.T.: 0.016 min
Response: 133576
Conc: 1.16 ug/ml

Instrument :
FID_F
ClientSampleId :

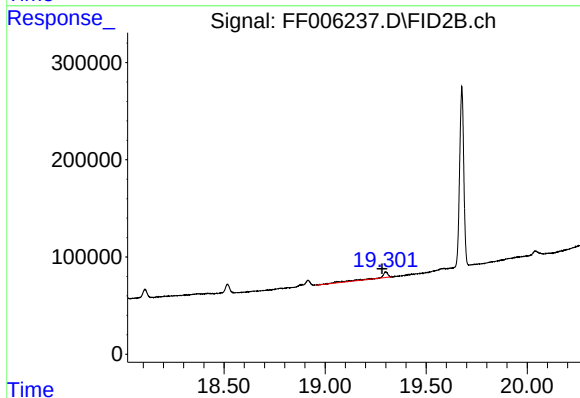


#15 N-TETRATRIACONTANE

R.T.: 19.301 min
Delta R.T.: 0.018 min
Response: 160293
Conc: 1.42 ug/ml

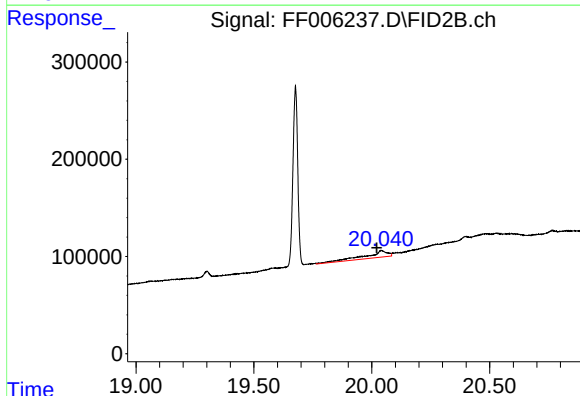

#16 N-HEXATRIACONTANE

R.T.: 20.041 min
Delta R.T.: 0.019 min
Response: 444072
Conc: 4.15 ug/ml

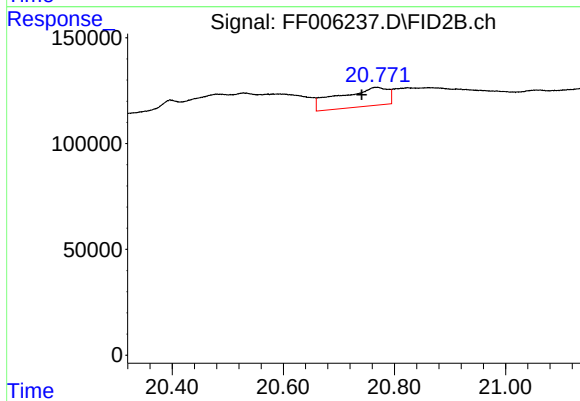

#17 N-OCTATRIACONTANE

R.T.: 20.768 min
Delta R.T.: 0.026 min
Response: 548395
Conc: 5.93 ug/ml