

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
 Data File : FF006238.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2020 13:41
 Operator : DD\AJ
 Sample : L1164-06
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 01:30:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	1534985	14.166 ug/ml
Target Compounds			
4) N-TETRADECANE	8.251f	292145	2.314 ug/ml
8) N-DOCOSANE	13.735	161916	1.284 ug/ml
10) N-TETRACOSANE	14.826	279852	2.247 ug/ml
11) N-HEXACOSANE	15.856	244799	1.991 ug/ml
12) N-OCTACOSANE	16.804	685471	5.639 ug/ml
13) N-TRIACONTANE	17.693	614663	5.126 ug/ml
14) N-DOTRIACONTANE	18.519	894899	7.744 ug/ml
15) N-TETRATRIACONTANE	19.309	262616	2.331 ug/ml
16) N-HEXATRIACONTANE	20.052	436430	4.082 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006238.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 13:41
Operator : DD\AJ
Sample : L1164-06
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:30:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

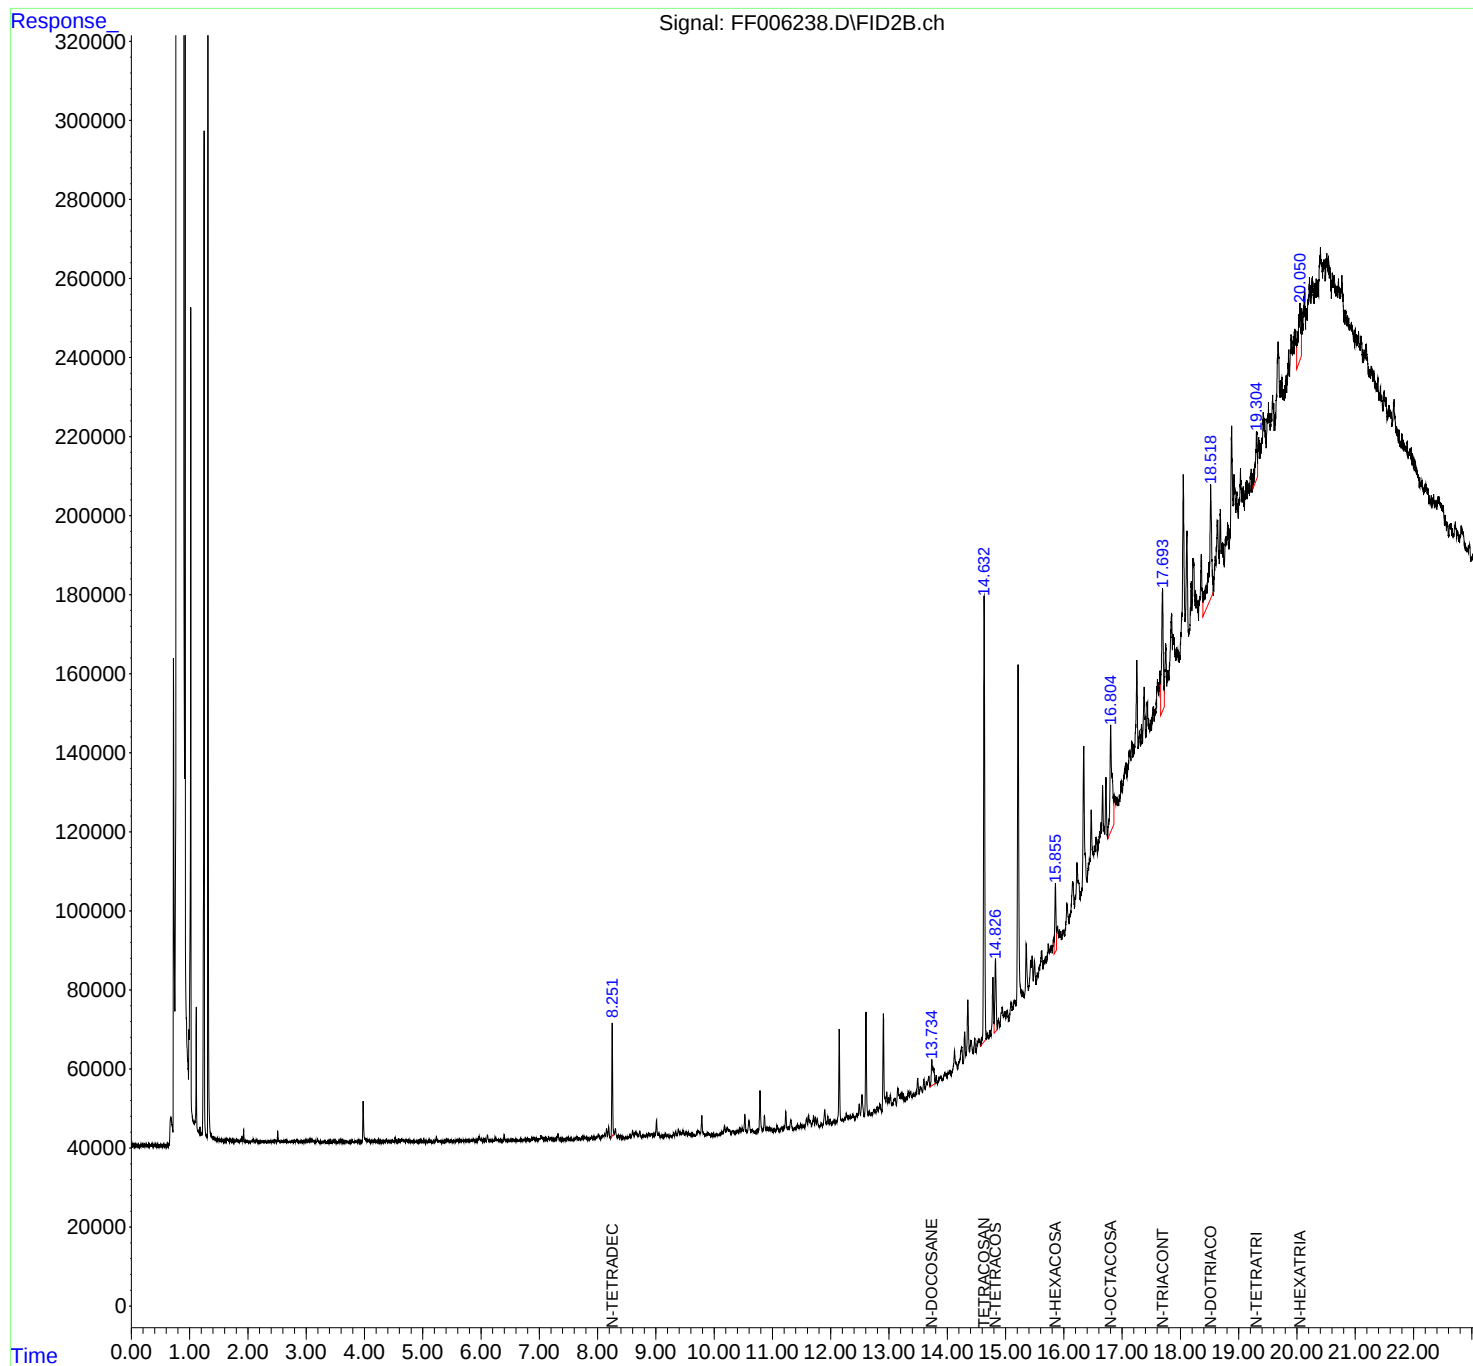


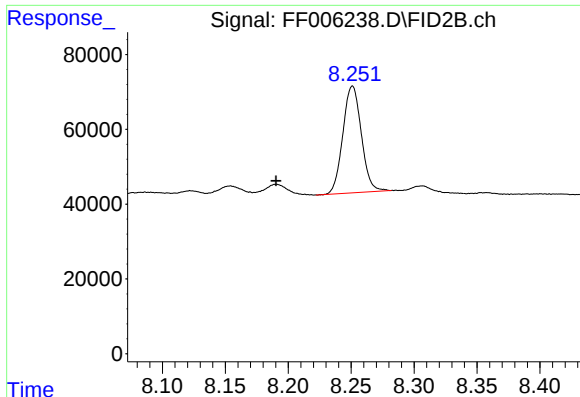

#4 N-TETRADECANE


R.T.: 8.251 min
Delta R.T.: 0.061 min
Response: 292145
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :

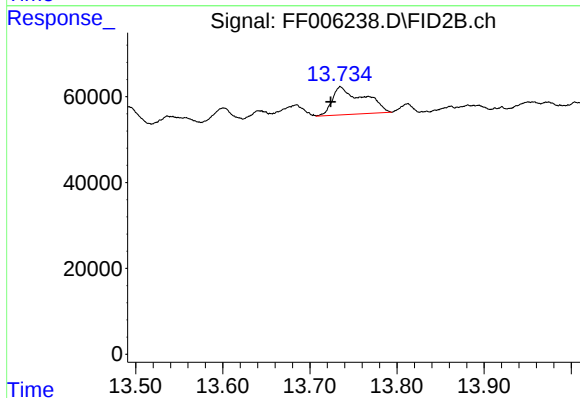


#8 N-DOCOSANE

R.T.: 13.735 min
Delta R.T.: 0.011 min
Response: 161916
Conc: 1.28 ug/ml

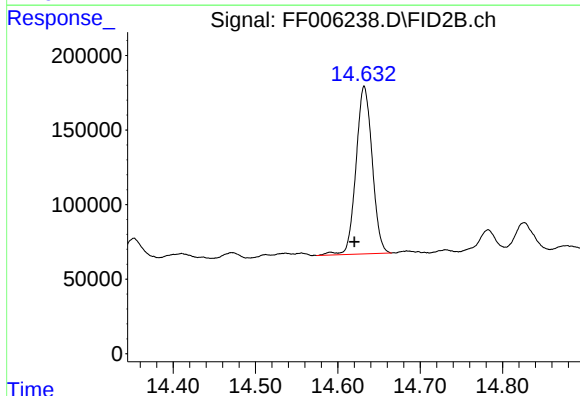


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: 0.012 min
Response: 1534985
Conc: 14.17 ug/ml

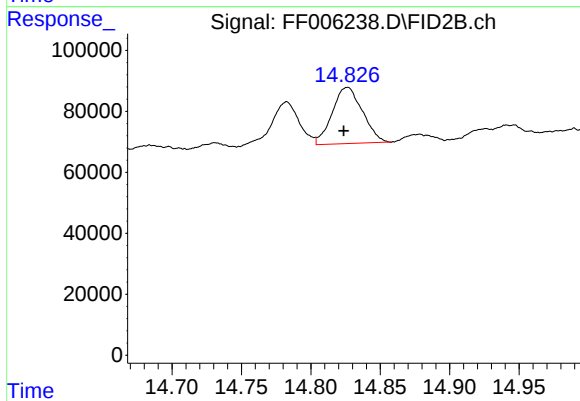

#10 N-TETRACOSANE


R.T.: 14.826 min
Delta R.T.: 0.003 min
Response: 279852
Conc: 2.25 ug/ml

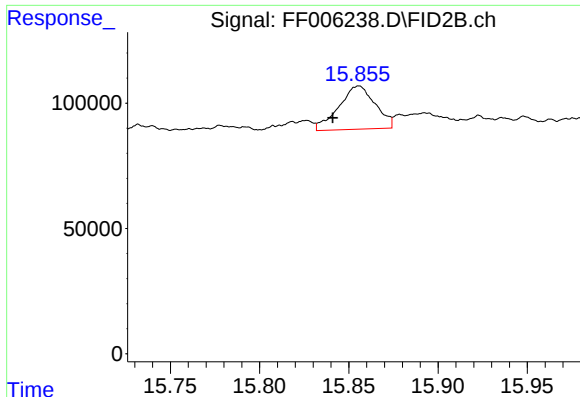

#11 N-HEXACOSANE


R.T.: 15.856 min
Delta R.T.: 0.015 min
Response: 244799
Conc: 1.99 ug/ml

Instrument :
FID_F
ClientSampleId :

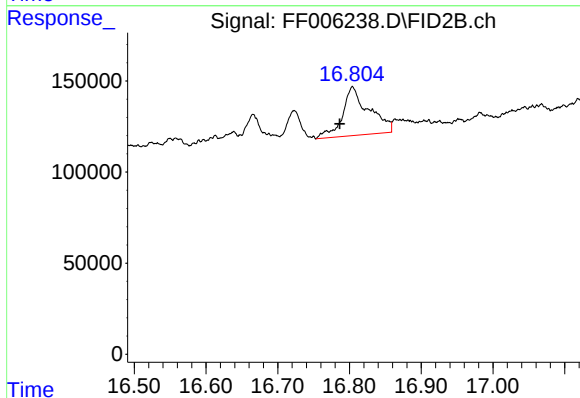


#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: 0.018 min
Response: 685471
Conc: 5.64 ug/ml

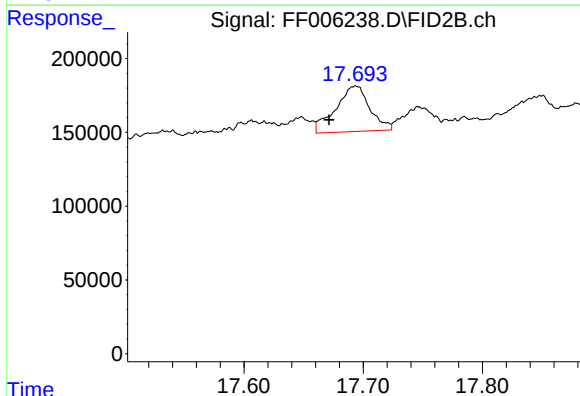


#13 N-TRIACONTANE

R.T.: 17.693 min
Delta R.T.: 0.022 min
Response: 614663
Conc: 5.13 ug/ml

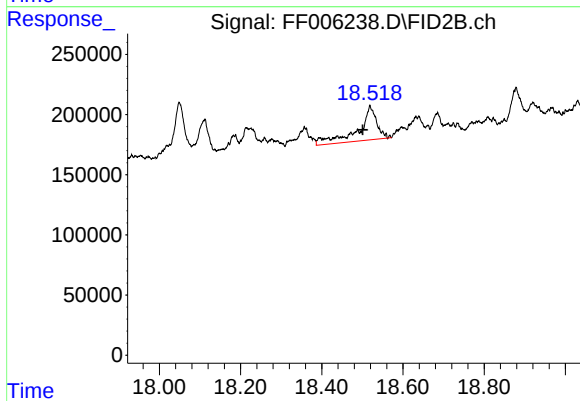

#14 N-DOTRIACONTANE


R.T.: 18.519 min
Delta R.T.: 0.018 min
Response: 894899
Conc: 7.74 ug/ml

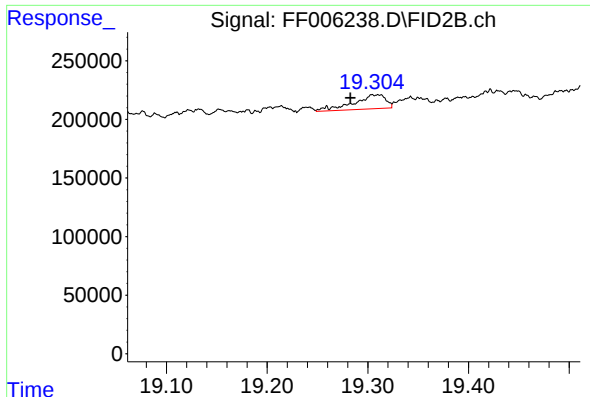

#15 N-TETRATRIACONTANE

R.T.: 19.309 min
Delta R.T.: 0.026 min
Response: 262616
Conc: 2.33 ug/ml

Instrument :
FID_F
ClientSampleId :

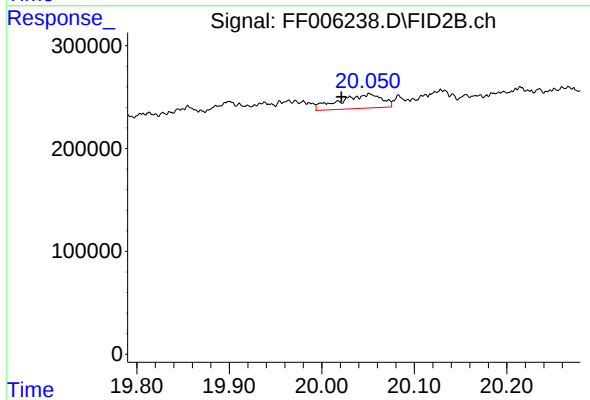

#16 N-HEXATRIACONTANE

R.T.: 20.052 min
Delta R.T.: 0.031 min
Response: 436430
Conc: 4.08 ug/ml