

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
 Data File : FF006242.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2020 16:12
 Operator : DD\AJ
 Sample : PB126191BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 01:31:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	2217422	20.464 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.807	32236	0.265 ug/ml
13) N-TRIACONTANE	17.691	219111	1.827 ug/ml
14) N-DOTRIACONTANE	18.523	407323	3.525 ug/ml
15) N-TETRATRIACONTANE	19.266	51716	0.459 ug/ml
16) N-HEXATRIACONTANE	20.044	260397	2.435 ug/ml
17) N-OCTATRIACONTANE	20.725	243066	2.627 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006242.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 16:12
Operator : DD\AJ
Sample : PB126191BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:31:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

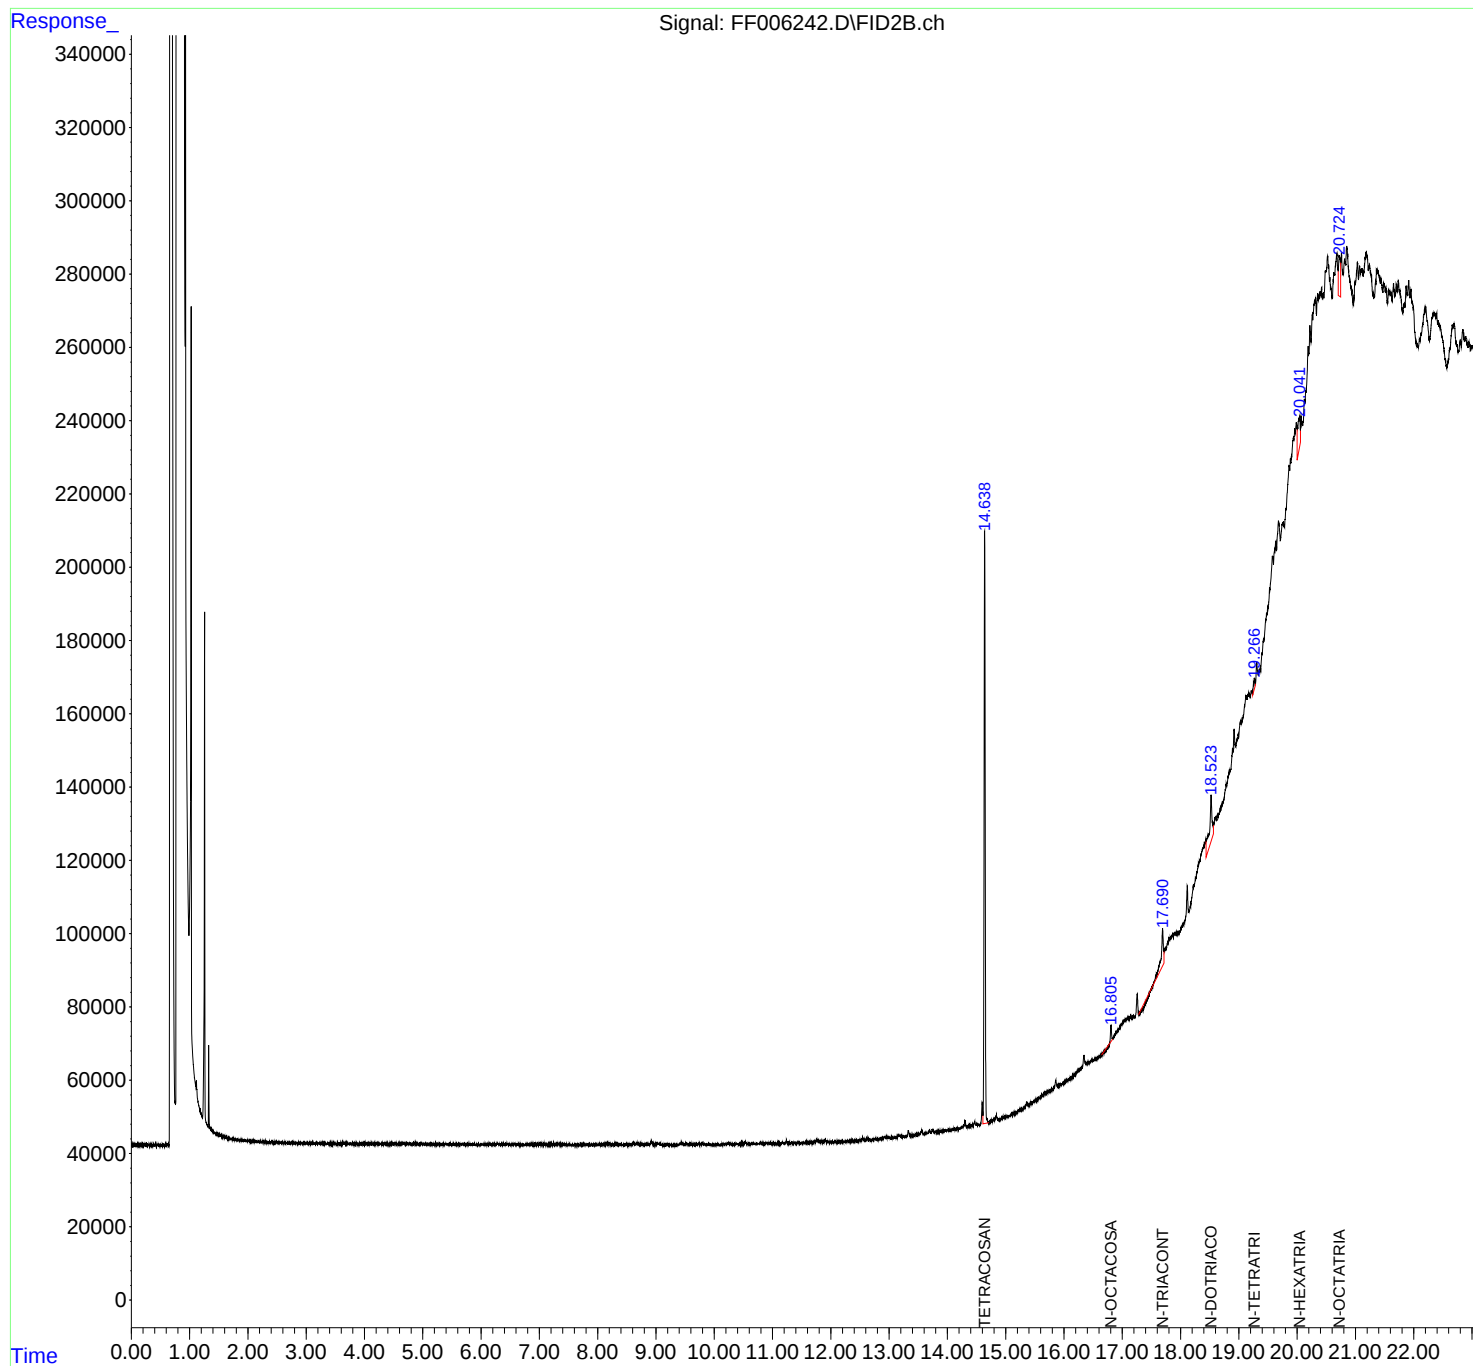


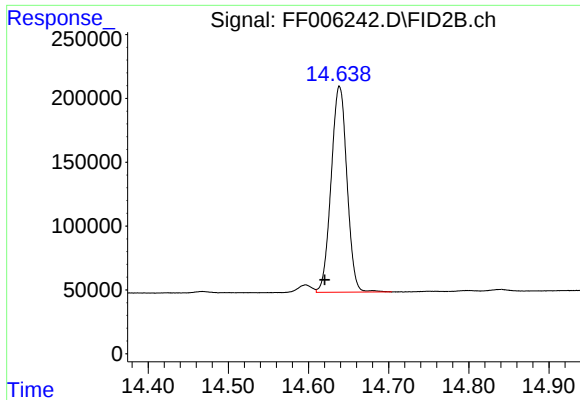

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.639 min
Delta R.T.: 0.019 min
Response: 2217422
Conc: 20.46 ug/ml

Instrument :
FID_F
ClientSampleId :

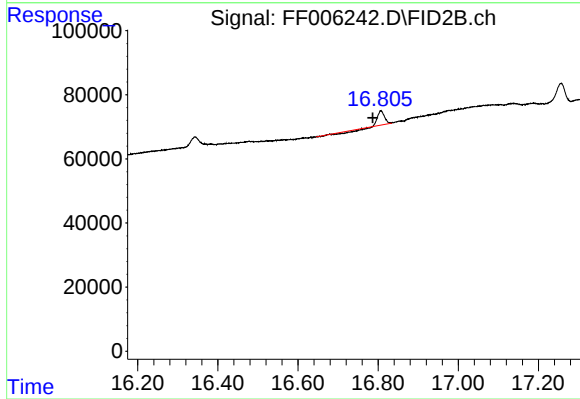


#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: 0.020 min
Response: 32236
Conc: 0.27 ug/ml

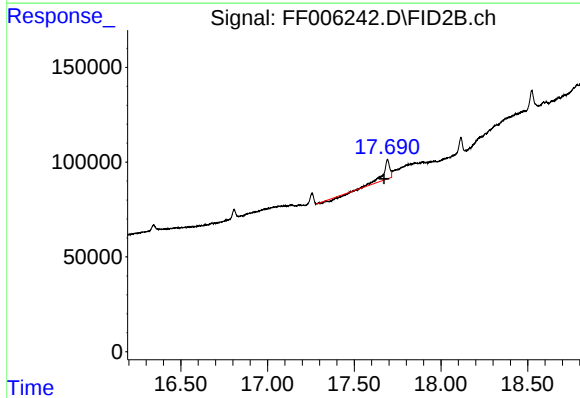


#13 N-TRIACONTANE

R.T.: 17.691 min
Delta R.T.: 0.020 min
Response: 219111
Conc: 1.83 ug/ml

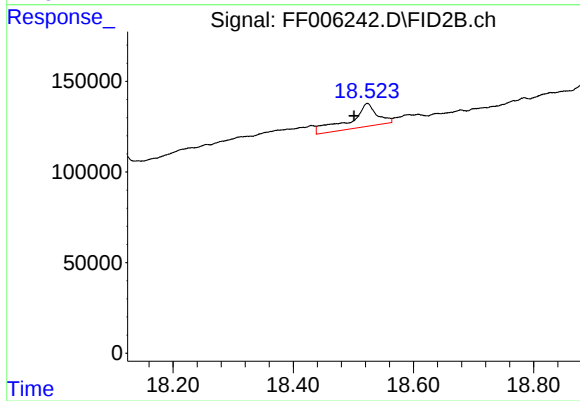

#14 N-DOTRIACONTANE


R.T.: 18.523 min
Delta R.T.: 0.022 min
Response: 407323
Conc: 3.52 ug/ml

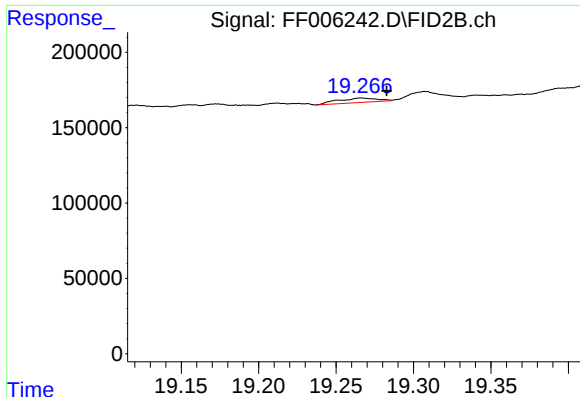

#15 N-TETRATRIACONTANE


R.T.: 19.266 min
Delta R.T.: -0.017 min
Response: 51716
Conc: 0.46 ug/ml

Instrument :
FID_F
ClientSampleId :

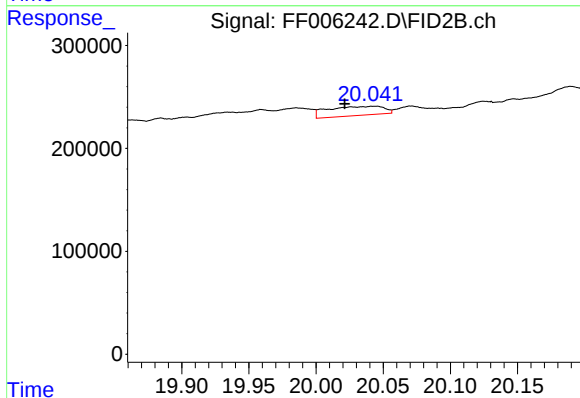

#16 N-HEXATRIACONTANE

R.T.: 20.044 min
Delta R.T.: 0.022 min
Response: 260397
Conc: 2.44 ug/ml

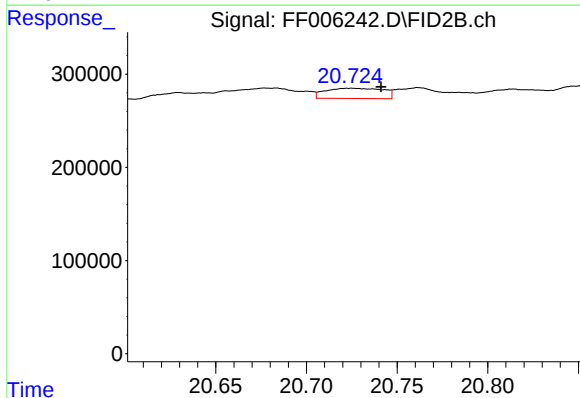

#17 N-OCTATRIACONTANE

R.T.: 20.725 min
Delta R.T.: -0.016 min
Response: 243066
Conc: 2.63 ug/ml