

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
 Data File : FF006244.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2020 17:12
 Operator : DD\AJ
 Sample : L1164-06 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 01:31:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	273893	2.528 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.806	111594	0.918 ug/ml
13) N-TRIACONTANE	17.653	96222	0.803 ug/ml
14) N-DOTRIACONTANE	18.519	233401	2.020 ug/ml
15) N-TETRATRIACONTANE	19.303	32995	0.293 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012020\
Data File : FF006244.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2020 17:12
Operator : DD\AJ
Sample : L1164-06 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 01:31:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

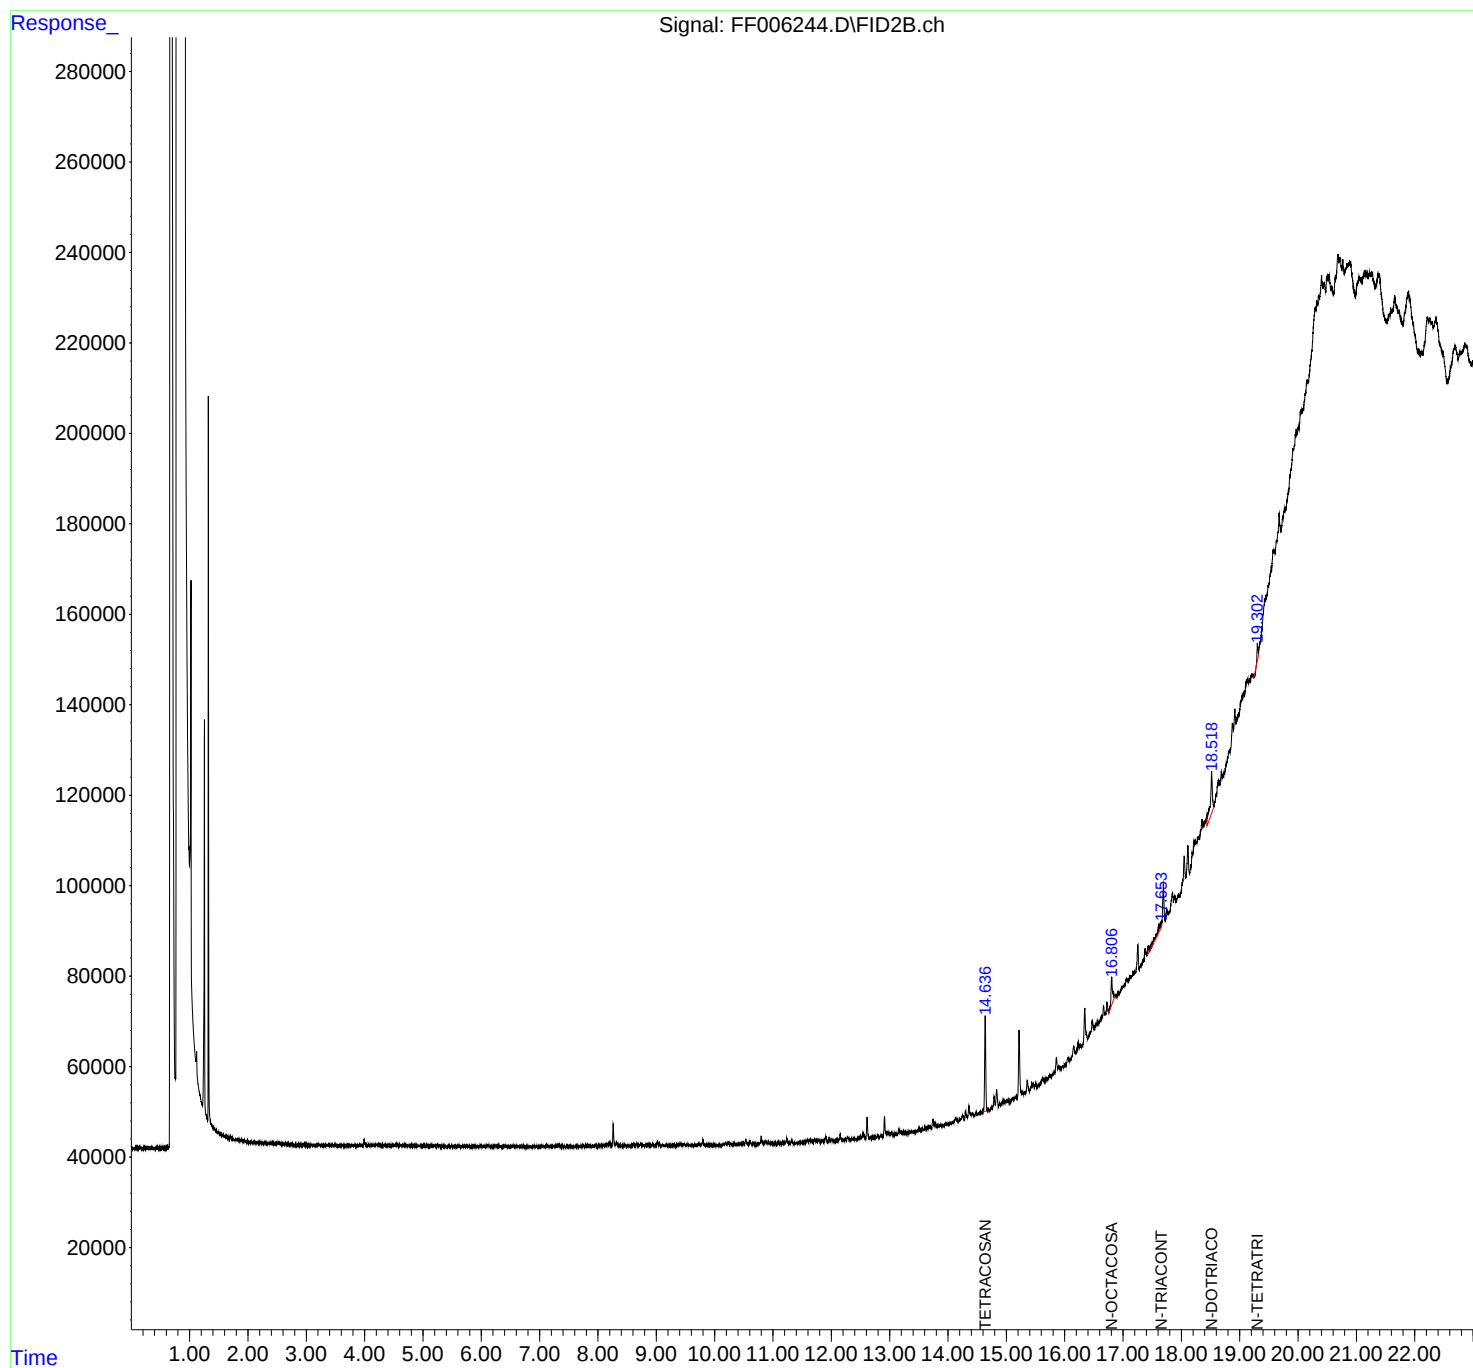


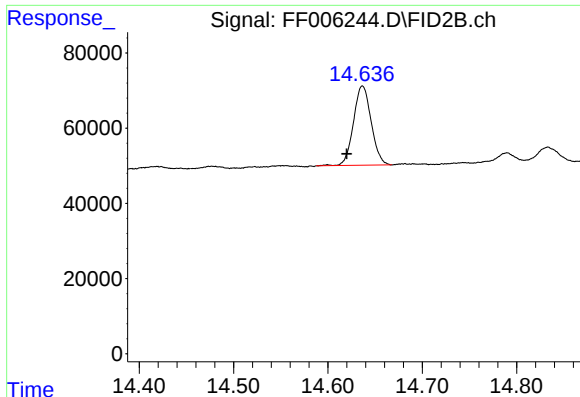

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.637 min
Delta R.T.: 0.017 min
Response: 273893
Conc: 2.53 ug/ml

Instrument :
FID_F
ClientSampleId :

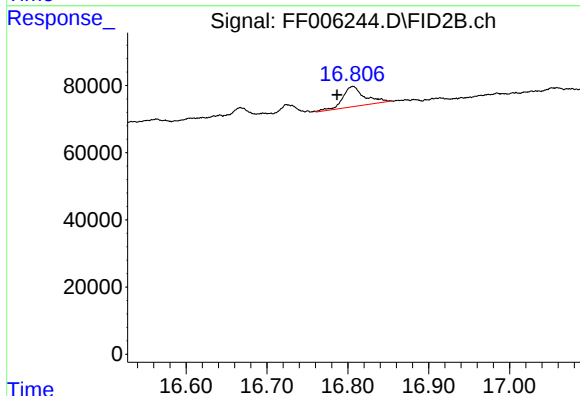


#12 N-OCTACOSANE

R.T.: 16.806 min
Delta R.T.: 0.020 min
Response: 111594
Conc: 0.92 ug/ml

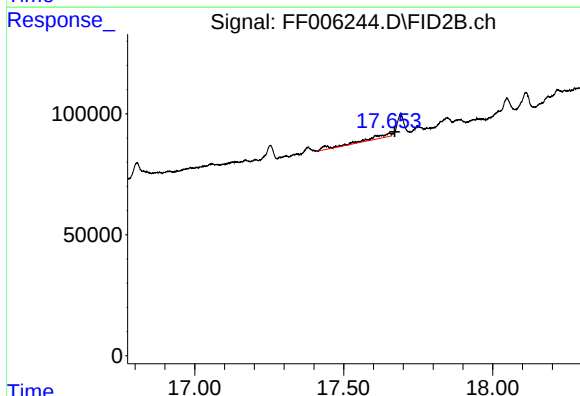


#13 N-TRIACONTANE

R.T.: 17.653 min
Delta R.T.: -0.018 min
Response: 96222
Conc: 0.80 ug/ml

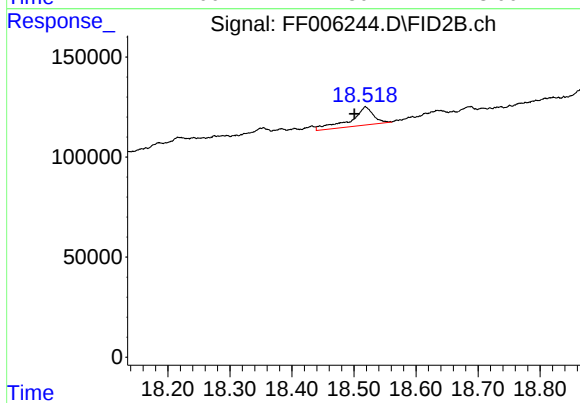

#14 N-DOTRIACONTANE

R.T.: 18.519 min
Delta R.T.: 0.018 min
Response: 233401
Conc: 2.02 ug/ml

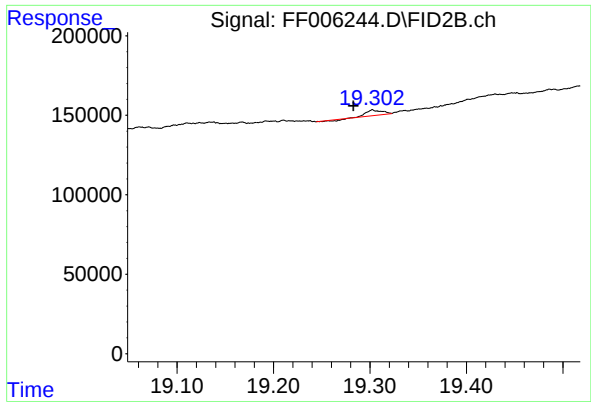

#15 N-TETRATRIACONTANE

R.T.: 19.303 min
Delta R.T.: 0.021 min
Response: 32995
Conc: 0.29 ug/ml

Instrument :
FID_F
ClientSampleId :