

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009727.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 15:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 23:48:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.242	4281547	29.920 ug/ml
11)	N-HEXACOSANE	15.664	41612	0.285 ug/ml
12)	N-OCTACOSANE	16.611	3904128	26.894 ug/ml
13)	N-TRIACONTANE	17.493	122235	0.854 ug/ml
14)	N-DOTRIACONTANE	18.323	178013	1.308 ug/ml
15)	N-TETRATRIACONTANE	19.101	129165	1.087 ug/ml
16)	N-HEXATRIACONTANE	19.840	76789	0.745 ug/ml
18)	N-TETRACONTANE	21.400	233468	2.570 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009727.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 15:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 23:48:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

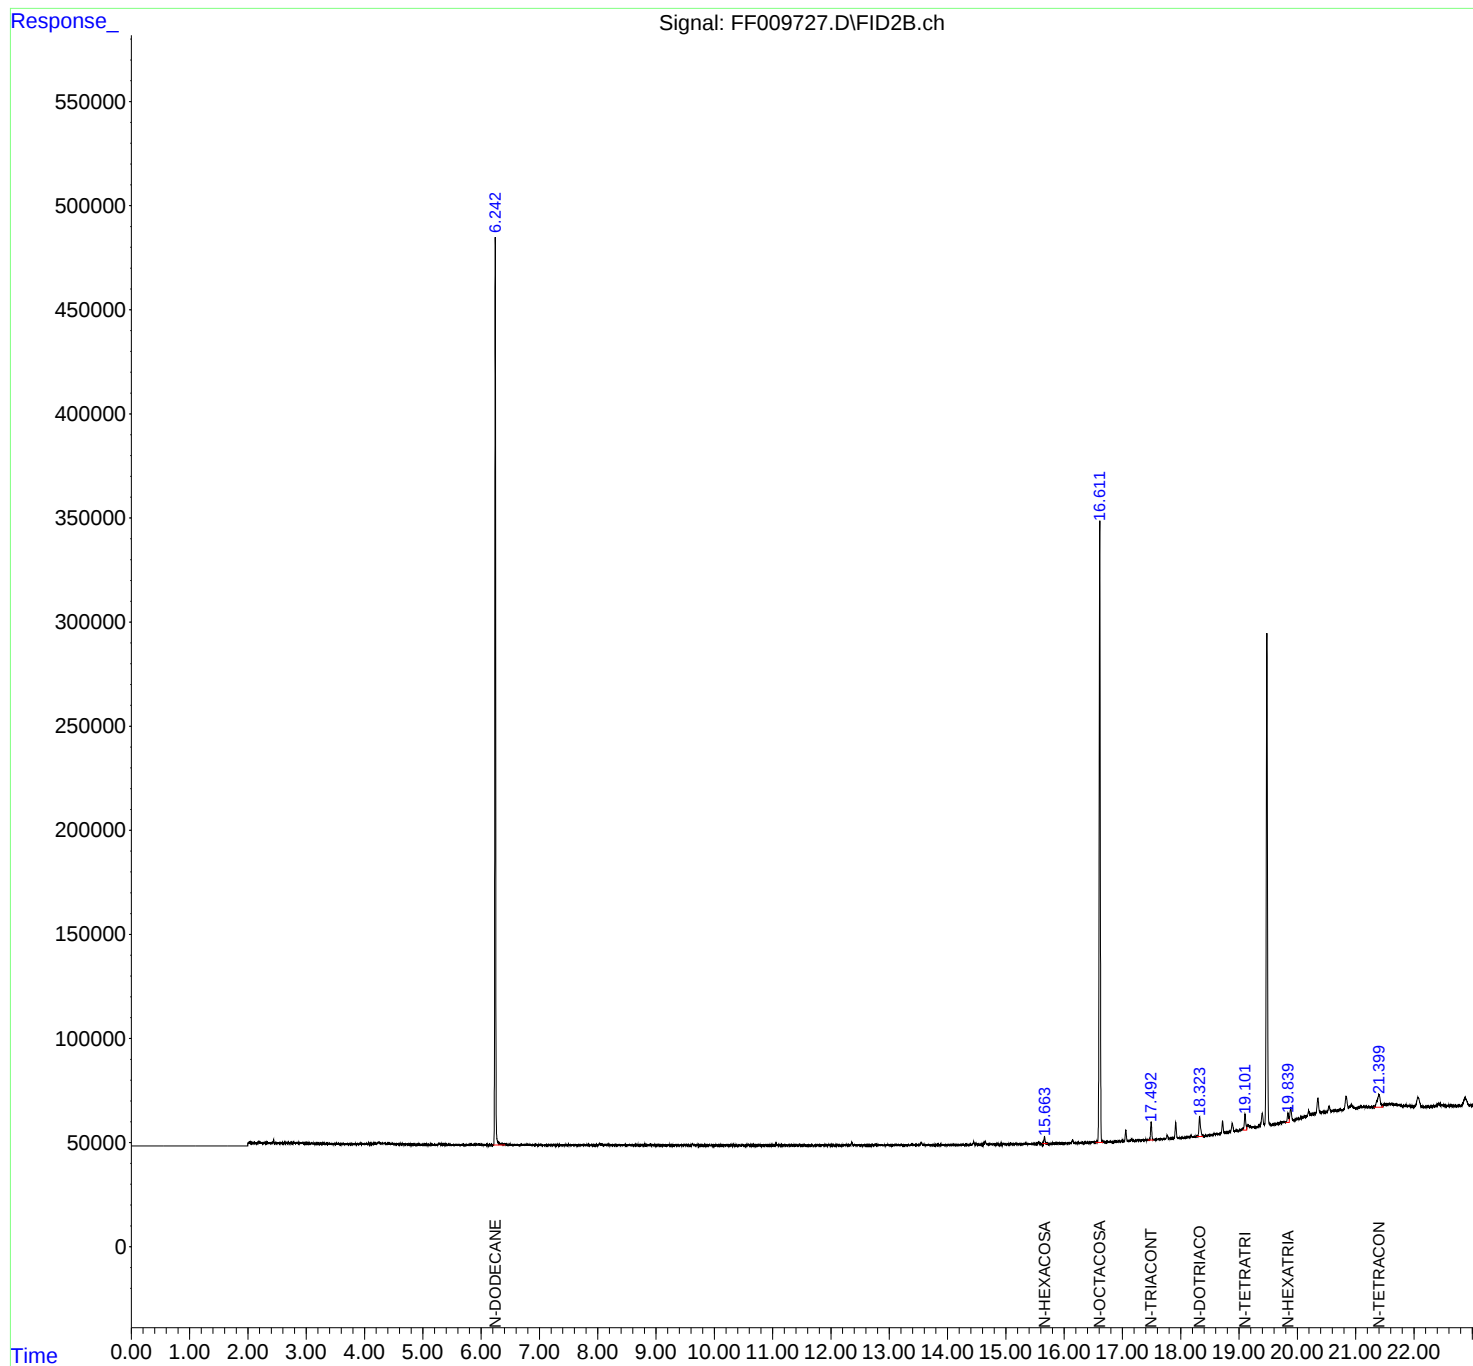


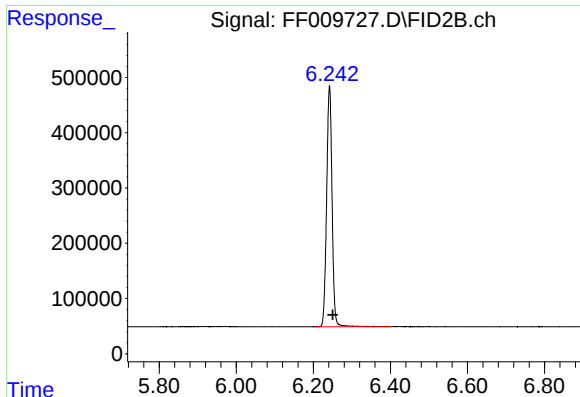

#3 N-DODECANE


R.T.: 6.242 min
Delta R.T.: -0.008 min
Response: 4281547
Conc: 29.92 ug/ml

Instrument :
FID_F
ClientSampleId :

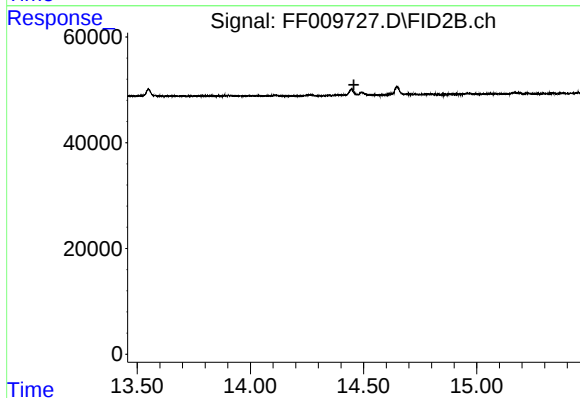


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

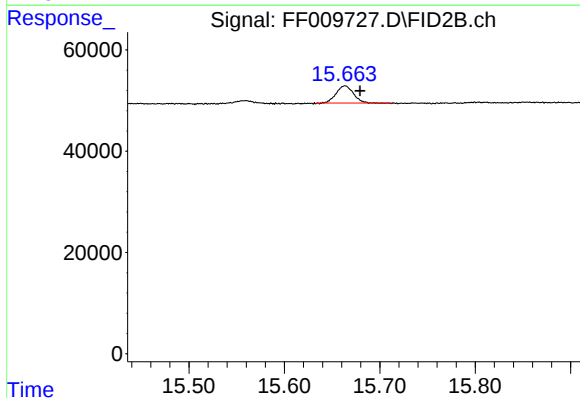


#11 N-HEXACOSANE

R.T.: 15.664 min
Delta R.T.: -0.016 min
Response: 41612
Conc: 0.28 ug/ml

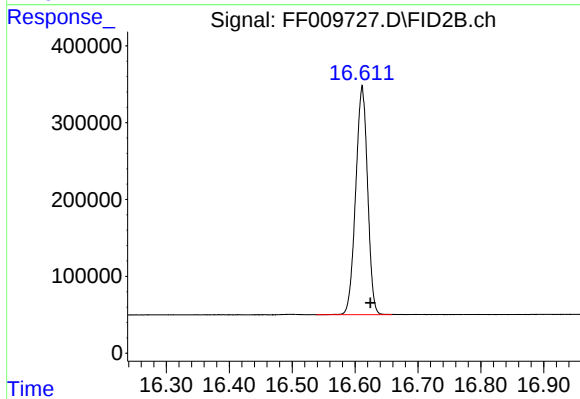

#12 N-OCTACOSANE


R.T.: 16.611 min
Delta R.T.: -0.013 min
Response: 3904128
Conc: 26.89 ug/ml

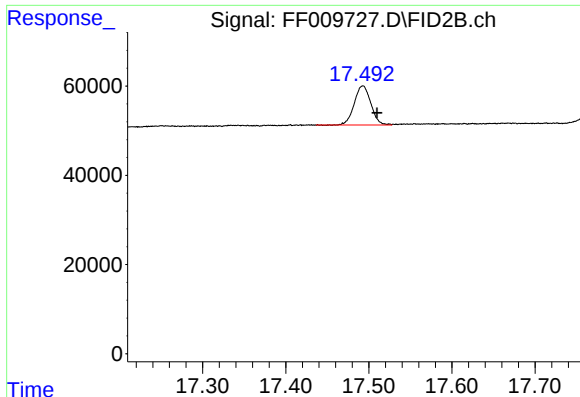

#13 N-TRIACONTANE


R.T.: 17.493 min
Delta R.T.: -0.017 min
Response: 122235
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

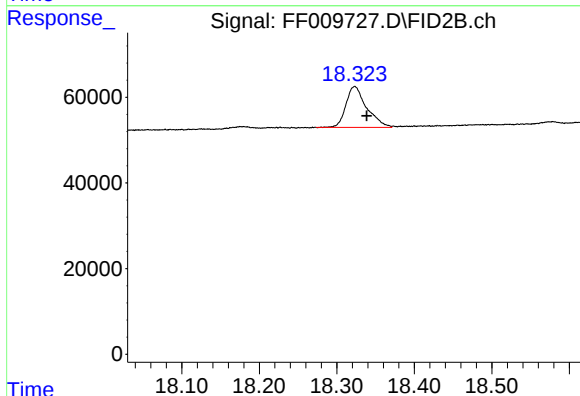


#14 N-DOTRIACONTANE

R.T.: 18.323 min
Delta R.T.: -0.015 min
Response: 178013
Conc: 1.31 ug/ml

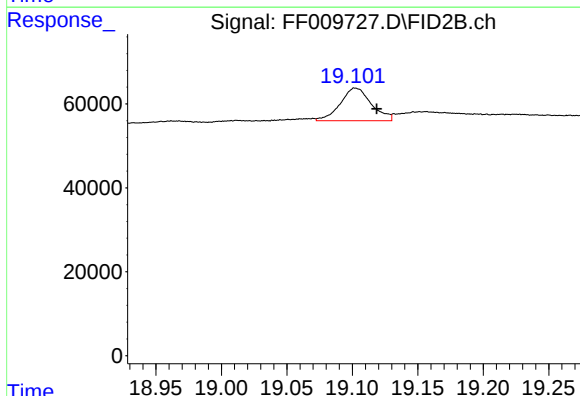


#15 N-TETRATRIACONTANE

R.T.: 19.101 min
Delta R.T.: -0.017 min
Response: 129165
Conc: 1.09 ug/ml

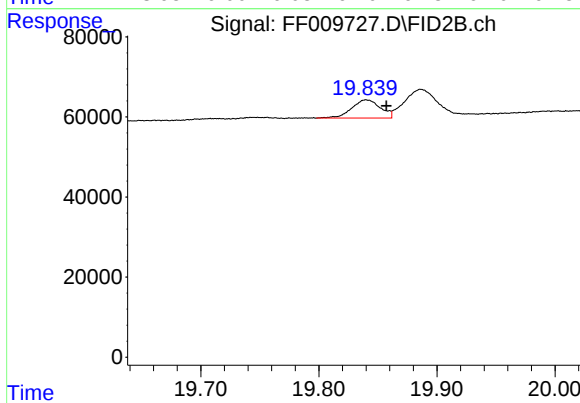

#16 N-HEXATRIACONTANE

R.T.: 19.840 min
Delta R.T.: -0.017 min
Response: 76789
Conc: 0.74 ug/ml

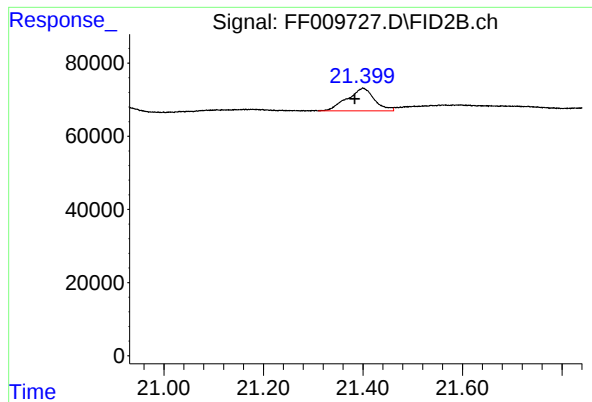

#18 N-TETRACONTANE

R.T.: 21.400 min
Delta R.T.: 0.016 min
Response: 233468
Conc: 2.57 ug/ml

Instrument :
FID_F
ClientSampleId :