

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009728.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 15:33
Operator : AJ\MA
Sample : PB142162BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 23:48:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.445	2431293	18.605 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.887	104649	1.015 ug/ml
18) N-TETRACONTANE	21.400	110032	1.211 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009728.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 15:33
Operator : AJ\MA
Sample : PB142162BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 20 23:48:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

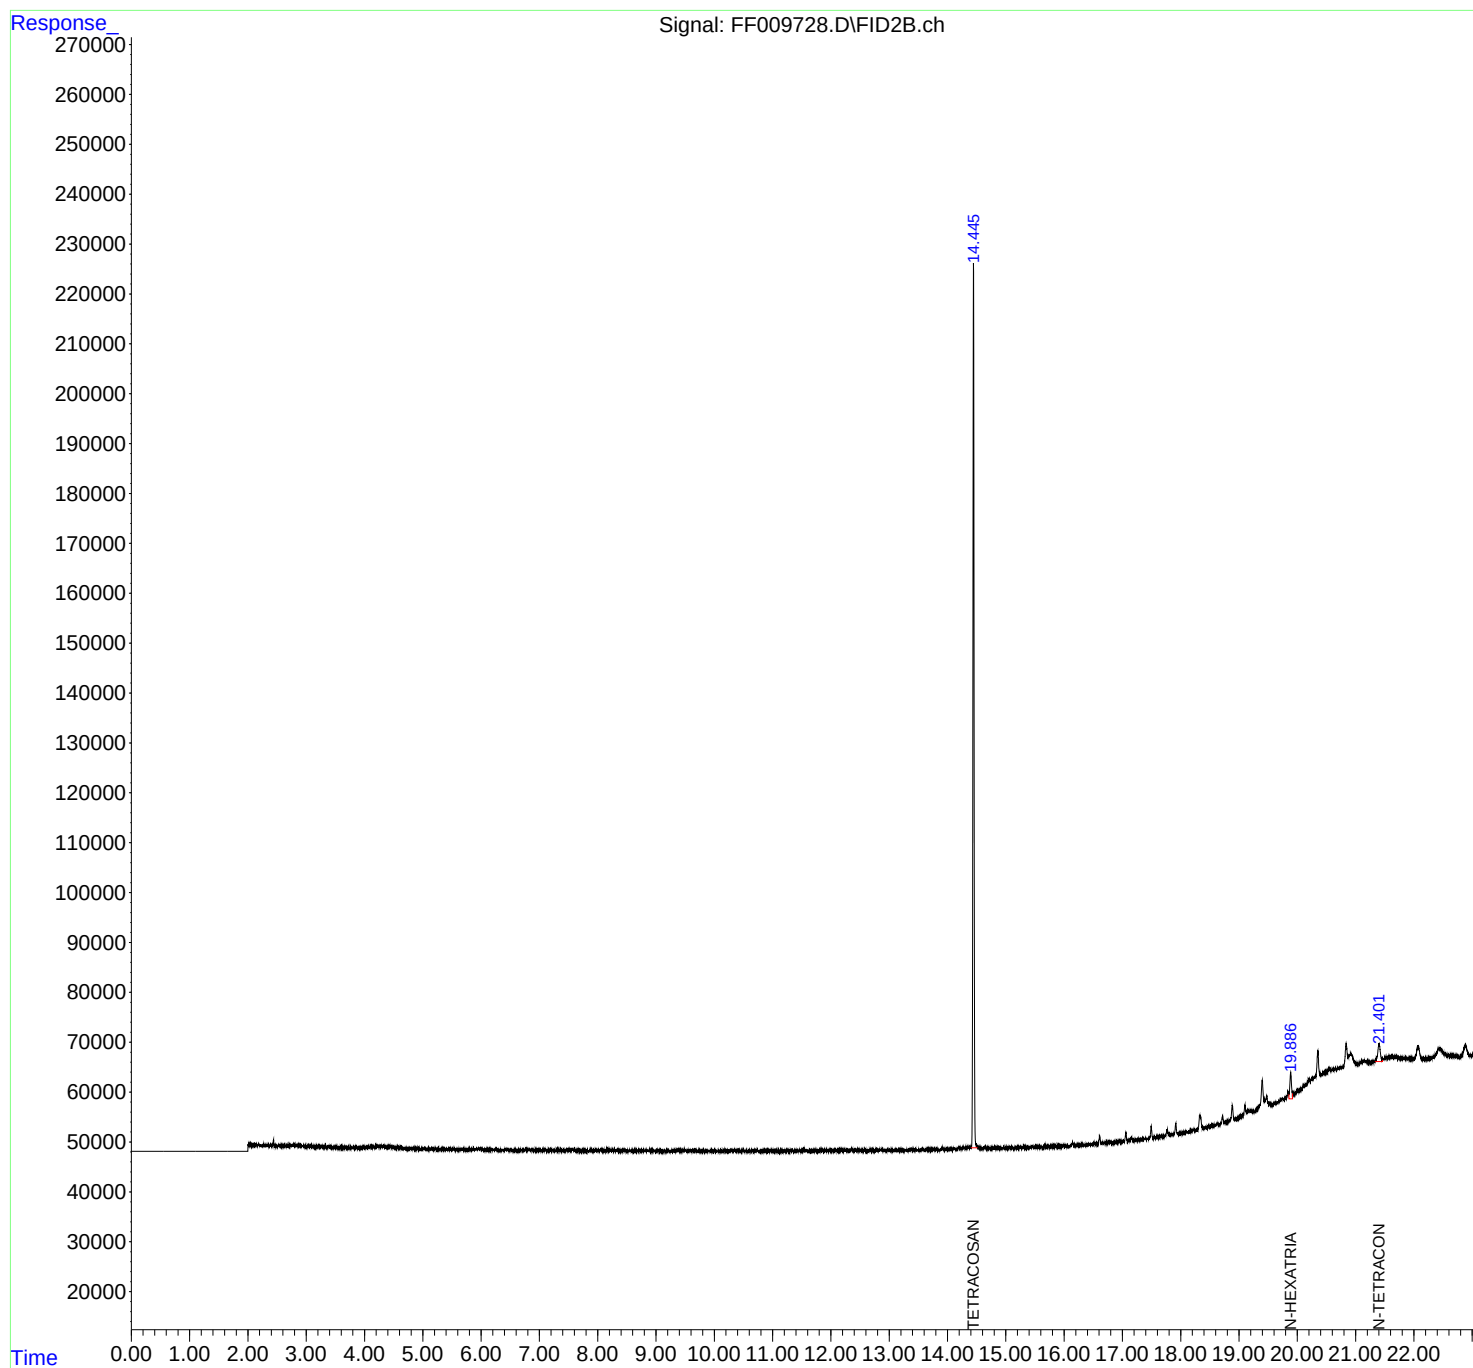


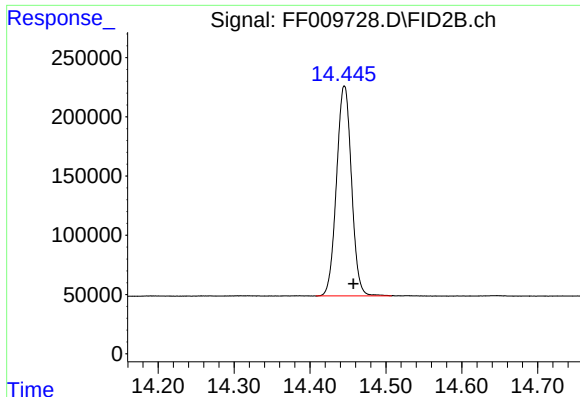

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.445 min
Delta R.T.: -0.012 min
Response: 2431293
Conc: 18.61 ug/ml

Instrument :
FID_F
ClientSampleId :

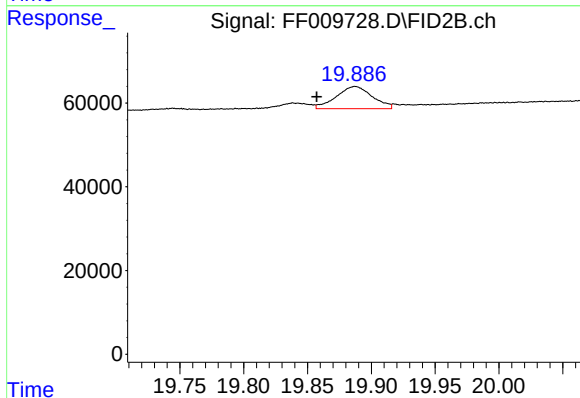

#16 N-HEXATRIACONTANE

R.T.: 19.887 min
Delta R.T.: 0.030 min
Response: 104649
Conc: 1.01 ug/ml

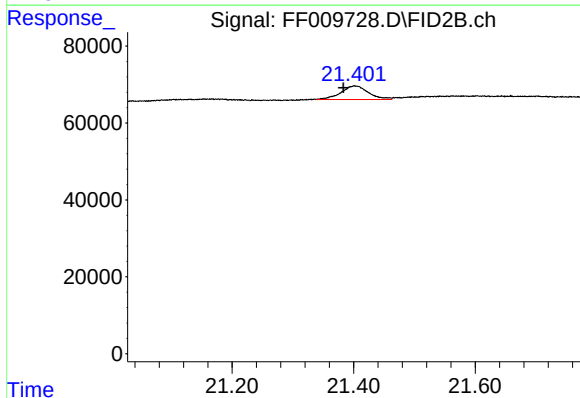

#18 N-TETRACONTANE

R.T.: 21.400 min
Delta R.T.: 0.017 min
Response: 110032
Conc: 1.21 ug/ml