

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009722.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 11:44
Operator : AJ\MA
Sample : N1177-02 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-08-20220117-19.5-20.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File: autoint1.e
Quant Time: Jan 20 23:47:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.443	280678	2.148 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012022\
Data File : FF009722.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2022 11:44
Operator : AJ\MA
Sample : N1177-02 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SP25-08-20220117-19.5-20.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File: autoint1.e
Quant Time: Jan 20 23:47:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

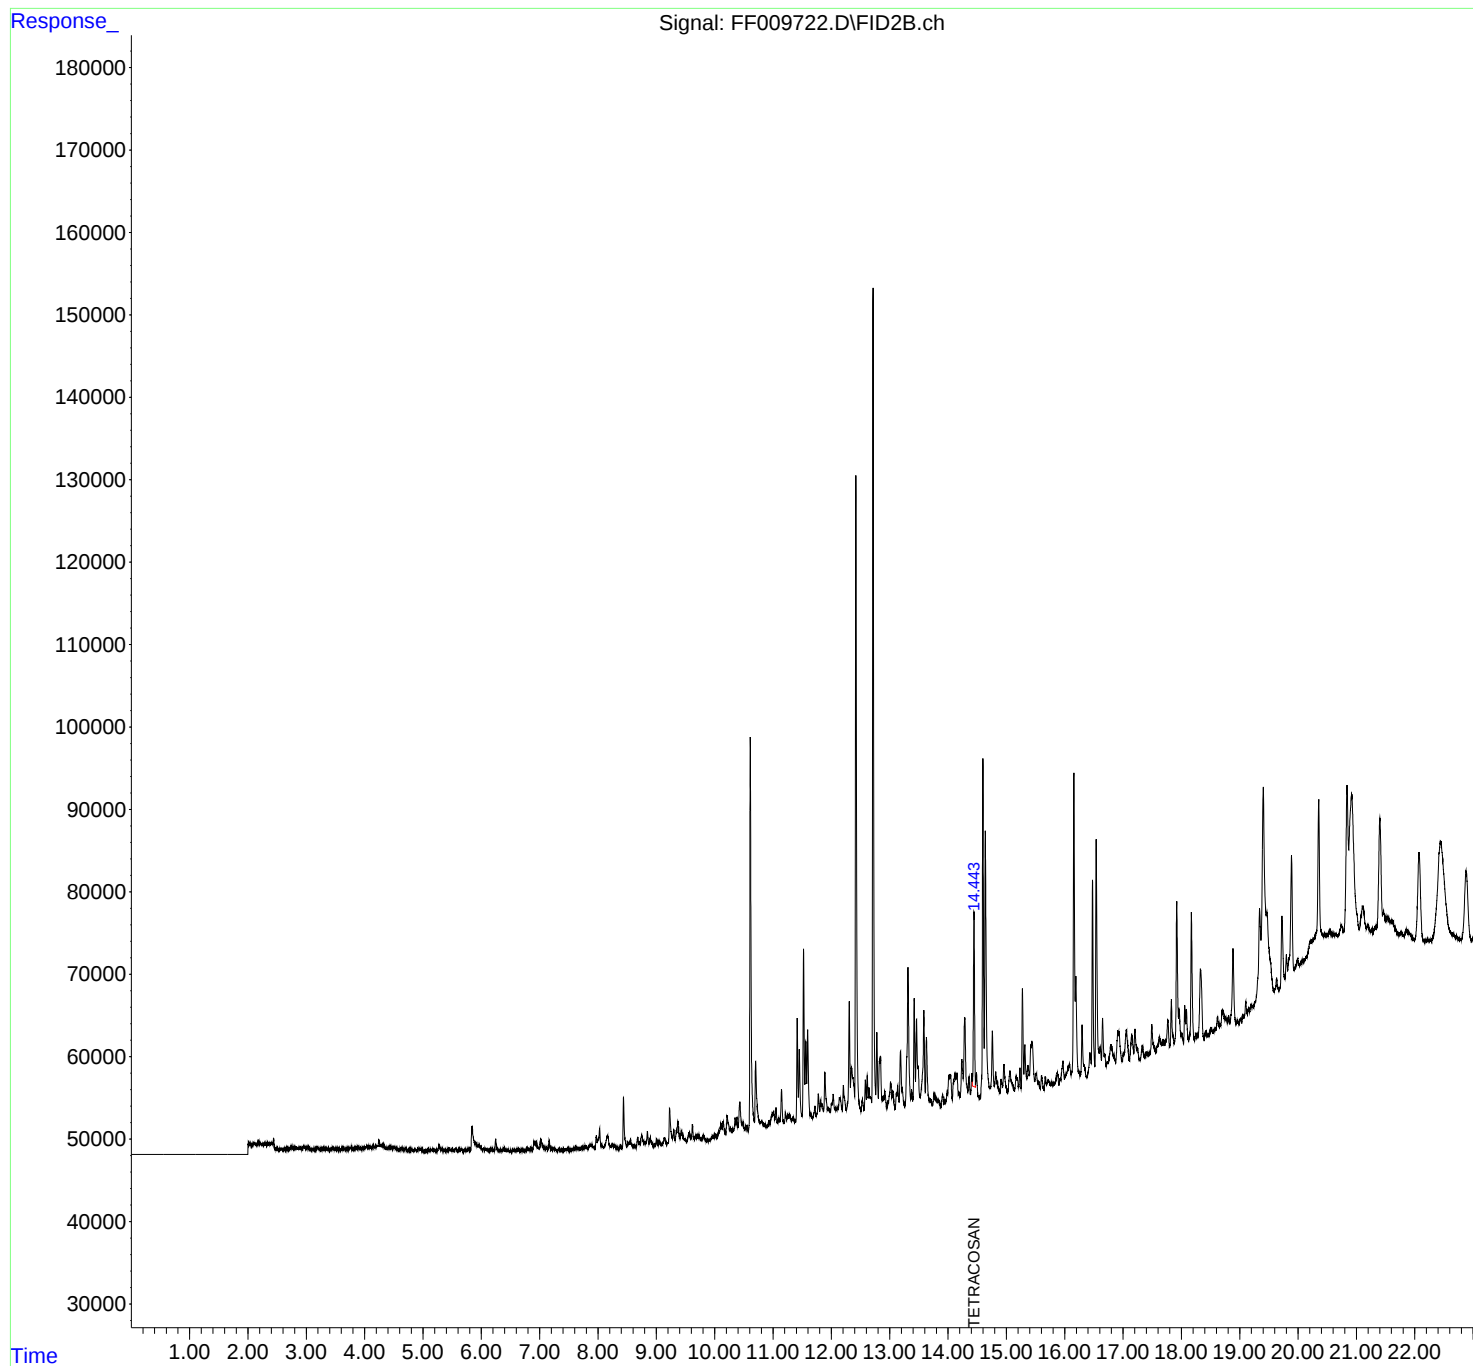

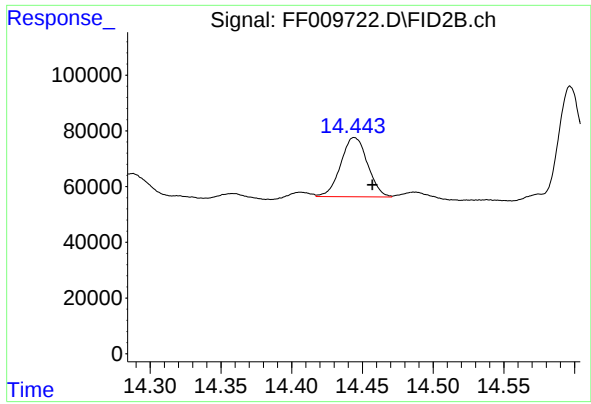

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.443 min
Delta R.T.: -0.014 min
Response: 280678
Conc: 2.15 ug/ml

Instrument :

FID_F

ClientSampleId :

SP25-08-20220117-19.5-20.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 01/21/2022

Supervised By :Ankita Jodhani 01/21/2022