

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011890.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 15:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.046	2141869	13.552 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.943	72838	0.450 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011890.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 15:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

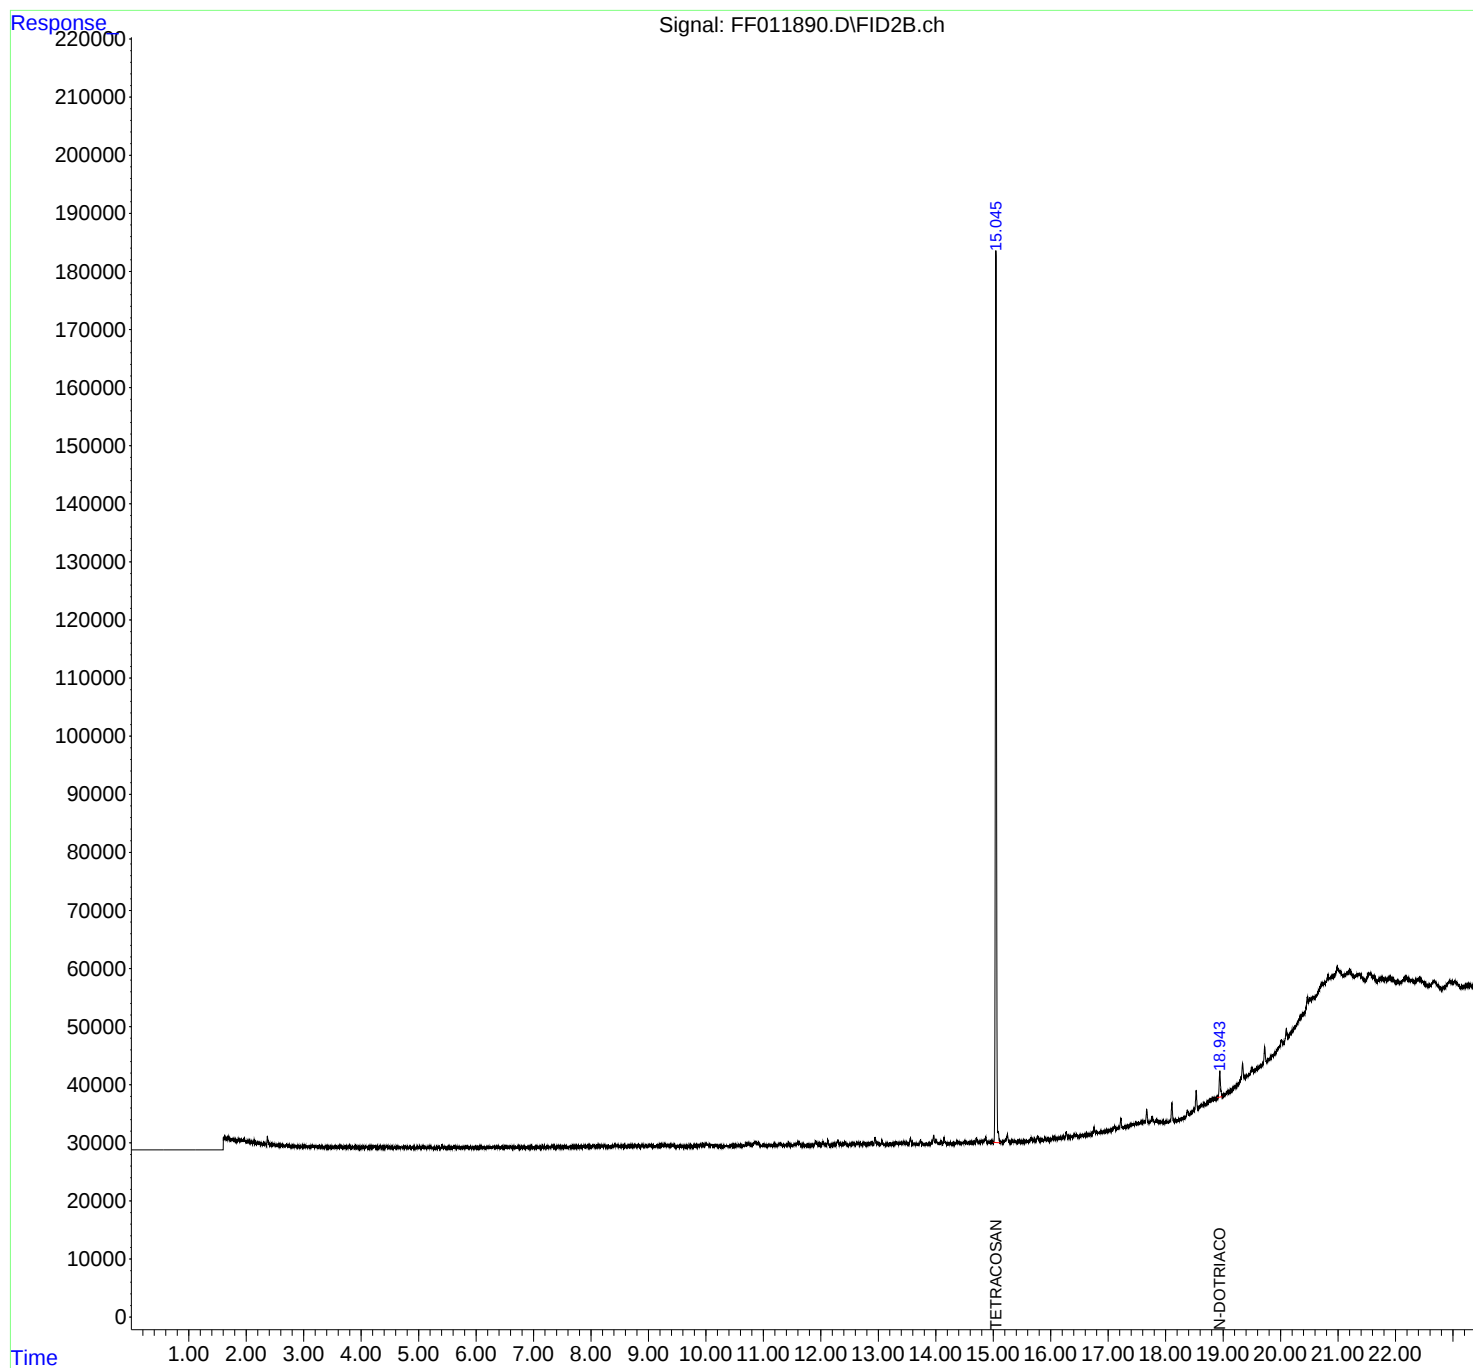


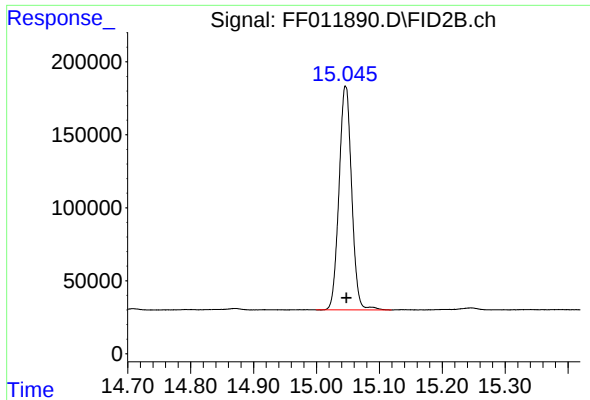

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: -0.002 min
Response: 2141869
Conc: 13.55 ug/ml

Instrument :
FID_F
ClientSampleId :

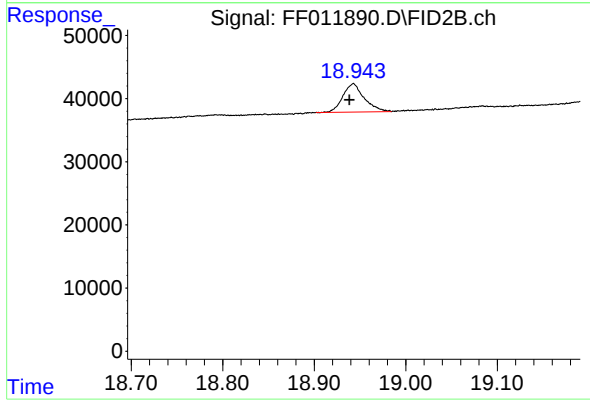

#14 N-DOTRIACONTANE

R.T.: 18.943 min
Delta R.T.: 0.005 min
Response: 72838
Conc: 0.45 ug/ml