

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011892.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 15:58
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.769	3453041	21.452 ug/ml
12)	N-OCTACOSANE	17.225	3482241	20.130 ug/ml
13)	N-TRIACONTANE	18.110	76032	0.454 ug/ml
14)	N-DOTRIACONTANE	18.943	103588	0.640 ug/ml
15)	N-TETRATRIACONTANE	19.725	83012	0.557 ug/ml
16)	N-HEXATRIACONTANE	20.467	40160	0.300 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011892.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 15:58
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

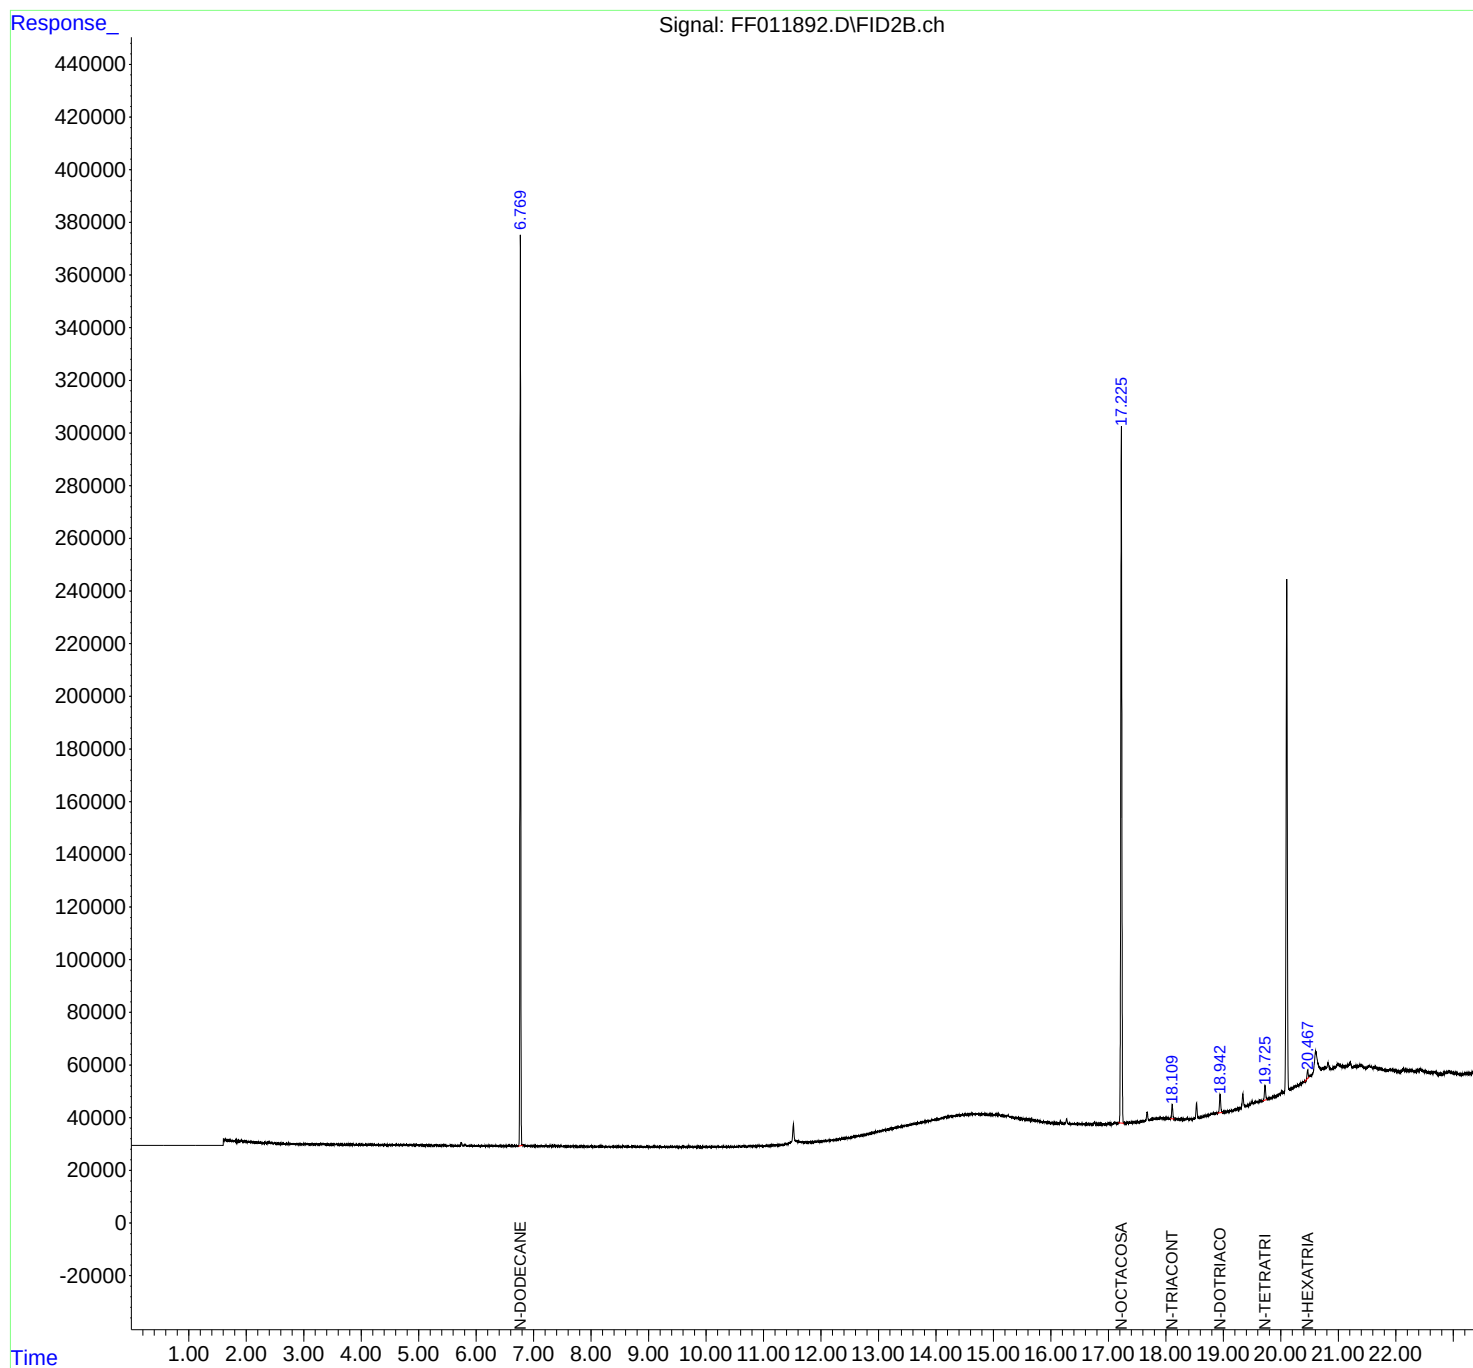


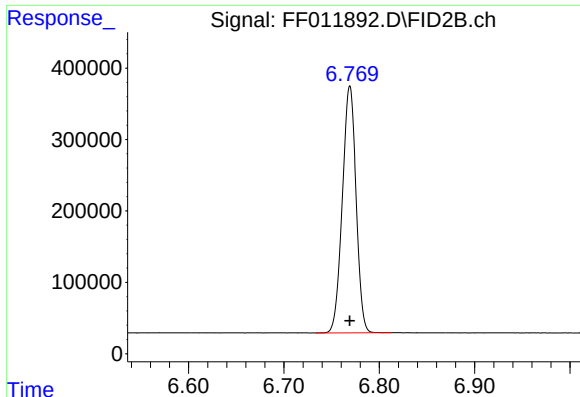

#3 N-DODECANE


R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 3453041
Conc: 21.45 ug/ml

Instrument :
FID_F
ClientSampleId :

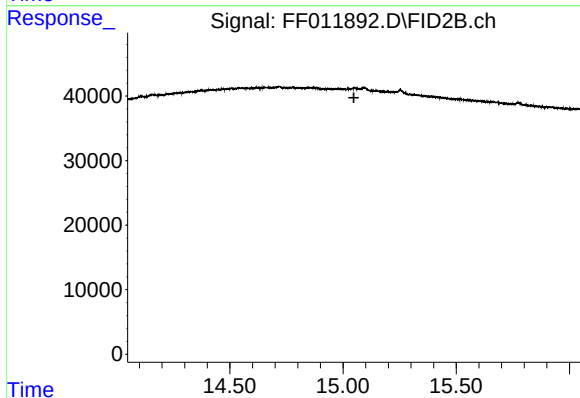


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.048 min
Response: 0
Conc: N.D.

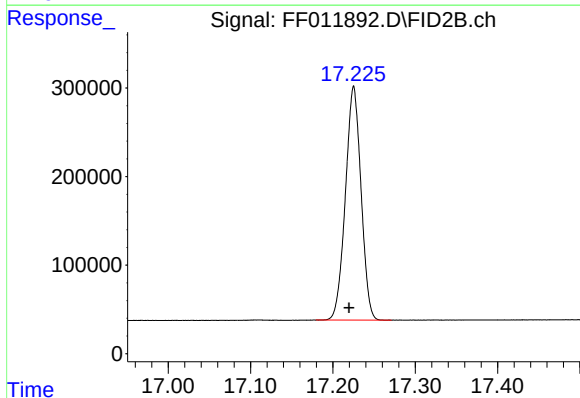


#12 N-OCTACOSANE

R.T.: 17.225 min
Delta R.T.: 0.005 min
Response: 3482241
Conc: 20.13 ug/ml

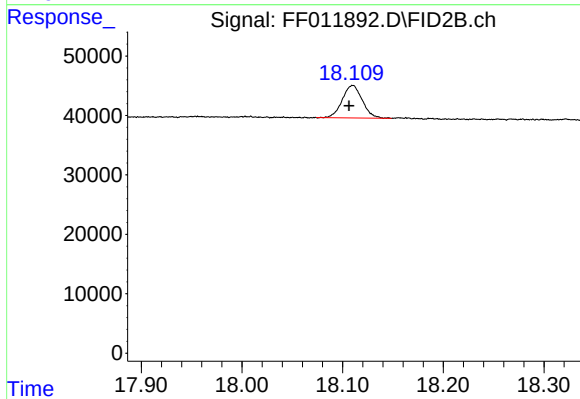

#13 N-TRIACONTANE


R.T.: 18.110 min
Delta R.T.: 0.003 min
Response: 76032
Conc: 0.45 ug/ml

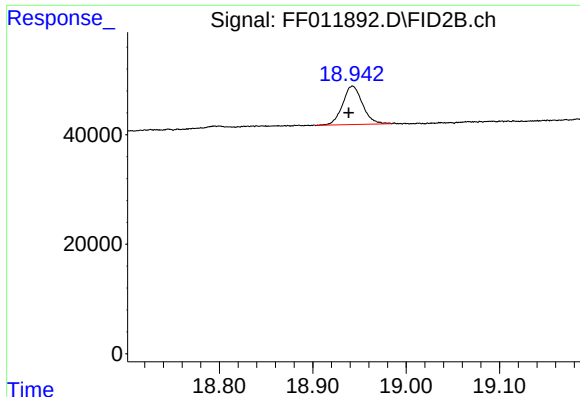

#14 N-DOTRIACONTANE


R.T.: 18.943 min
Delta R.T.: 0.004 min
Response: 103588
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

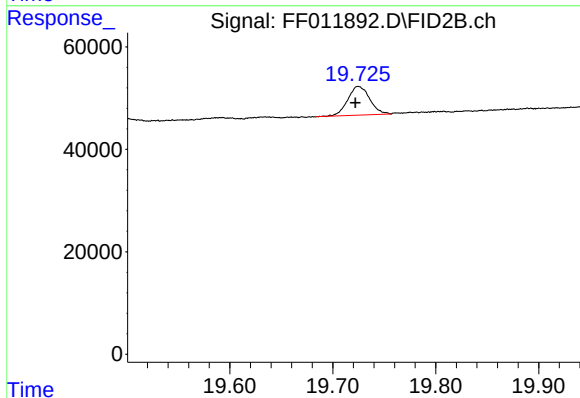

#15 N-TETRATRIACONTANE

R.T.: 19.725 min
Delta R.T.: 0.003 min
Response: 83012
Conc: 0.56 ug/ml

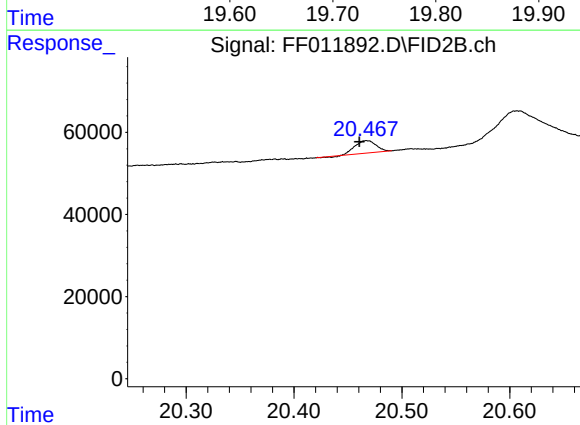

#16 N-HEXATRIACONTANE

R.T.: 20.467 min
Delta R.T.: 0.007 min
Response: 40160
Conc: 0.30 ug/ml