

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
 Data File : FF011895.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2023 17:29
 Operator : YP\AJ
 Sample : 01232-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 03:04:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.049	1637387	10.360 ug/ml
Target Compounds			
7) N-EICOSANE	12.890f	63770	0.359 ug/ml
10) N-TETRACOSANE	15.250	110232	0.611 ug/ml
11) N-HEXACOSANE	16.273	85870	0.482 ug/ml
12) N-OCTACOSANE	17.222	77340	0.447 ug/ml
13) N-TRIACONTANE	18.110	103147	0.616 ug/ml
14) N-DOTRIACONTANE	18.942	112174	0.693 ug/ml
15) N-TETRATRIACONTANE	19.725	52405	0.351 ug/ml
16) N-HEXATRIACONTANE	20.464	56058	0.418 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011895.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 17:29
Operator : YP\AJ
Sample : 01232-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:04:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

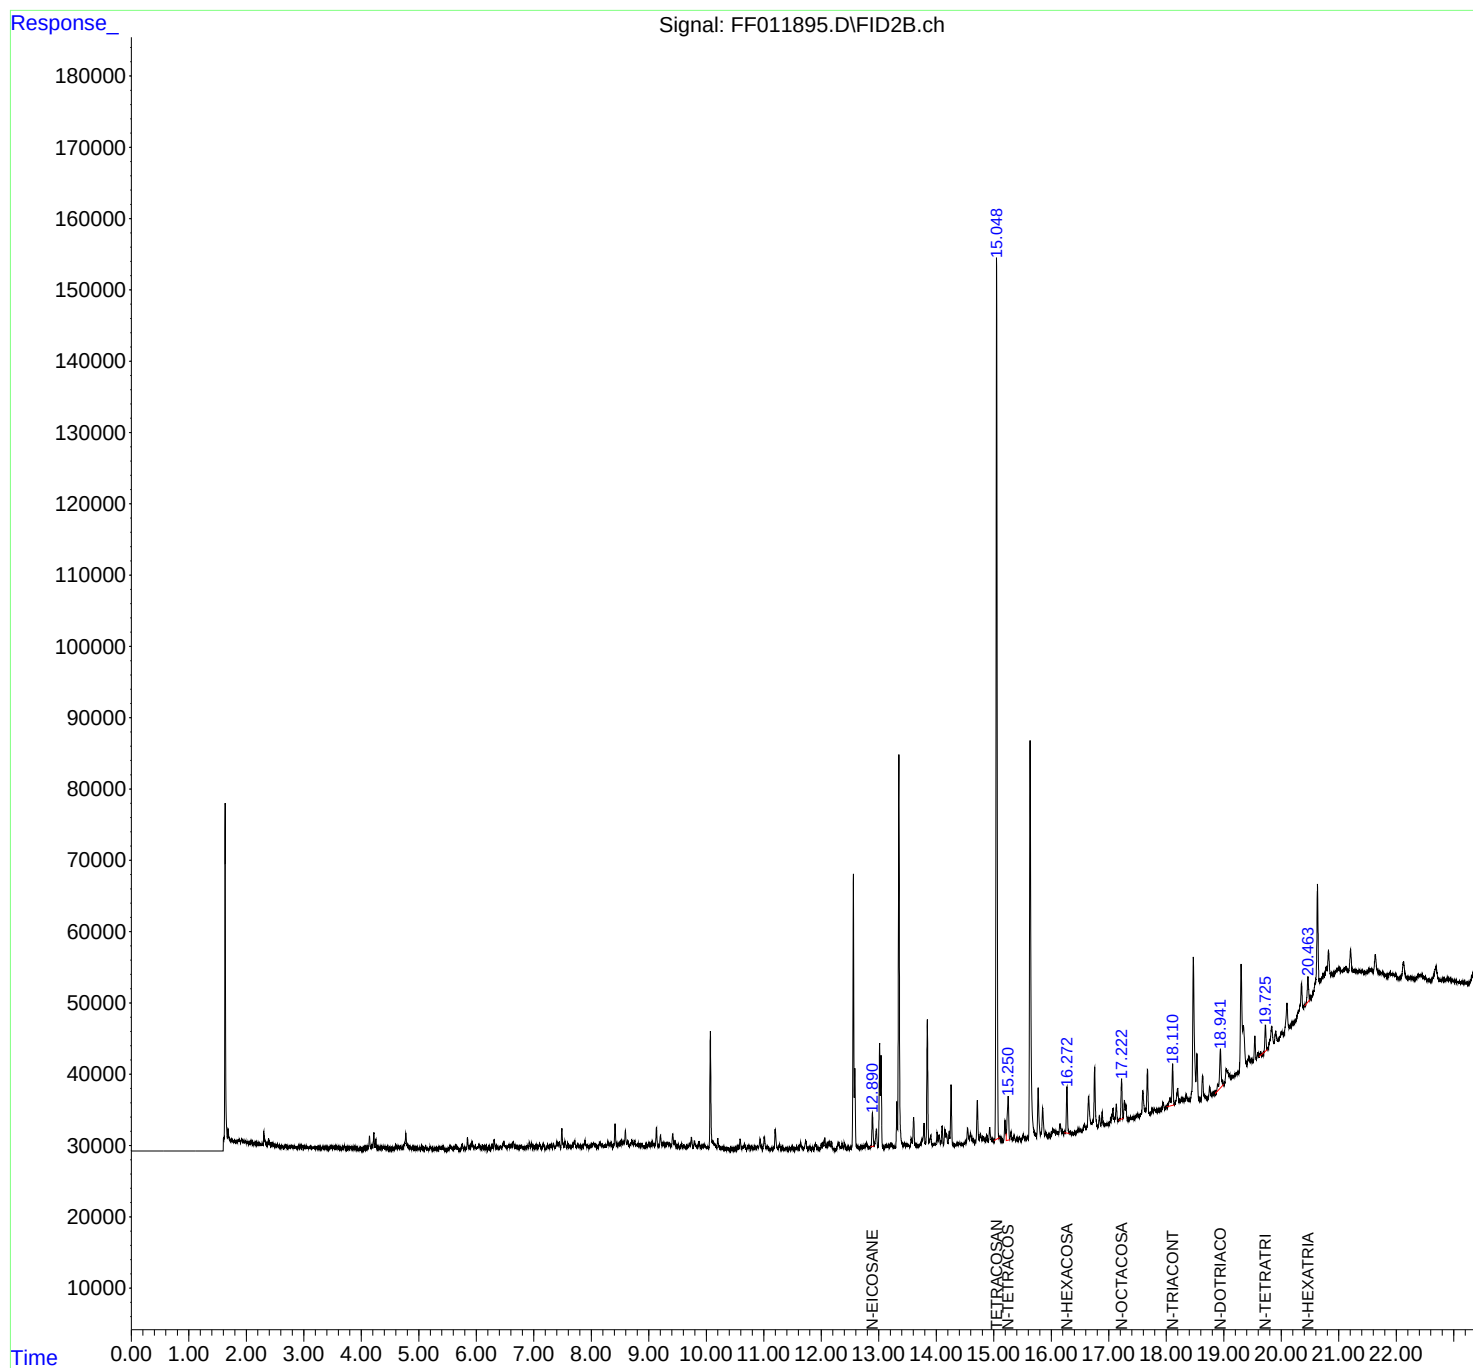


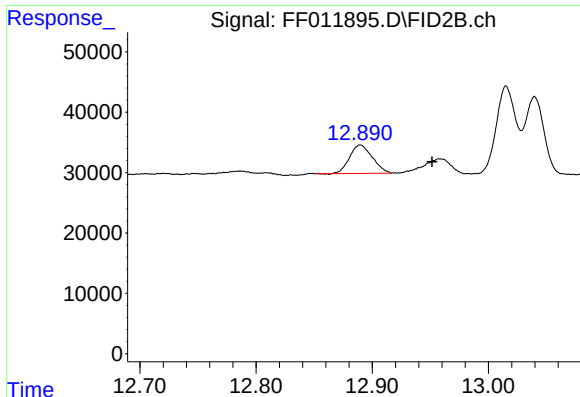

#7 N-EICOSANE


R.T.: 12.890 min
Delta R.T.: -0.062 min
Response: 63770
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :

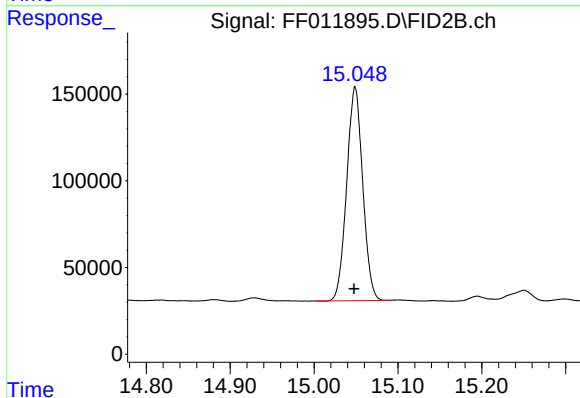


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.049 min
Delta R.T.: 0.001 min
Response: 1637387
Conc: 10.36 ug/ml

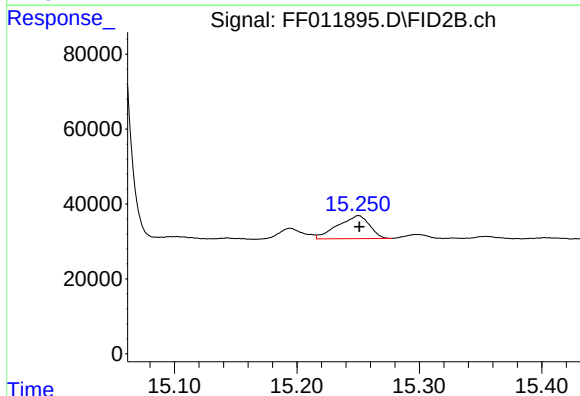


#10 N-TETRACOSANE

R.T.: 15.250 min
Delta R.T.: 0.000 min
Response: 110232
Conc: 0.61 ug/ml

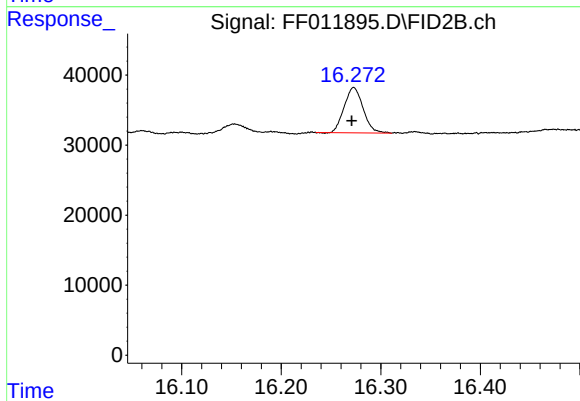

#11 N-HEXACOSANE


R.T.: 16.273 min
Delta R.T.: 0.002 min
Response: 85870
Conc: 0.48 ug/ml

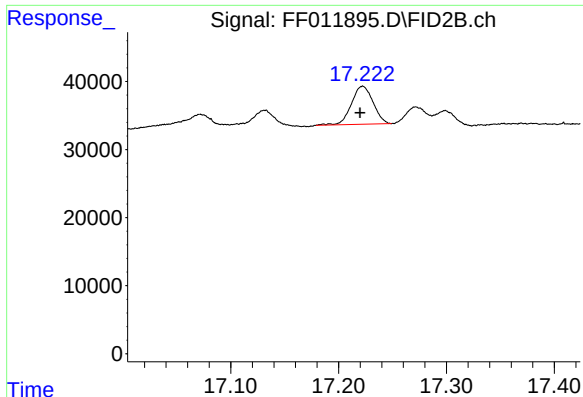

#12 N-OCTACOSANE


R.T.: 17.222 min
Delta R.T.: 0.003 min
Response: 77340
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :

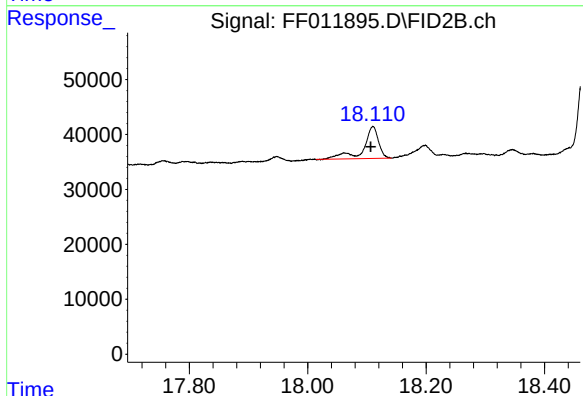


#13 N-TRIACONTANE

R.T.: 18.110 min
Delta R.T.: 0.004 min
Response: 103147
Conc: 0.62 ug/ml

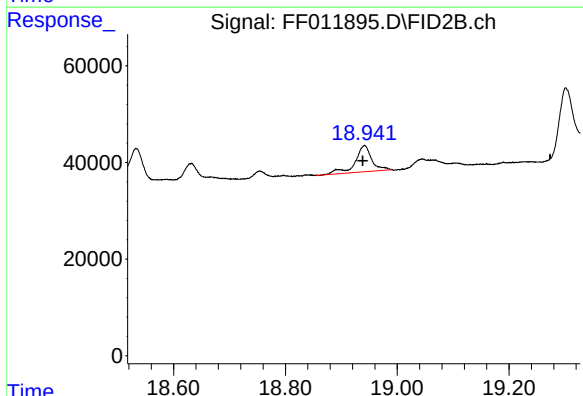


#14 N-DOTRIACONTANE

R.T.: 18.942 min
Delta R.T.: 0.003 min
Response: 112174
Conc: 0.69 ug/ml

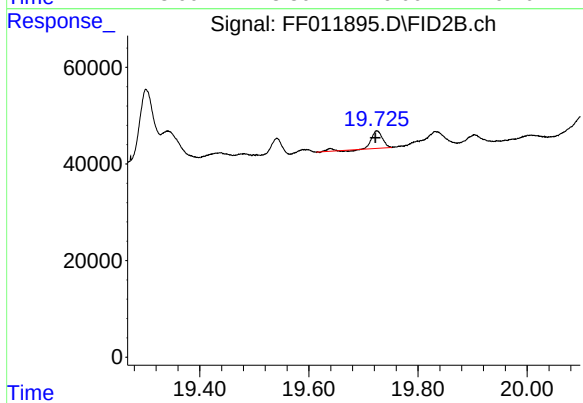

#15 N-TETRATRIACONTANE

R.T.: 19.725 min
Delta R.T.: 0.003 min
Response: 52405
Conc: 0.35 ug/ml

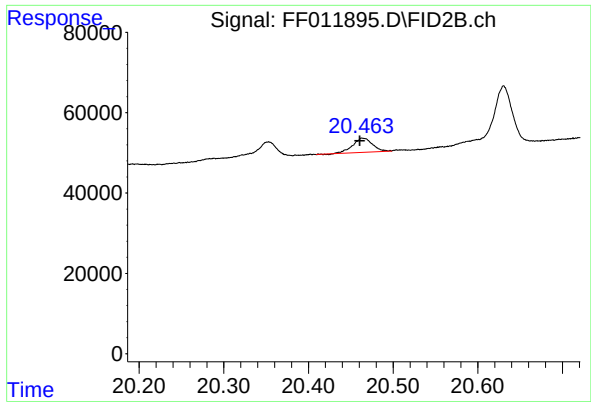

#16 N-HEXATRIACONTANE

R.T.: 20.464 min
Delta R.T.: 0.003 min
Response: 56058
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :