

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011899.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 19:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:04:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.049	2154647	13.632 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.108	58824	0.351 ug/ml
14) N-DOTRIACONTANE	18.940	79125	0.489 ug/ml
15) N-TETRATRIACONTANE	19.724	52799	0.354 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011899.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 19:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:04:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

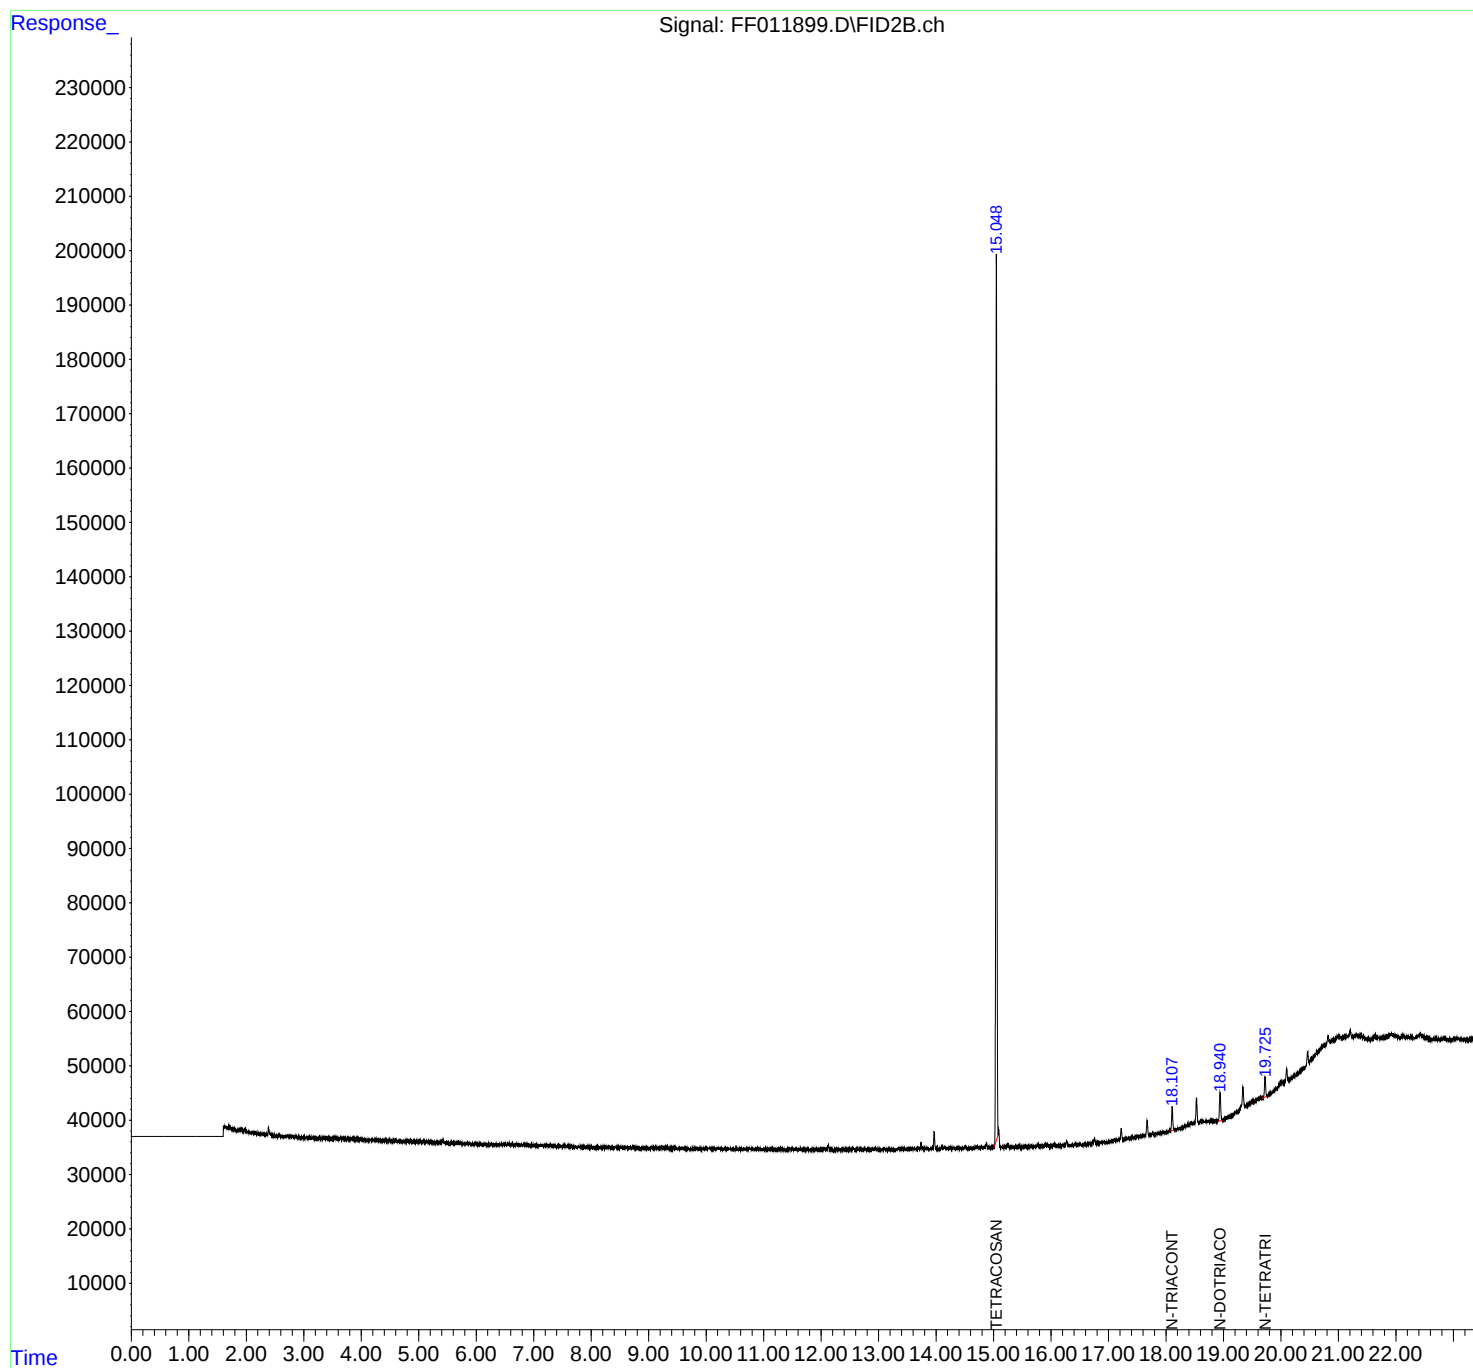


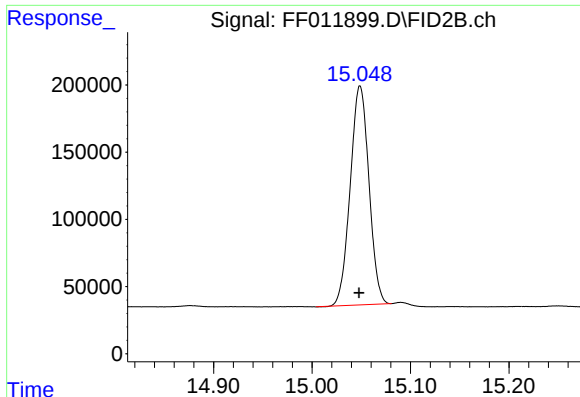

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.049 min
Delta R.T.: 0.000 min
Response: 2154647
Conc: 13.63 ug/ml

Instrument :
FID_F
ClientSampleId :

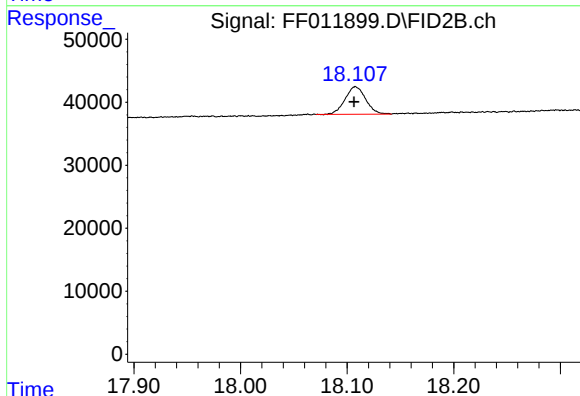


#13 N-TRIACONTANE

R.T.: 18.108 min
Delta R.T.: 0.001 min
Response: 58824
Conc: 0.35 ug/ml

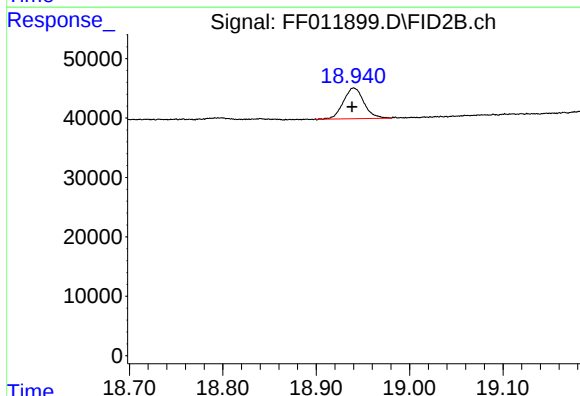

#14 N-DOTRIACONTANE

R.T.: 18.940 min
Delta R.T.: 0.002 min
Response: 79125
Conc: 0.49 ug/ml

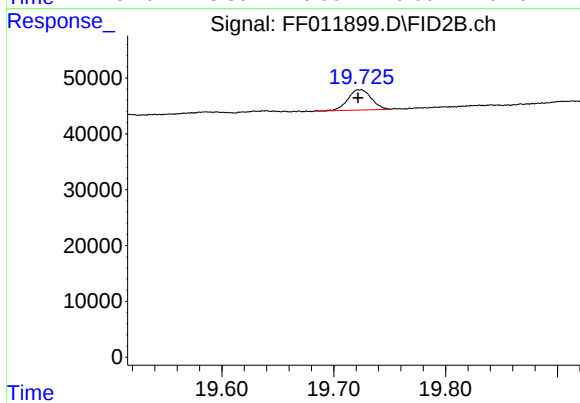

#15 N-TETRATRIACONTANE

R.T.: 19.724 min
Delta R.T.: 0.002 min
Response: 52799
Conc: 0.35 ug/ml