

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
 Data File : FF011897.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2023 18:28
 Operator : YP\AJ
 Sample : 01232-03MSD
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-17MSD

Integration File: autoint1.e
 Quant Time: Jan 21 03:04:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	2336745	14.785 ug/ml
Target Compounds			
2) N-DECANE	4.607	2774996	17.625 ug/ml
3) N-DODECANE	6.769	3108080	19.309 ug/ml
4) N-TETRADECANE	8.595	3403062	20.687 ug/ml
5) N-HEXADECANE	10.201	3556999	20.857 ug/ml
6) N-OCTADECANE	11.643	3662826	20.738 ug/ml
7) N-EICOSANE	12.953	3639958	20.500 ug/ml
8) N-DOCOSANE	14.151	3597243	20.101 ug/ml
10) N-TETRACOSANE	15.254	3609512	20.005 ug/ml
11) N-HEXACOSANE	16.275	3498777	19.622 ug/ml
12) N-OCTACOSANE	17.225	3334042	19.274 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011897.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 18:28
Operator : YP\AJ
Sample : 01232-03MSD
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-17MSD

Integration File: autoint1.e
Quant Time: Jan 21 03:04:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

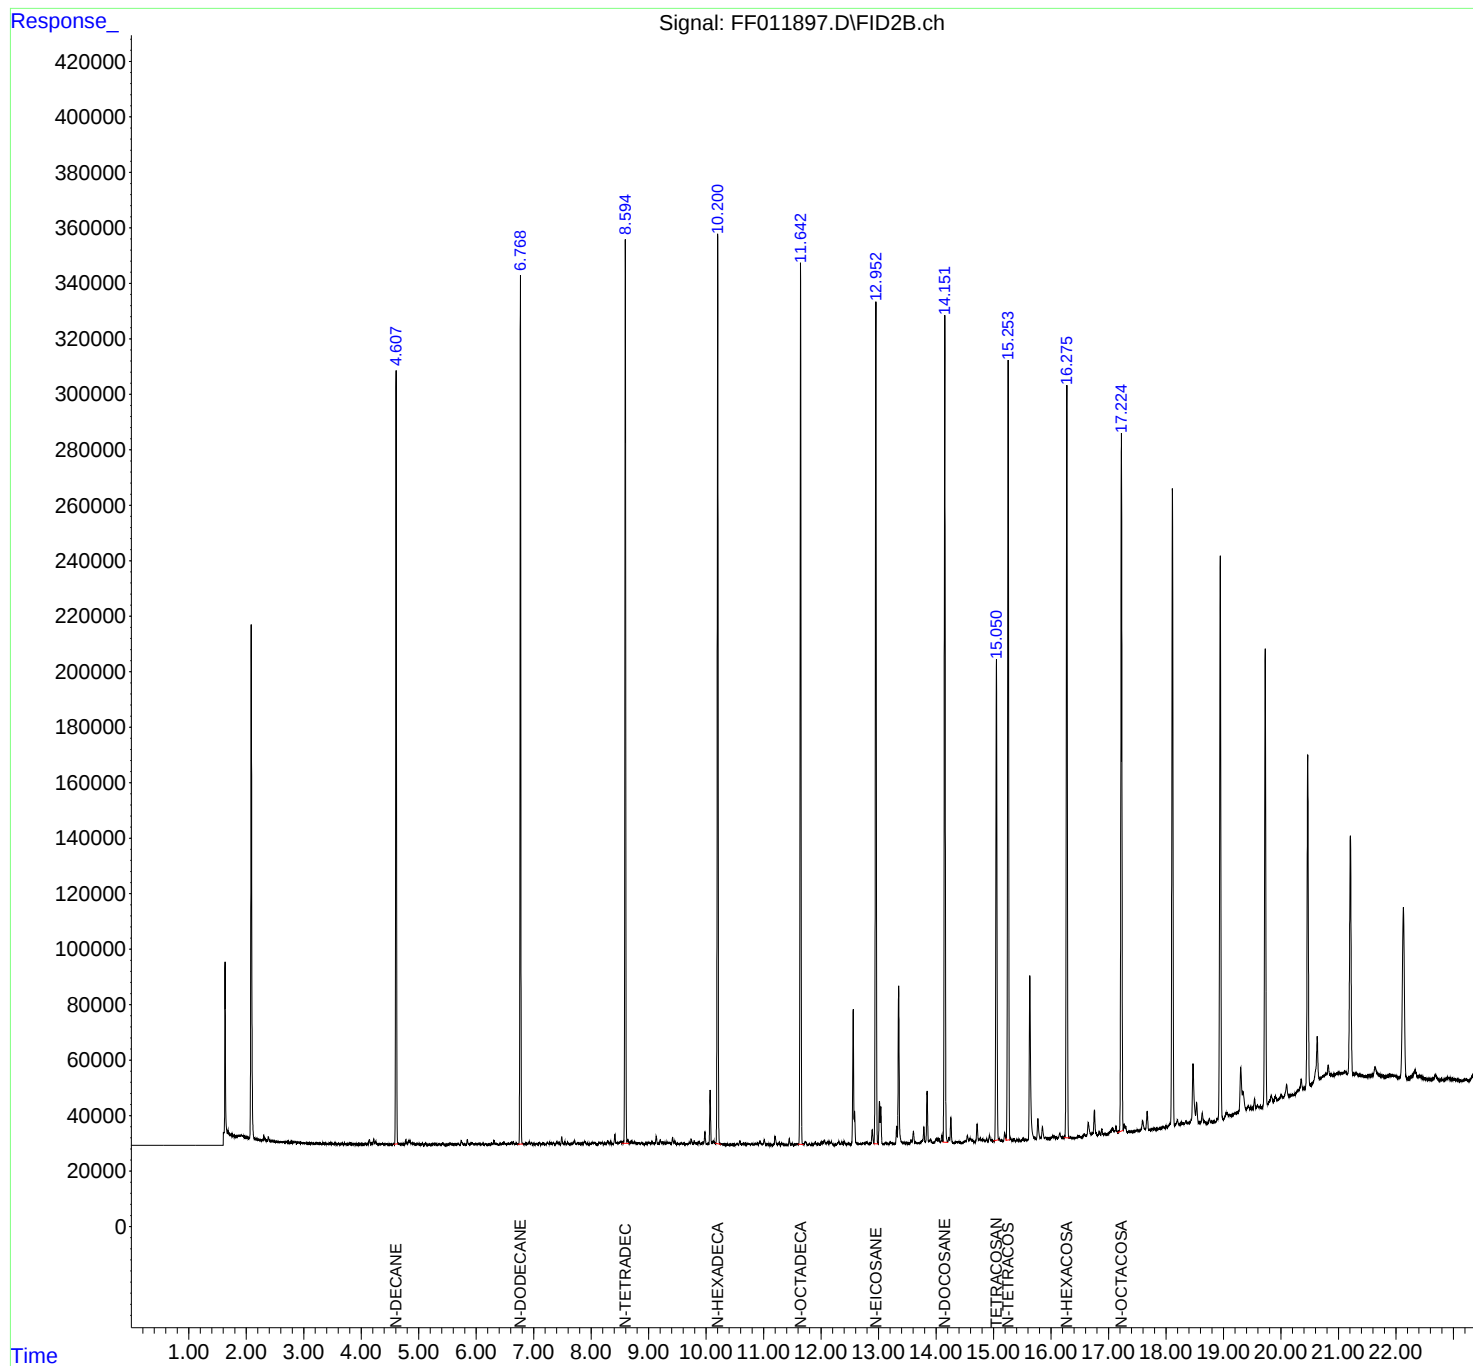


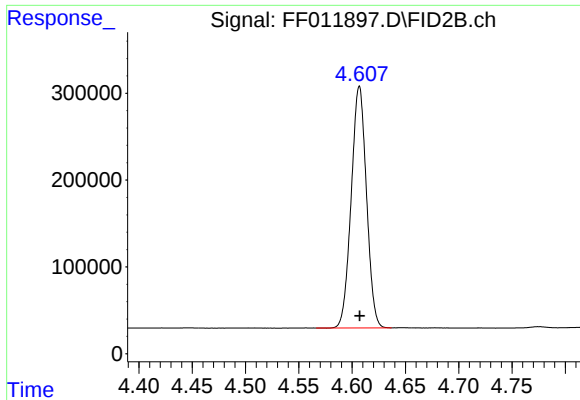

#2 N-DECANE


R.T.: 4.607 min
Delta R.T.: 0.000 min
Response: 2774996
Conc: 17.63 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

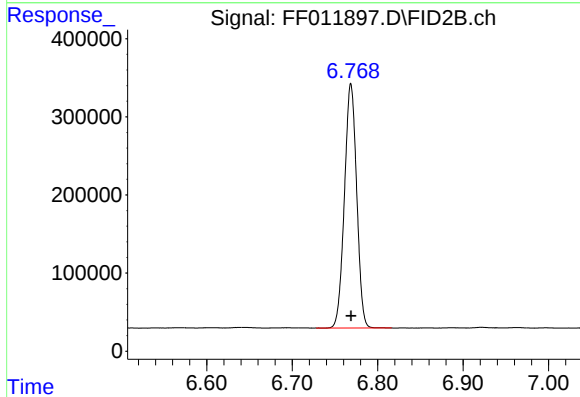


#3 N-DODECANE

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 3108080
Conc: 19.31 ug/ml

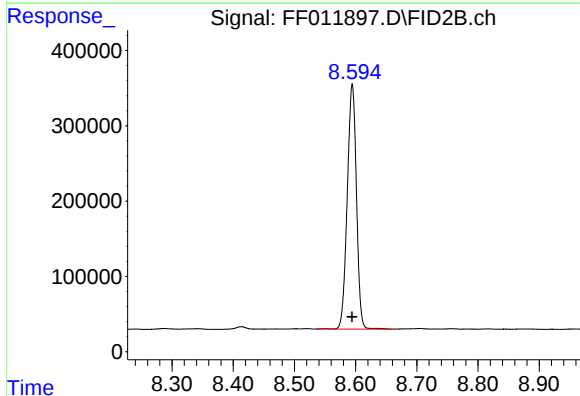


#4 N-TETRADECANE

R.T.: 8.595 min
Delta R.T.: 0.000 min
Response: 3403062
Conc: 20.69 ug/ml

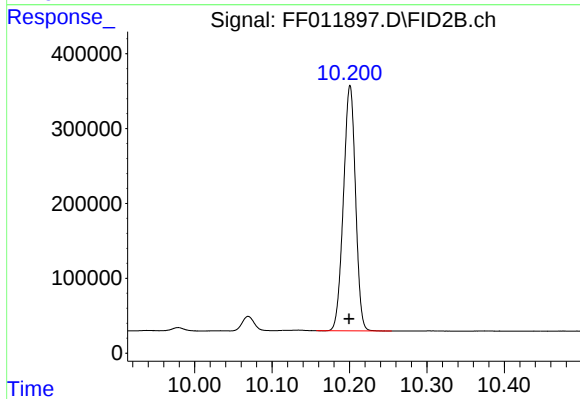

#5 N-HEXADECANE


R.T.: 10.201 min
Delta R.T.: 0.001 min
Response: 3556999
Conc: 20.86 ug/ml

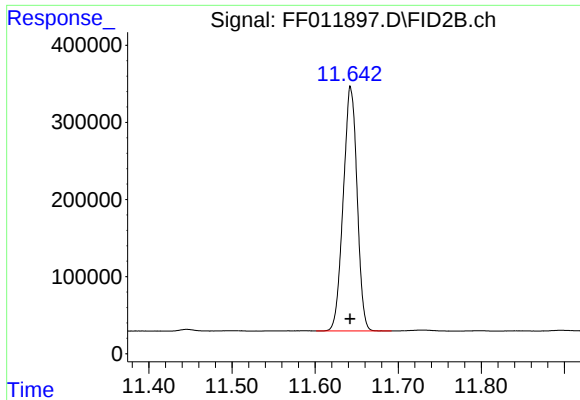

#6 N-OCTADECANE


R.T.: 11.643 min
Delta R.T.: 0.000 min
Response: 3662826
Conc: 20.74 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

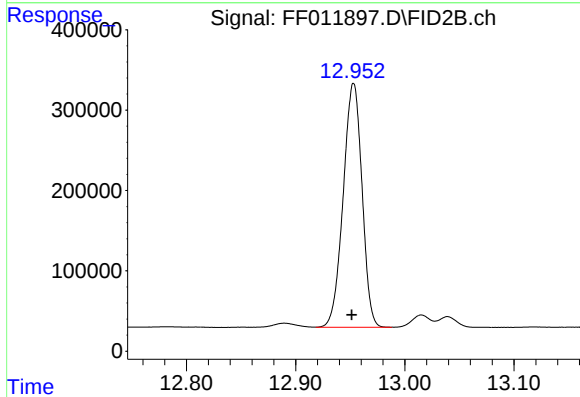


#7 N-EICOSANE

R.T.: 12.953 min
Delta R.T.: 0.002 min
Response: 3639958
Conc: 20.50 ug/ml

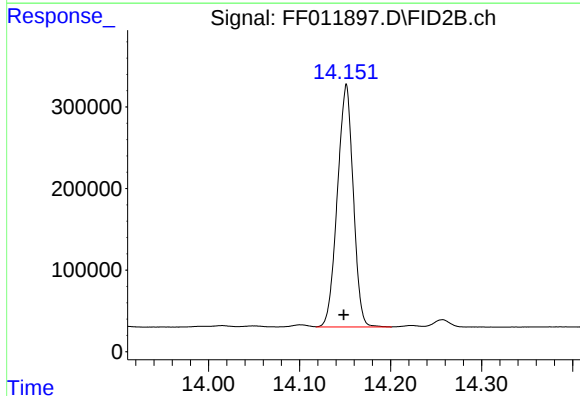


#8 N-DOCOSANE

R.T.: 14.151 min
Delta R.T.: 0.003 min
Response: 3597243
Conc: 20.10 ug/ml

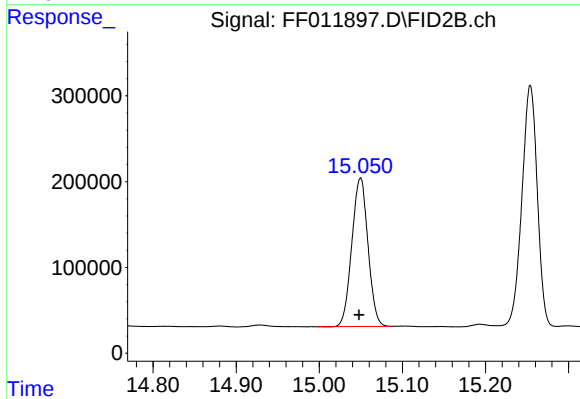

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.050 min
Delta R.T.: 0.002 min
Response: 2336745
Conc: 14.78 ug/ml

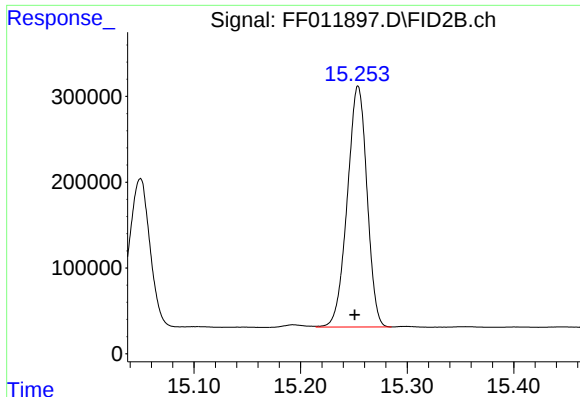

#10 N-TETRACOSANE


R.T.: 15.254 min
Delta R.T.: 0.003 min
Response: 3609512
Conc: 20.01 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

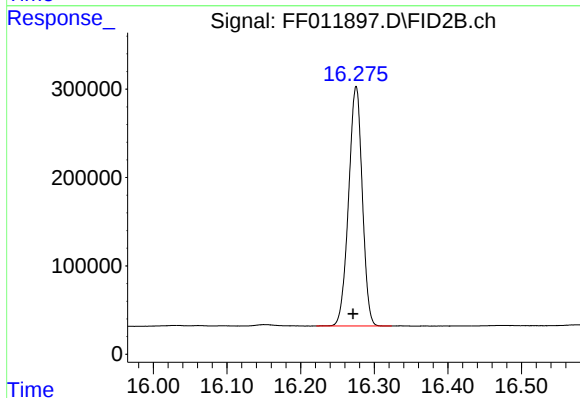

#11 N-HEXACOSANE

R.T.: 16.275 min
Delta R.T.: 0.004 min
Response: 3498777
Conc: 19.62 ug/ml

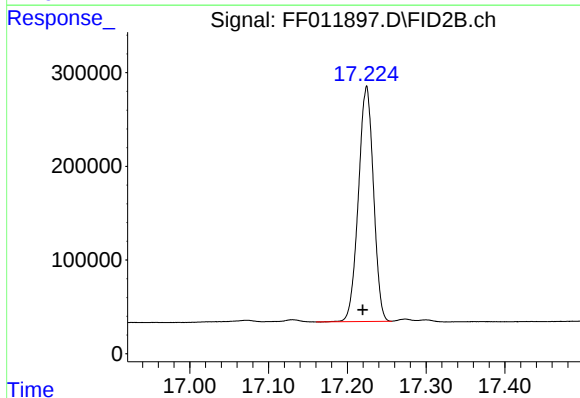

#12 N-OCTACOSANE

R.T.: 17.225 min
Delta R.T.: 0.005 min
Response: 3334042
Conc: 19.27 ug/ml