

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
 Data File : FF011900.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jan 2023 20:56
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 21 03:05:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	8188278	51.807 ug/ml
Target Compounds			
2) N-DECANE	4.609	8487544	53.908 ug/ml
3) N-DODECANE	6.772	8788903	54.601 ug/ml
4) N-TETRADECANE	8.598	9026461	54.872 ug/ml
5) N-HEXADECANE	10.205	9326409	54.686 ug/ml
6) N-OCTADECANE	11.647	9564876	54.153 ug/ml
7) N-EICOSANE	12.957	9447248	53.205 ug/ml
8) N-DOCOSANE	14.155	9349999	52.247 ug/ml
10) N-TETRACOSANE	15.258	9234864	51.183 ug/ml
11) N-HEXACOSANE	16.278	8976605	50.342 ug/ml
12) N-OCTACOSANE	17.227	8641329	49.954 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012023\
Data File : FF011900.D
Signal(s) : FID2B.ch
Acq On : 20 Jan 2023 20:56
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Jan 21 03:05:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

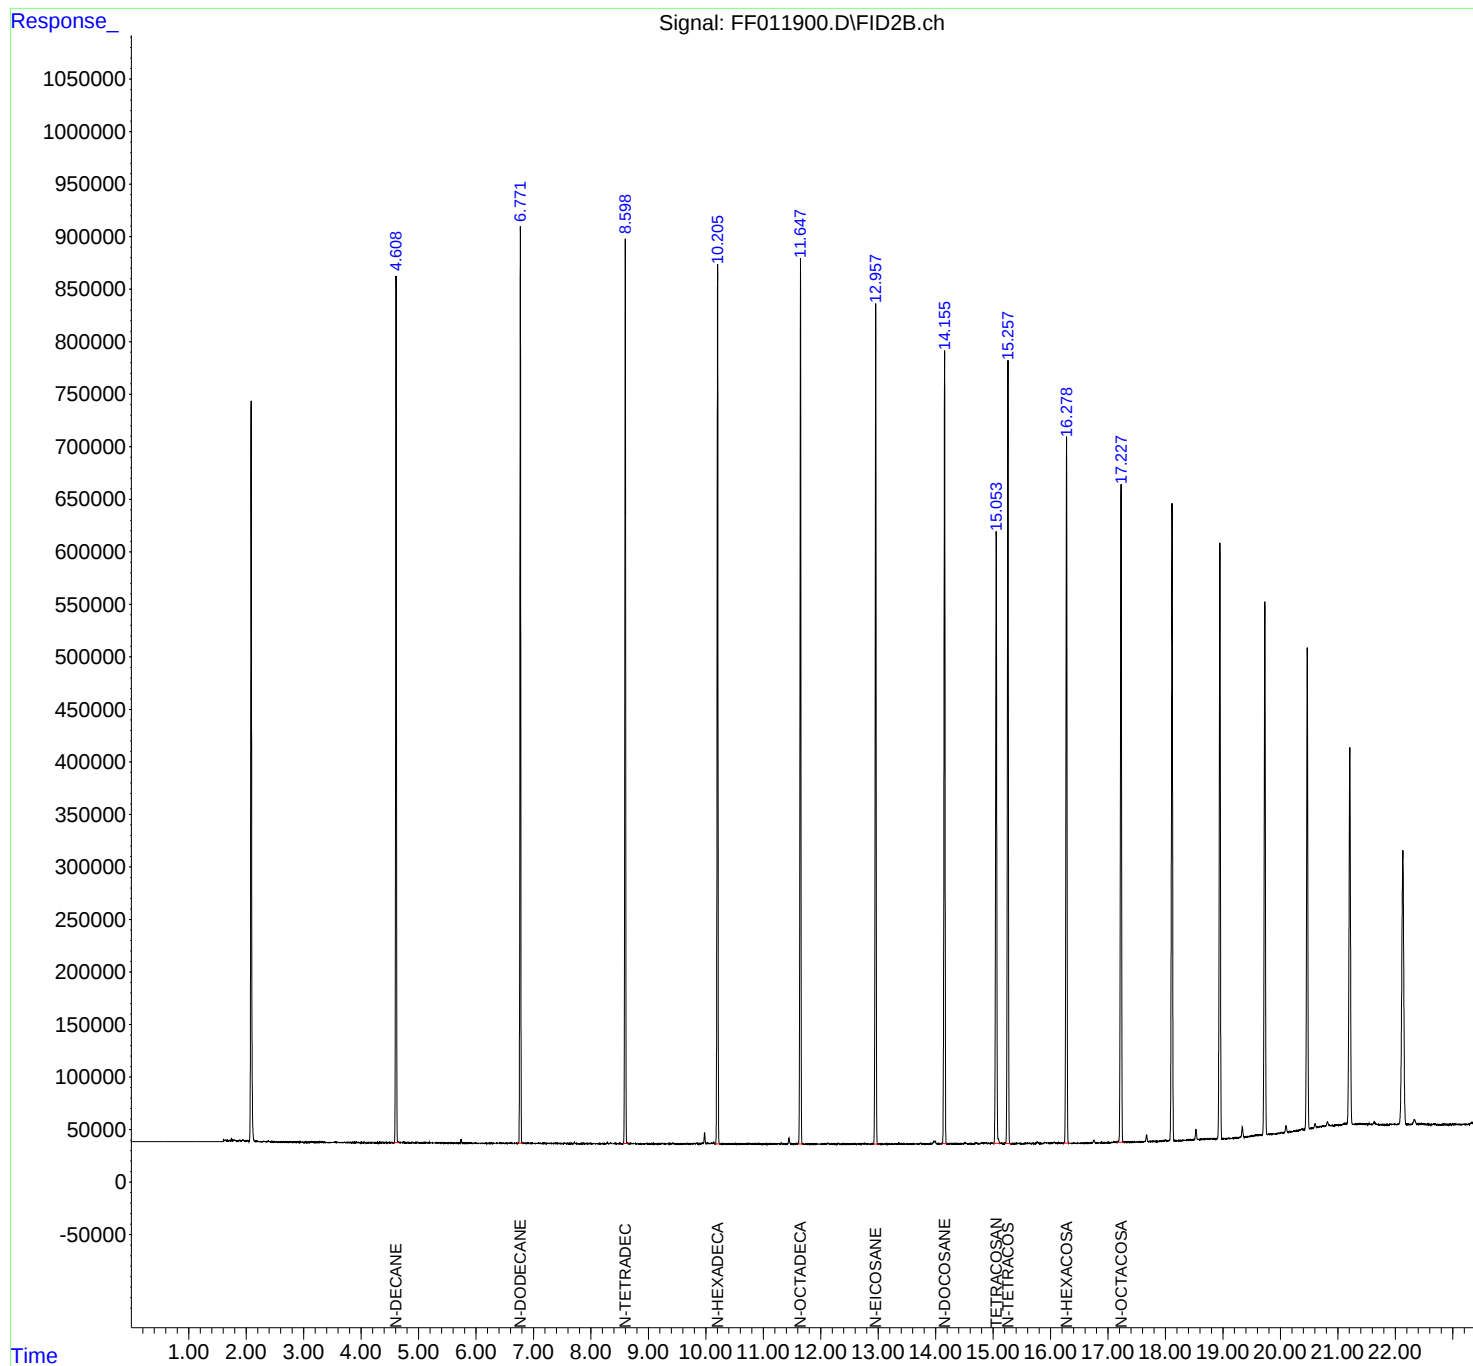


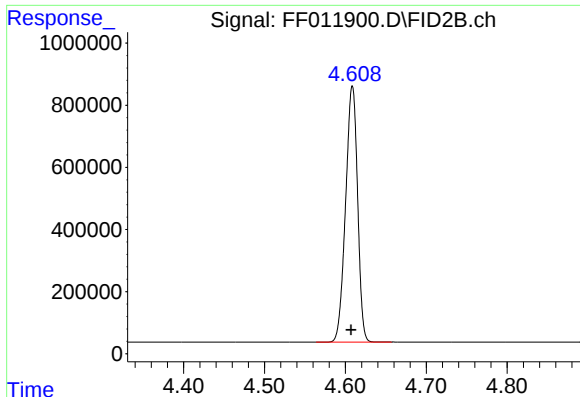

#2 N-DECANE


R.T.: 4.609 min
Delta R.T.: 0.001 min
Response: 8487544
Conc: 53.91 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

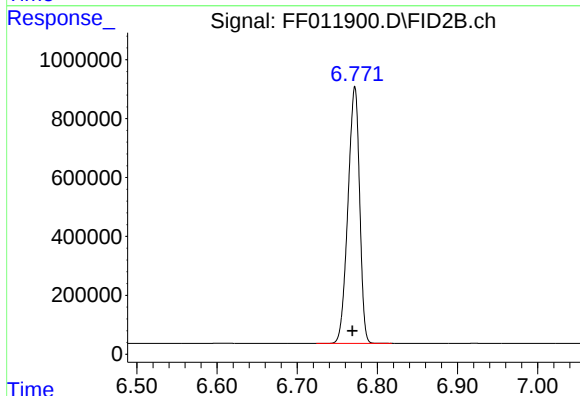


#3 N-DODECANE

R.T.: 6.772 min
Delta R.T.: 0.003 min
Response: 8788903
Conc: 54.60 ug/ml

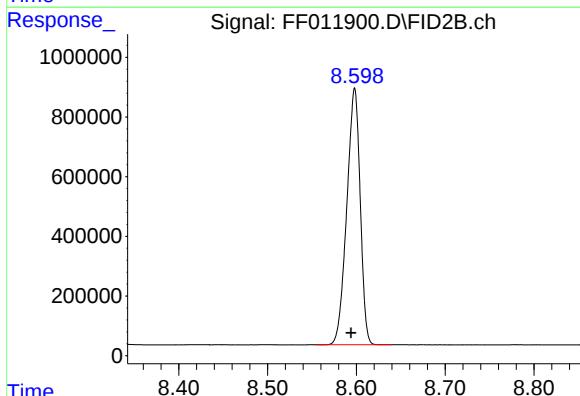


#4 N-TETRADECANE

R.T.: 8.598 min
Delta R.T.: 0.004 min
Response: 9026461
Conc: 54.87 ug/ml

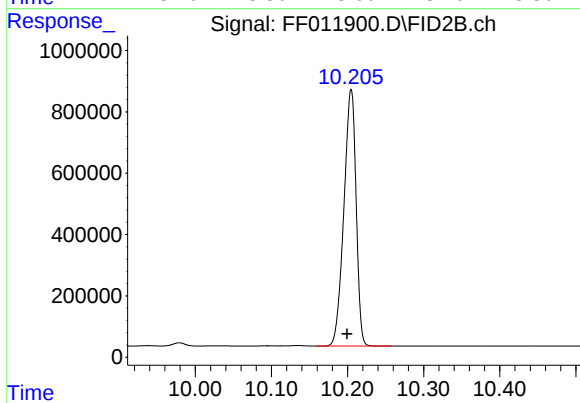

#5 N-HEXADECANE


R.T.: 10.205 min
Delta R.T.: 0.005 min
Response: 9326409
Conc: 54.69 ug/ml

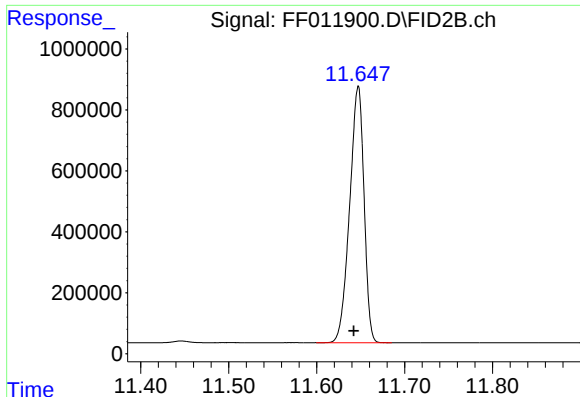

#6 N-OCTADECANE


R.T.: 11.647 min
Delta R.T.: 0.005 min
Response: 9564876
Conc: 54.15 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

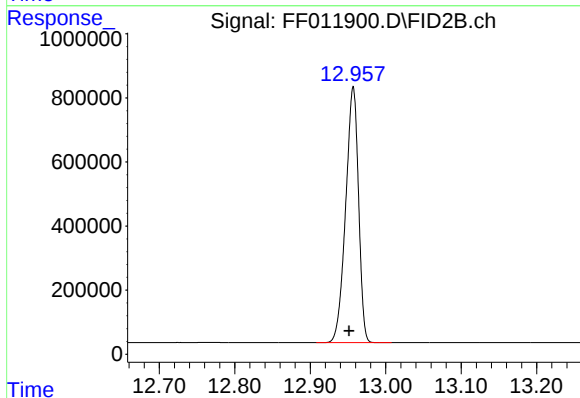


#7 N-EICOSANE

R.T.: 12.957 min
Delta R.T.: 0.006 min
Response: 9447248
Conc: 53.21 ug/ml

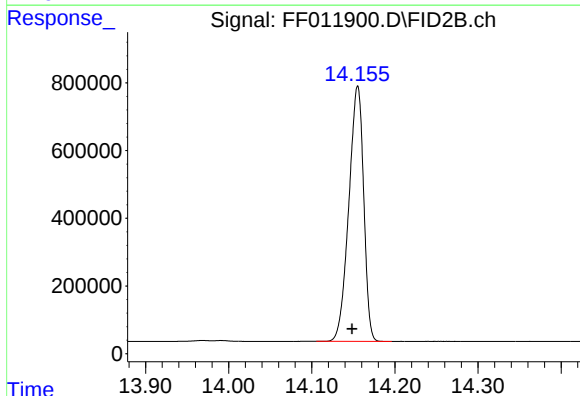


#8 N-DOCOSANE

R.T.: 14.155 min
Delta R.T.: 0.007 min
Response: 9349999
Conc: 52.25 ug/ml

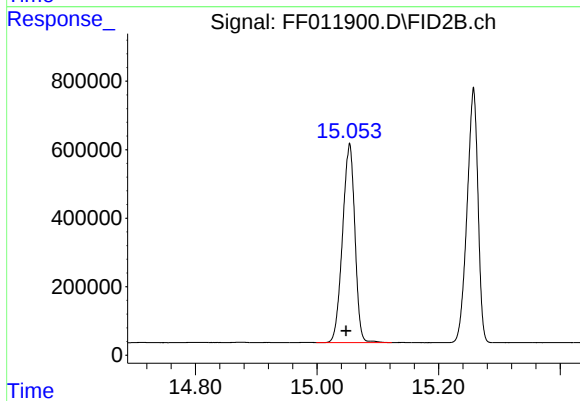

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: 0.006 min
Response: 8188278
Conc: 51.81 ug/ml

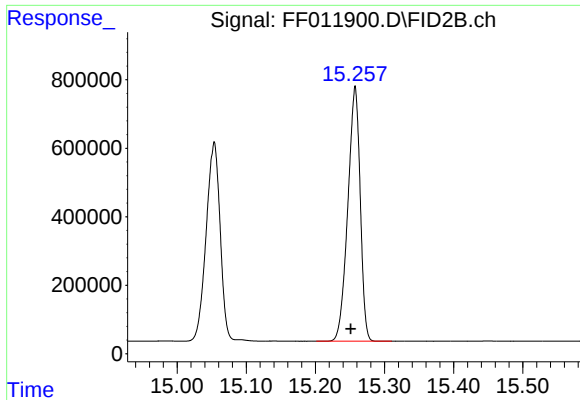

#10 N-TETRACOSANE


R.T.: 15.258 min
Delta R.T.: 0.007 min
Response: 9234864
Conc: 51.18 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

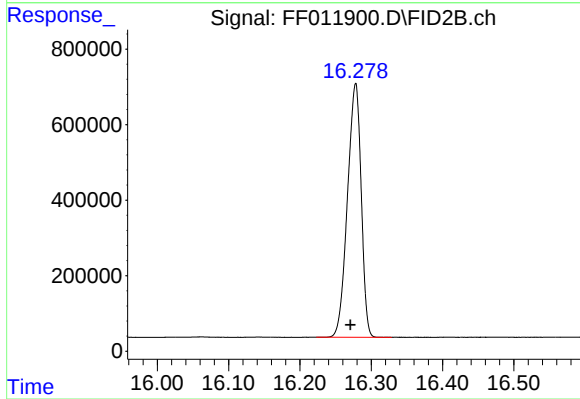

#11 N-HEXACOSANE

R.T.: 16.278 min
Delta R.T.: 0.007 min
Response: 8976605
Conc: 50.34 ug/ml

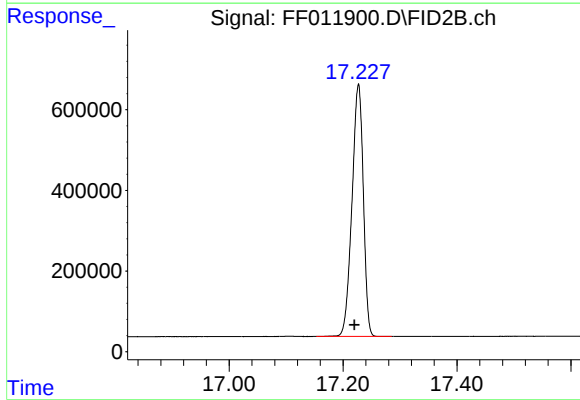

#12 N-OCTACOSANE

R.T.: 17.227 min
Delta R.T.: 0.007 min
Response: 8641329
Conc: 49.95 ug/ml