

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
 Data File : FF009749.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jan 2022 16:38
 Operator : AJ\MA
 Sample : N1208-04
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 22:59:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.238	127566	0.902 ug/ml
3) N-DODECANE	6.242	261536	1.828 ug/ml
4) N-TETRADECANE	8.026	756213	5.146 ug/ml
5) N-HEXADECANE	9.631	3224549	21.555 ug/ml
6) N-OCTADECANE	11.050	659191	4.276 ug/ml
10) N-TETRACOSANE	14.647	1452578	9.795 ug/ml
16) N-HEXATRIACONTANE	19.852	1202546	11.664 ug/ml
18) N-TETRACONTANE	21.354	929068	10.228 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009749.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 16:38
Operator : AJ\MA
Sample : N1208-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 22:59:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

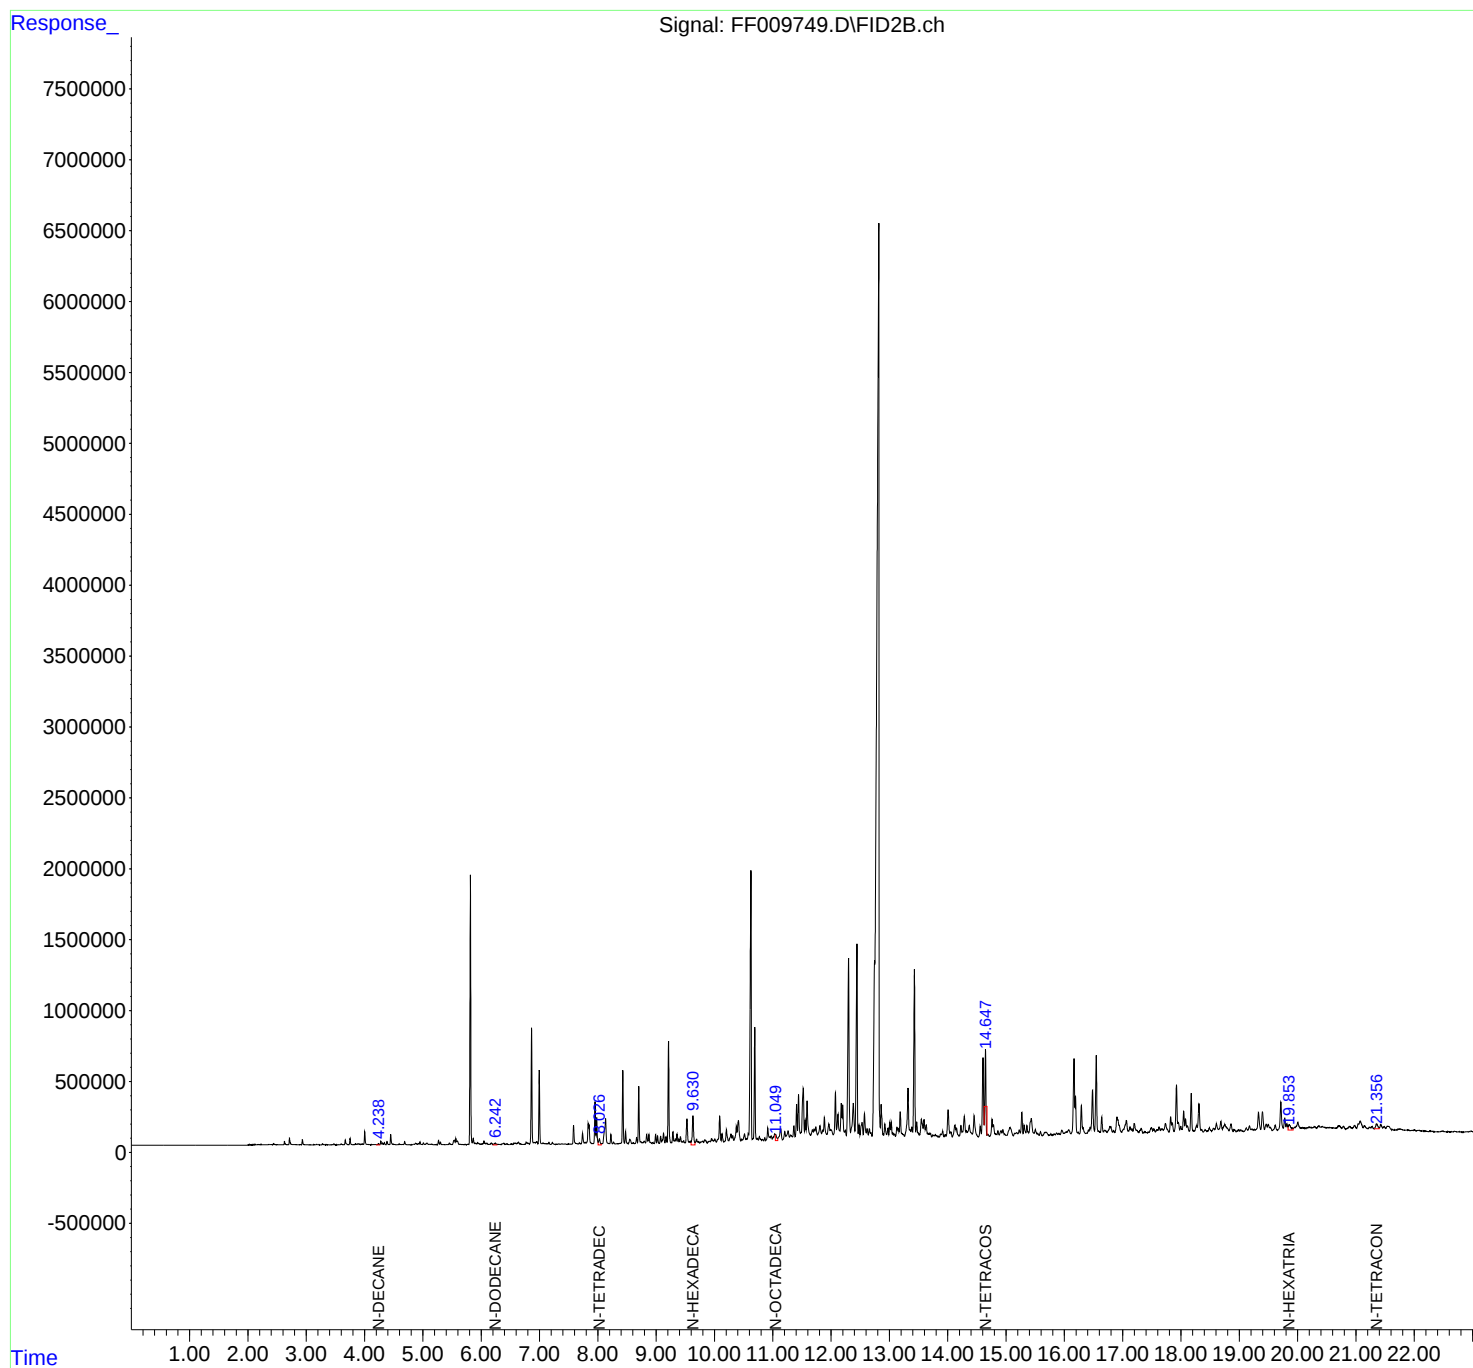


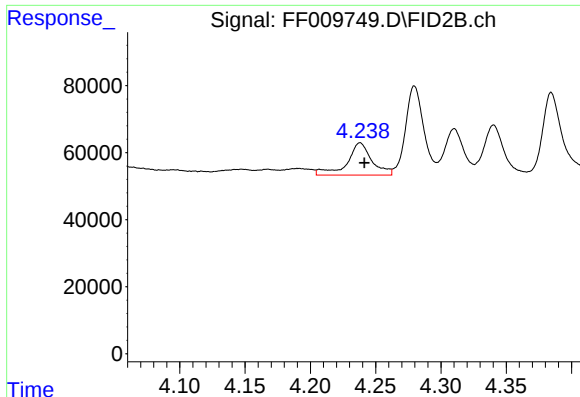

#2 N-DECANE


R.T.: 4.238 min
Delta R.T.: -0.003 min
Response: 127566
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

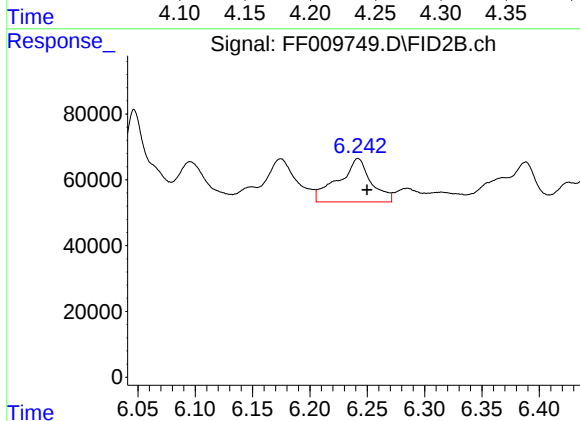


#3 N-DODECANE

R.T.: 6.242 min
Delta R.T.: -0.008 min
Response: 261536
Conc: 1.83 ug/ml

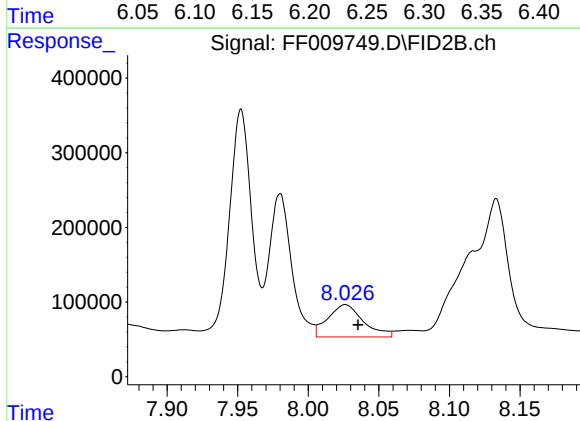


#4 N-TETRADECANE

R.T.: 8.026 min
Delta R.T.: -0.009 min
Response: 756213
Conc: 5.15 ug/ml

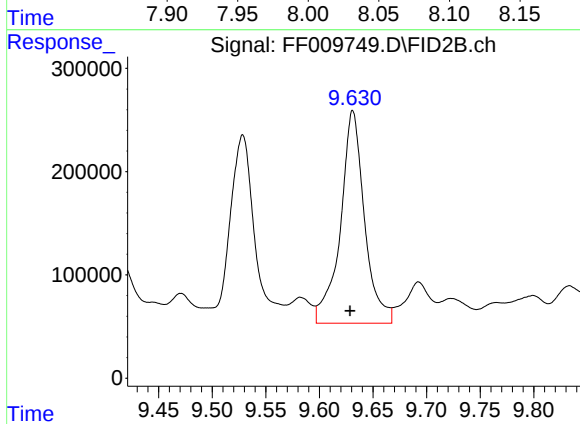

#5 N-HEXADECANE


R.T.: 9.631 min
Delta R.T.: 0.002 min
Response: 3224549
Conc: 21.56 ug/ml

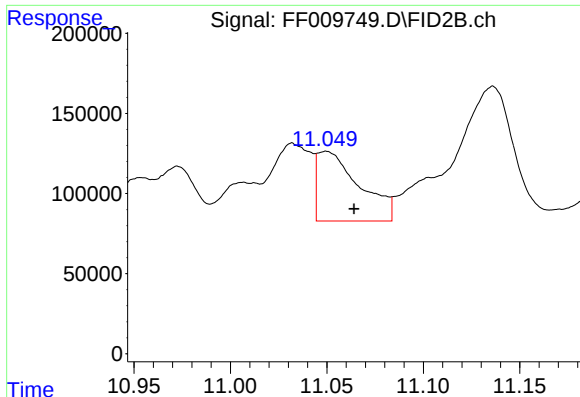

#6 N-OCTADECANE


R.T.: 11.050 min
Delta R.T.: -0.015 min
Response: 659191
Conc: 4.28 ug/ml

Instrument :
FID_F
ClientSampleId :

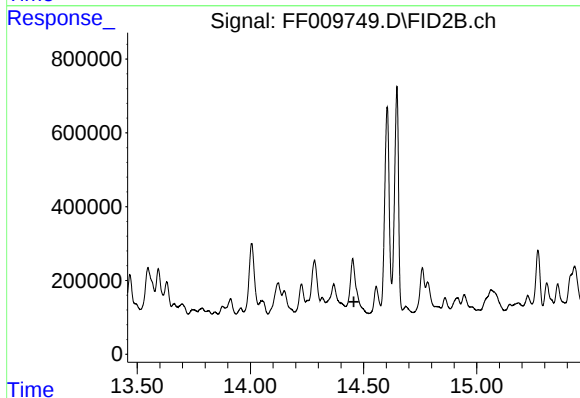


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.452 min
Delta R.T.: -0.005 min
Response: -10548936
Conc: N.D.

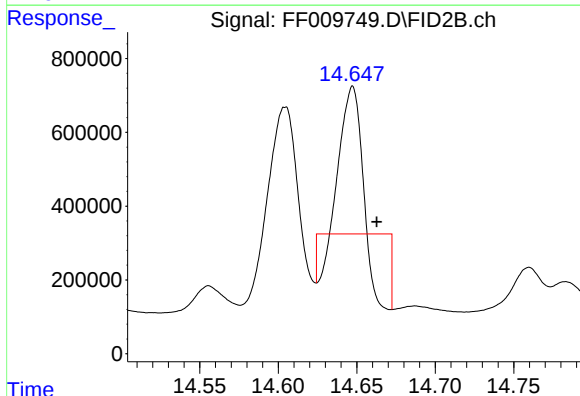


#10 N-TETRACOSANE

R.T.: 14.647 min
Delta R.T.: -0.015 min
Response: 1452578
Conc: 9.79 ug/ml

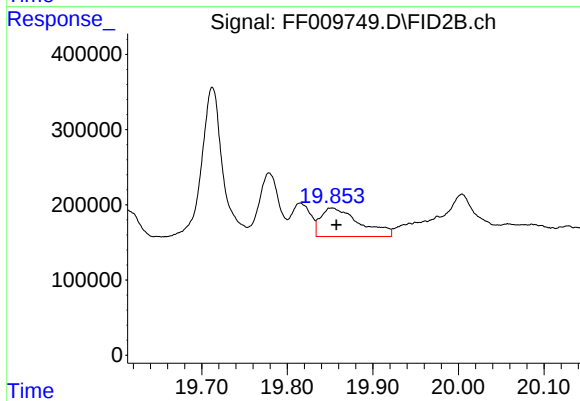

#16 N-HEXATRIACONTANE

R.T.: 19.852 min
Delta R.T.: -0.005 min
Response: 1202546
Conc: 11.66 ug/ml

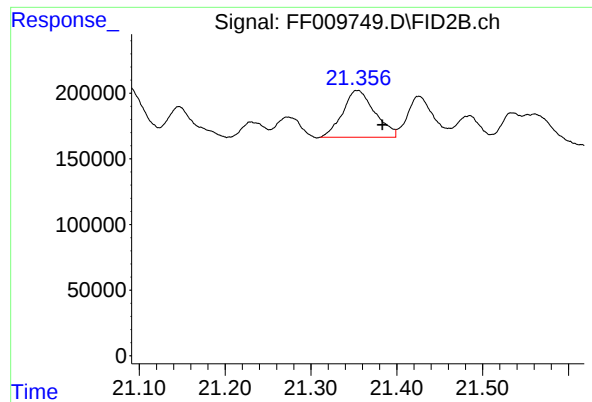

#18 N-TETRACONTANE

R.T.: 21.354 min
Delta R.T.: -0.029 min
Response: 929068
Conc: 10.23 ug/ml

Instrument :

FID_F

ClientSampleId :