

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
 Data File : FF009752.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jan 2022 18:06
 Operator : AJ\MA
 Sample : N1224-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 23:00:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.450	1864254	14.266 ug/ml
Target Compounds			
4) N-TETRADECANE	8.028	81401	0.554 ug/ml
8) N-DOCOSANE	13.553	71308	0.479 ug/ml
10) N-TETRACOSANE	14.651	235462	1.588 ug/ml
11) N-HEXACOSANE	15.669	961002	6.573 ug/ml
12) N-OCTACOSANE	16.615	370537	2.553 ug/ml
13) N-TRIACONTANE	17.498	468009	3.271 ug/ml
14) N-DOTRIACONTANE	18.349	200272	1.472 ug/ml
15) N-TETRATRIACONTANE	19.106	893839	7.526 ug/ml
16) N-HEXATRIACONTANE	19.855	667387	6.473 ug/ml
18) N-TETRACONTANE	21.386	173916	1.915 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009752.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 18:06
Operator : AJ\MA
Sample : N1224-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 23:00:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

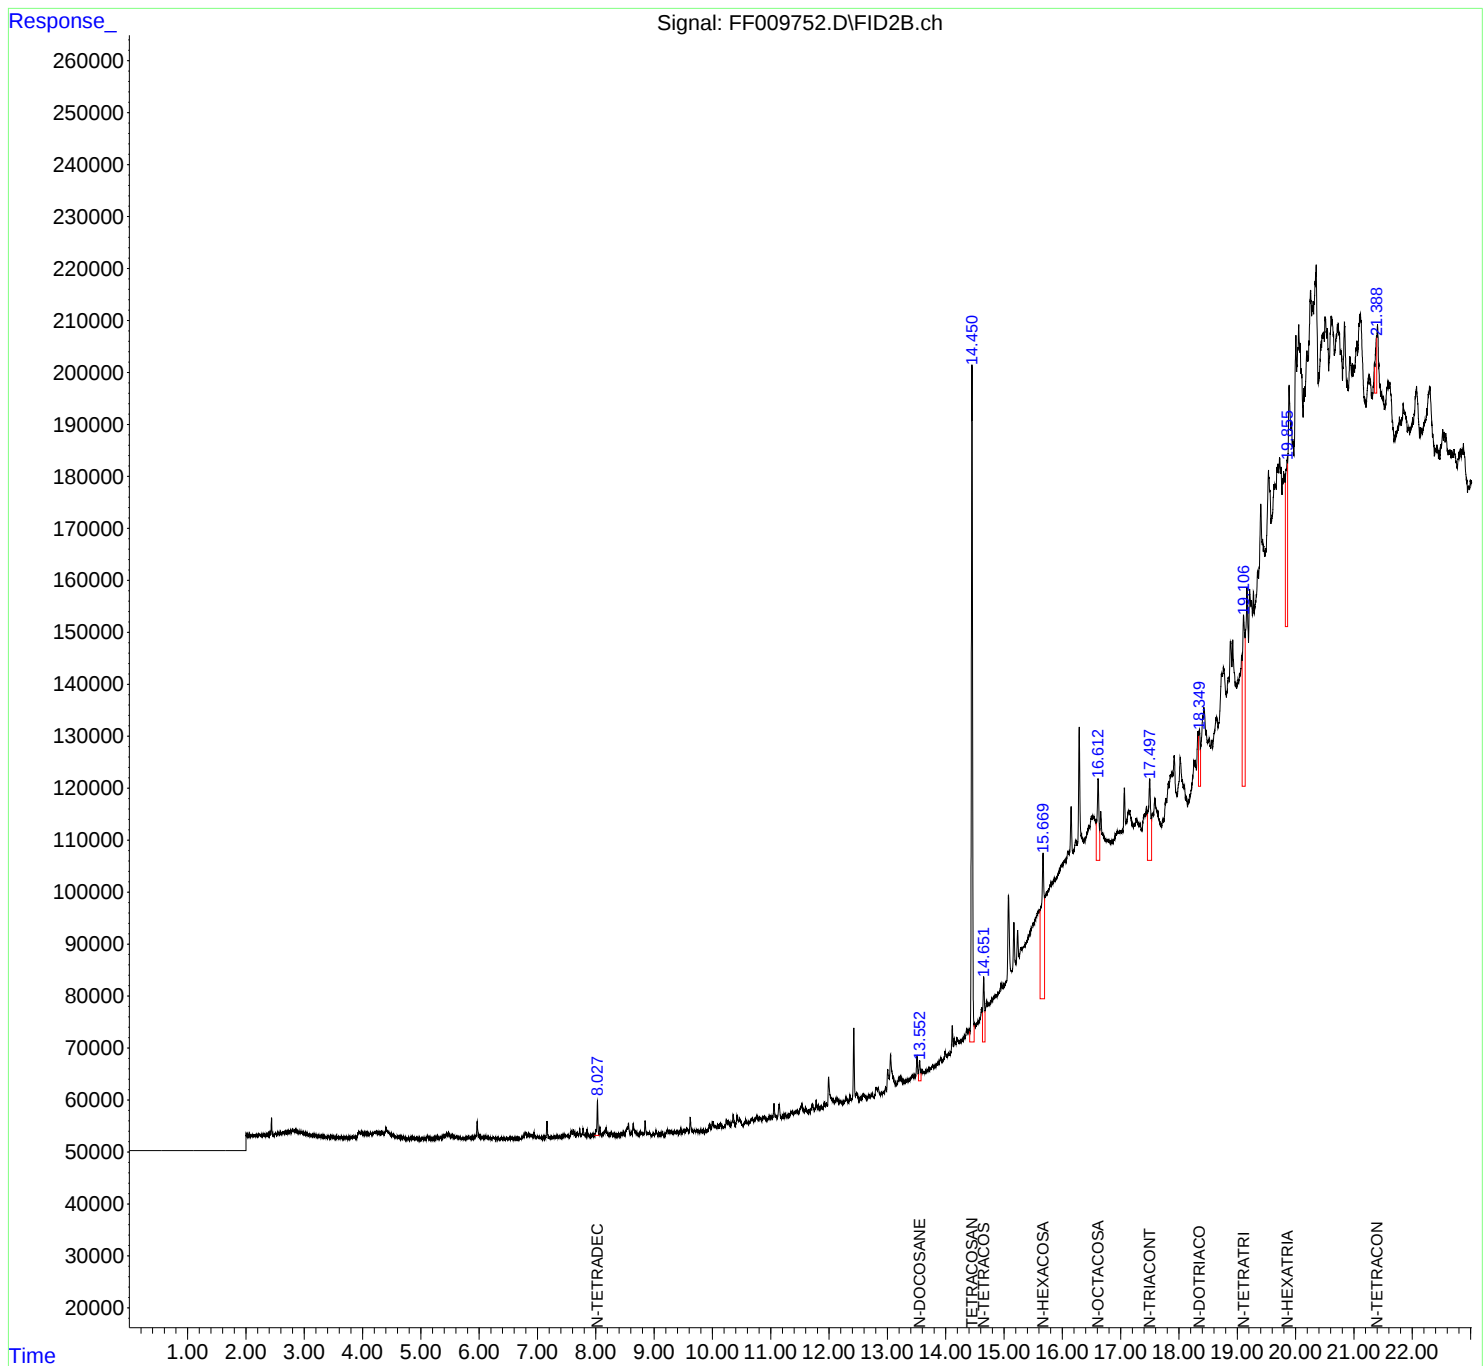


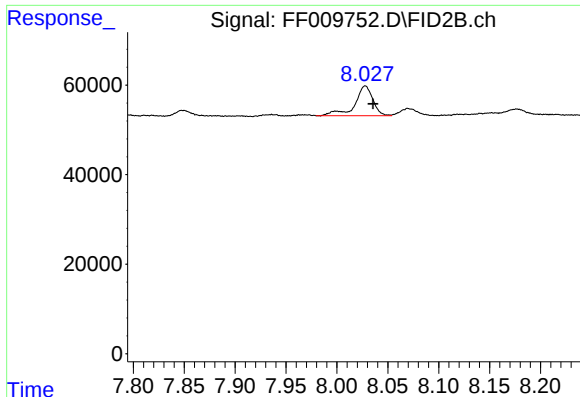

#4 N-TETRADECANE


R.T.: 8.028 min
Delta R.T.: -0.007 min
Response: 81401
Conc: 0.55 ug/ml

Instrument :
FID_F
ClientSampleId :

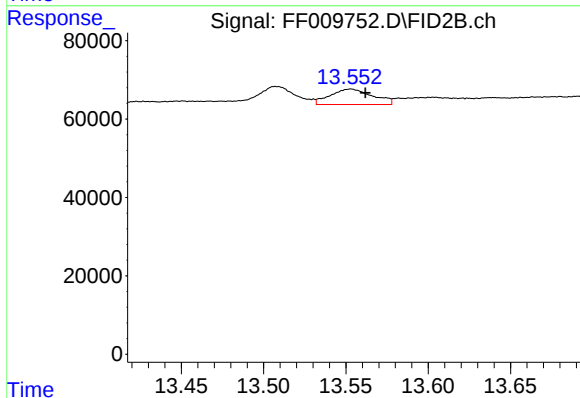


#8 N-DOCOSANE

R.T.: 13.553 min
Delta R.T.: -0.009 min
Response: 71308
Conc: 0.48 ug/ml

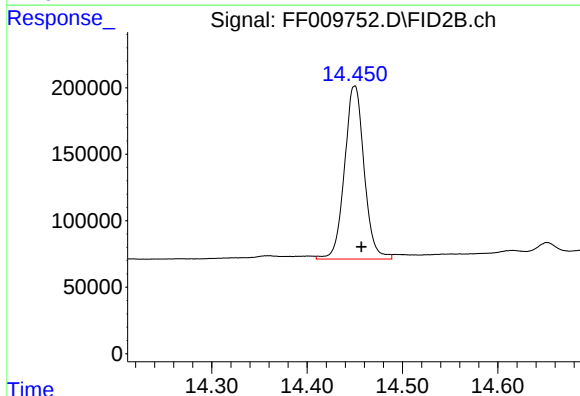


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.450 min
Delta R.T.: -0.007 min
Response: 1864254
Conc: 14.27 ug/ml

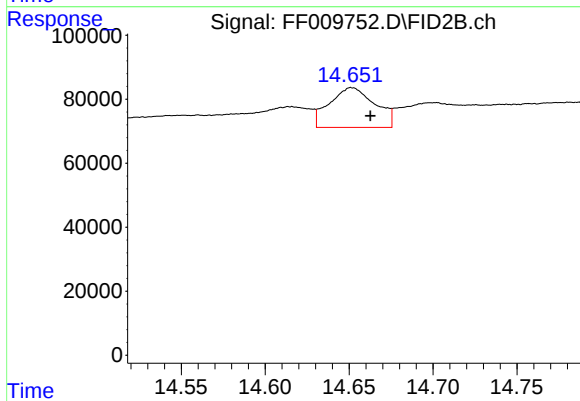

#10 N-TETRACOSANE


R.T.: 14.651 min
Delta R.T.: -0.012 min
Response: 235462
Conc: 1.59 ug/ml

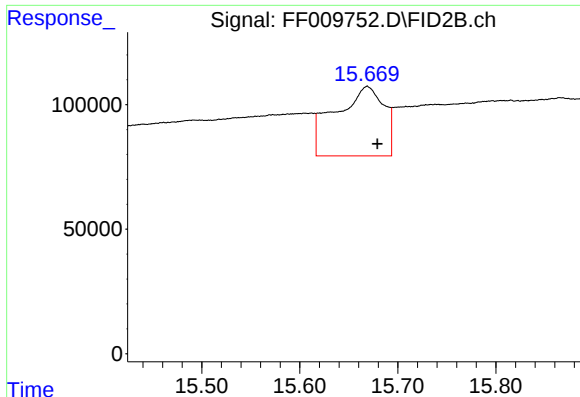

#11 N-HEXACOSANE


R.T.: 15.669 min
Delta R.T.: -0.010 min
Response: 961002
Conc: 6.57 ug/ml

Instrument :
FID_F
ClientSampleId :

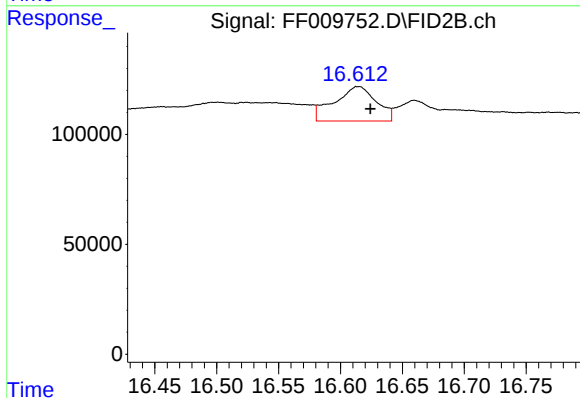


#12 N-OCTACOSANE

R.T.: 16.615 min
Delta R.T.: -0.009 min
Response: 370537
Conc: 2.55 ug/ml

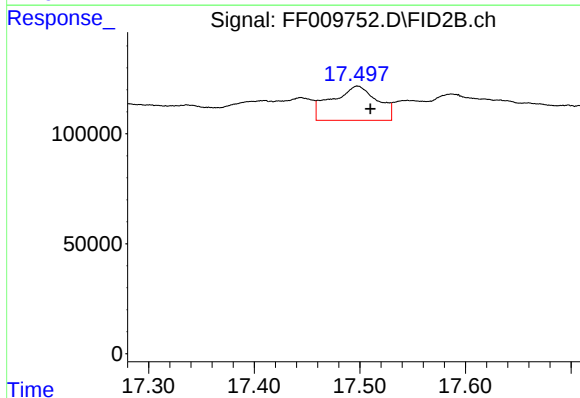


#13 N-TRIACONTANE

R.T.: 17.498 min
Delta R.T.: -0.012 min
Response: 468009
Conc: 3.27 ug/ml

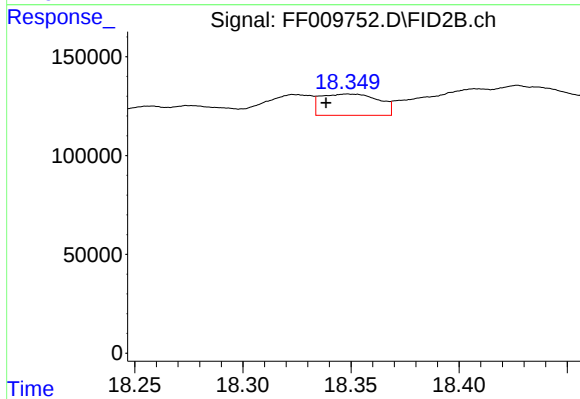

#14 N-DOTRIACONTANE


R.T.: 18.349 min
Delta R.T.: 0.010 min
Response: 200272
Conc: 1.47 ug/ml

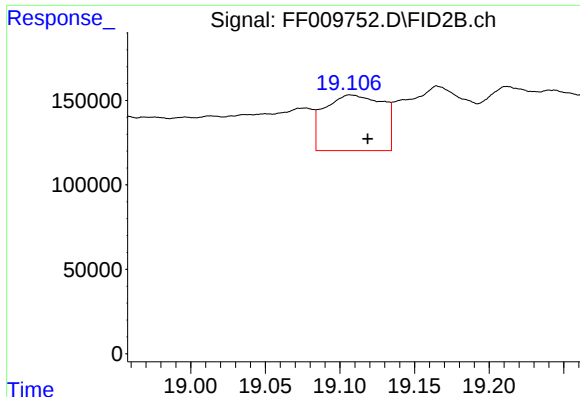

#15 N-TETRATRIACONTANE


R.T.: 19.106 min
Delta R.T.: -0.012 min
Response: 893839
Conc: 7.53 ug/ml

Instrument :
FID_F
ClientSampleId :

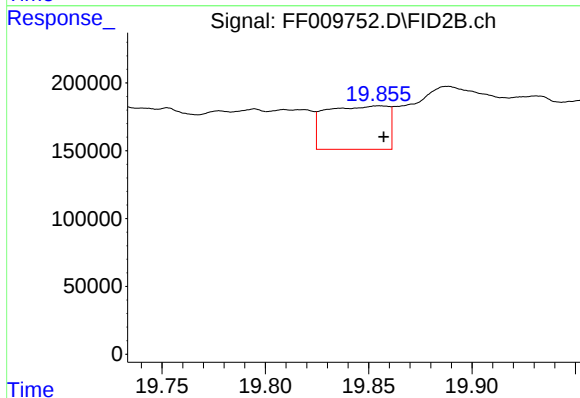

#16 N-HEXATRIACONTANE

R.T.: 19.855 min
Delta R.T.: -0.002 min
Response: 667387
Conc: 6.47 ug/ml

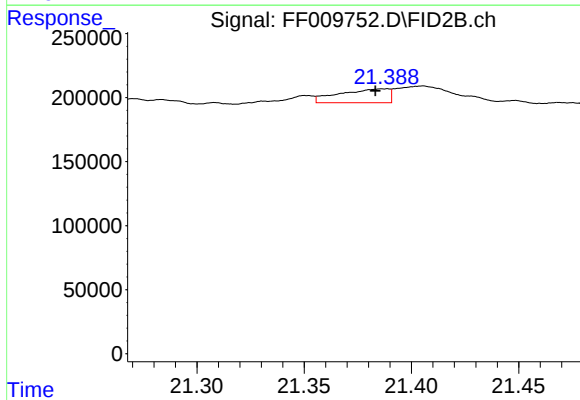

#18 N-TETRACONTANE

R.T.: 21.386 min
Delta R.T.: 0.003 min
Response: 173916
Conc: 1.91 ug/ml