

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009764.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 23:54
Operator : AJ\MA
Sample : N1208-02 50X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 01:28:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

6)	N-OCTADECANE	11.026	181565	1.178 ug/ml
10)	N-TETRACOSANE	14.649	74283	0.501 ug/ml
12)	N-OCTACOSANE	16.608	112996	0.778 ug/ml
13)	N-TRIACONTANE	17.492	92883	0.649 ug/ml
14)	N-DOTRIACONTANE	18.323	790133	5.806 ug/ml
15)	N-TETRATRIACONTANE	19.102	990641	8.341 ug/ml
16)	N-HEXATRIACONTANE	19.843	233047	2.260 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009764.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 23:54
Operator : AJ\MA
Sample : N1208-02 50X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 01:28:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

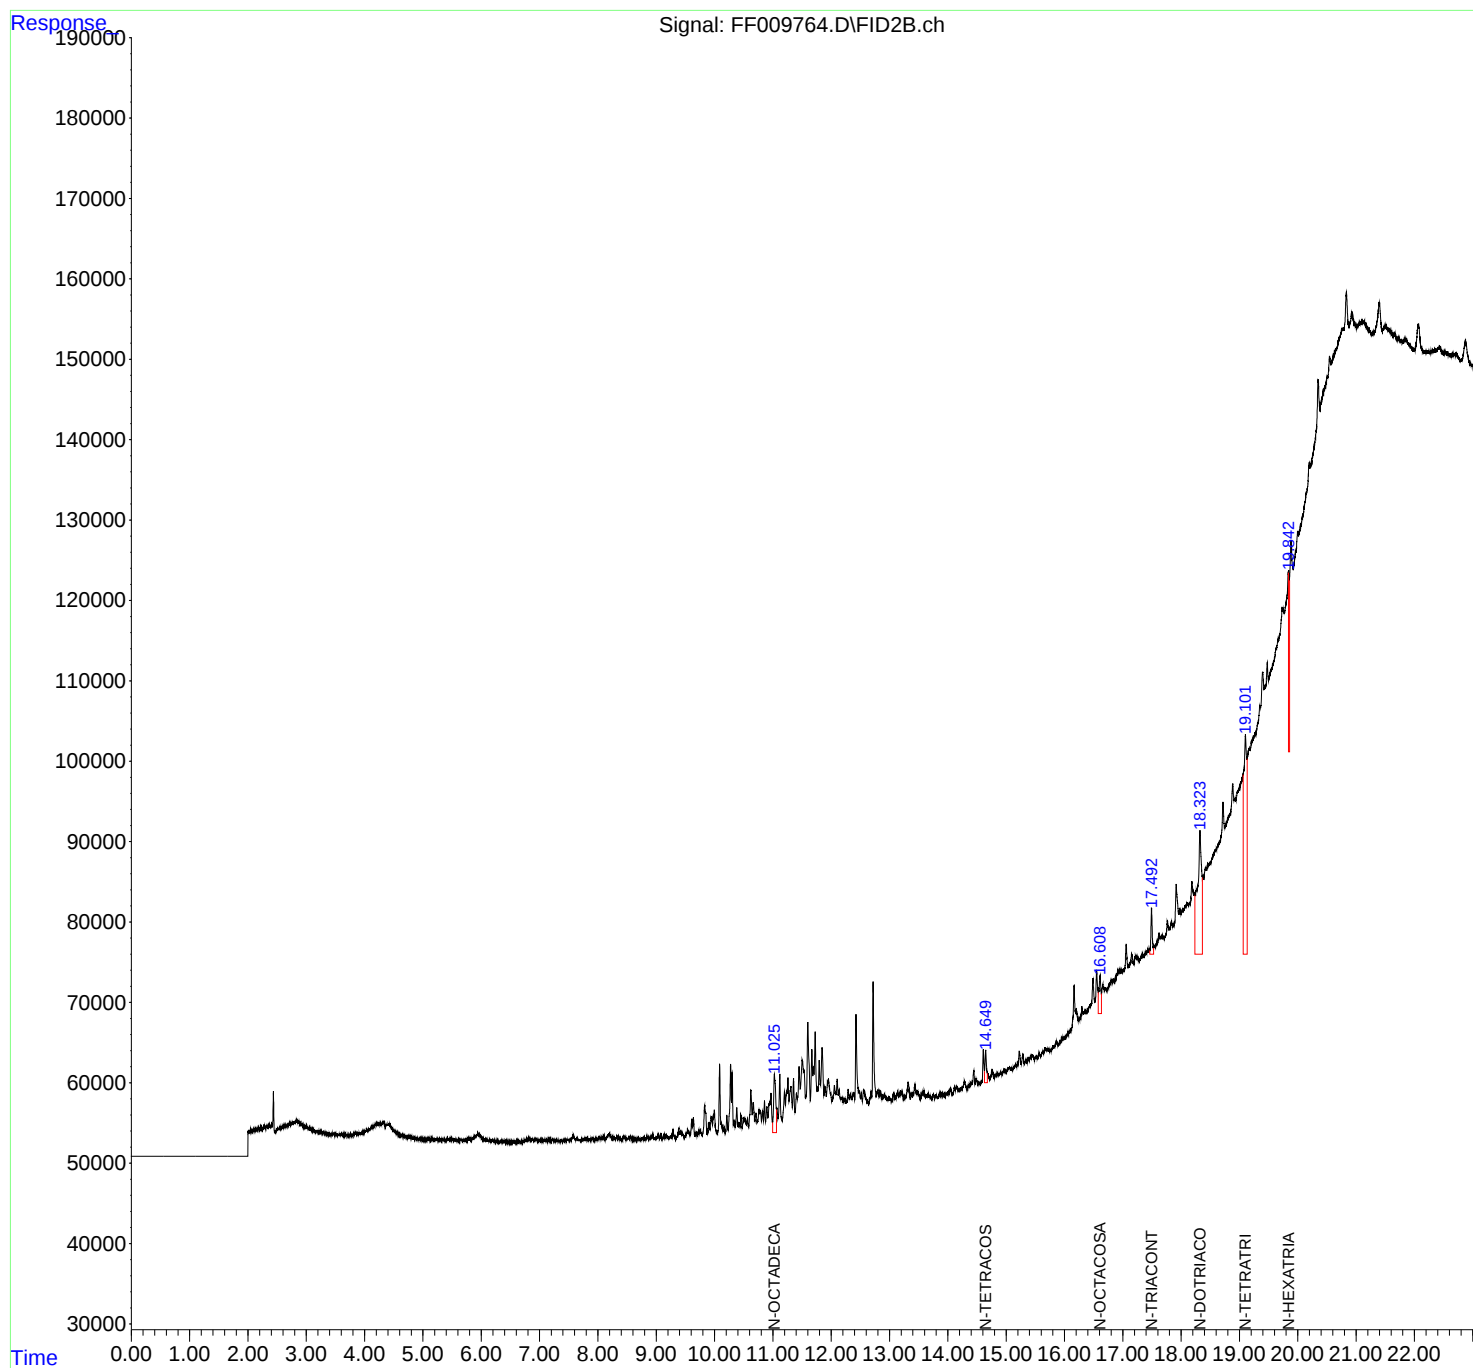


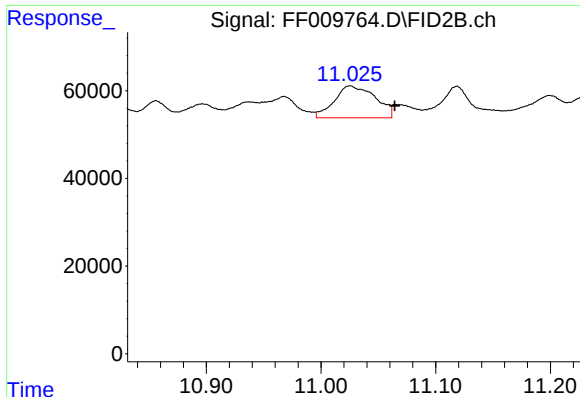

#6 N-OCTADECANE


R.T.: 11.026 min
Delta R.T.: -0.039 min
Response: 181565
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :

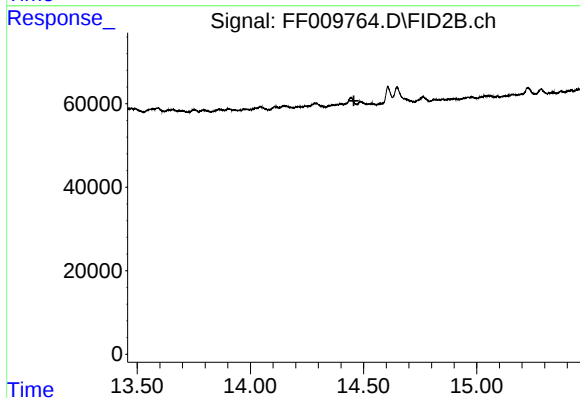


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

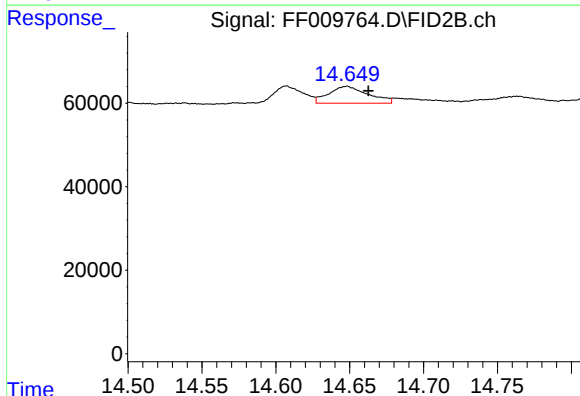


#10 N-TETRACOSANE

R.T.: 14.649 min
Delta R.T.: -0.014 min
Response: 74283
Conc: 0.50 ug/ml

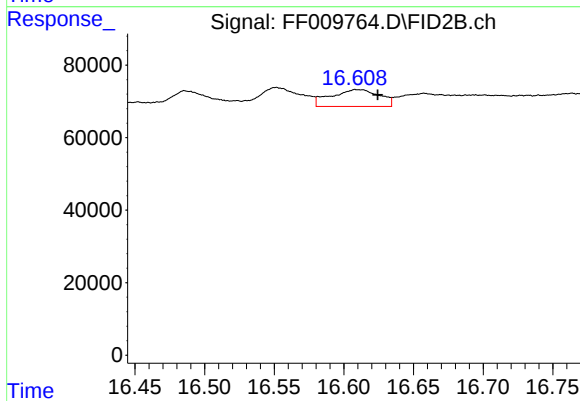

#12 N-OCTACOSANE


R.T.: 16.608 min
Delta R.T.: -0.016 min
Response: 112996
Conc: 0.78 ug/ml

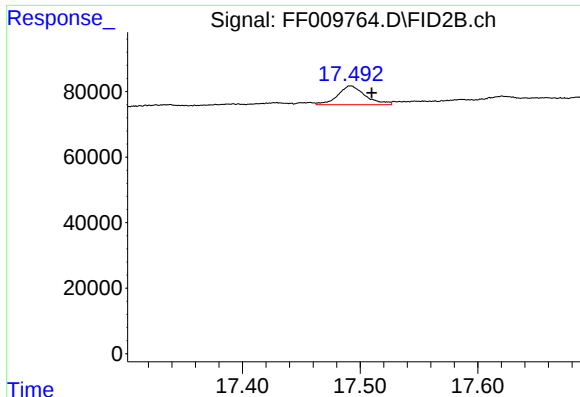

#13 N-TRIACONTANE


R.T.: 17.492 min
Delta R.T.: -0.017 min
Response: 92883
Conc: 0.65 ug/ml

Instrument :
FID_F
ClientSampleId :

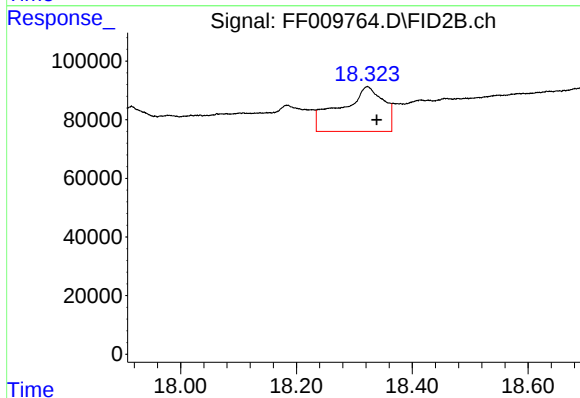


#14 N-DOTRIACONTANE

R.T.: 18.323 min
Delta R.T.: -0.015 min
Response: 790133
Conc: 5.81 ug/ml

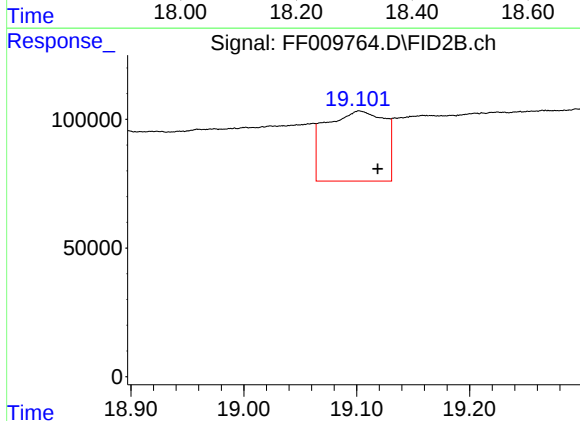

#15 N-TETRATRIACONTANE

R.T.: 19.102 min
Delta R.T.: -0.017 min
Response: 990641
Conc: 8.34 ug/ml

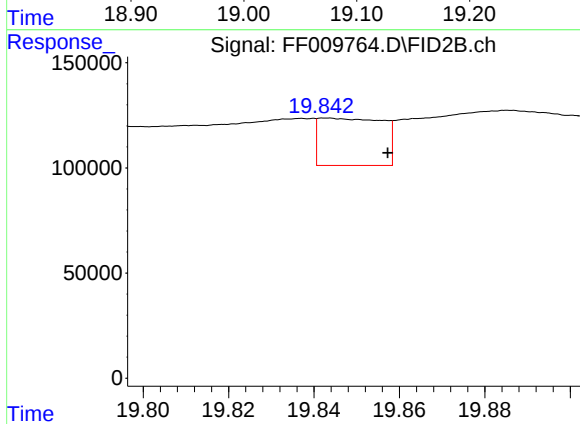

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.014 min
Response: 233047
Conc: 2.26 ug/ml