

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009766.D
Signal(s) : FID2B.ch
Acq On : 22 Jan 2022 00:52
Operator : AJ\MA
Sample : N1208-01 100X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 01:29:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5)	N-HEXADECANE	9.636	162455	1.086 ug/ml
6)	N-OCTADECANE	11.067	260088	1.687 ug/ml
7)	N-EICOSANE	12.388	68329	0.452 ug/ml
14)	N-DOTRIACONTANE	18.332	1655755	12.167 ug/ml
15)	N-TETRATRIACONTANE	19.119	113651	0.957 ug/ml
16)	N-HEXATRIACONTANE	19.888	3233081	31.358 ug/ml
18)	N-TETRACONTANE	21.398	117380	1.292 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009766.D
Signal(s) : FID2B.ch
Acq On : 22 Jan 2022 00:52
Operator : AJ\MA
Sample : N1208-01 100X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 01:29:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

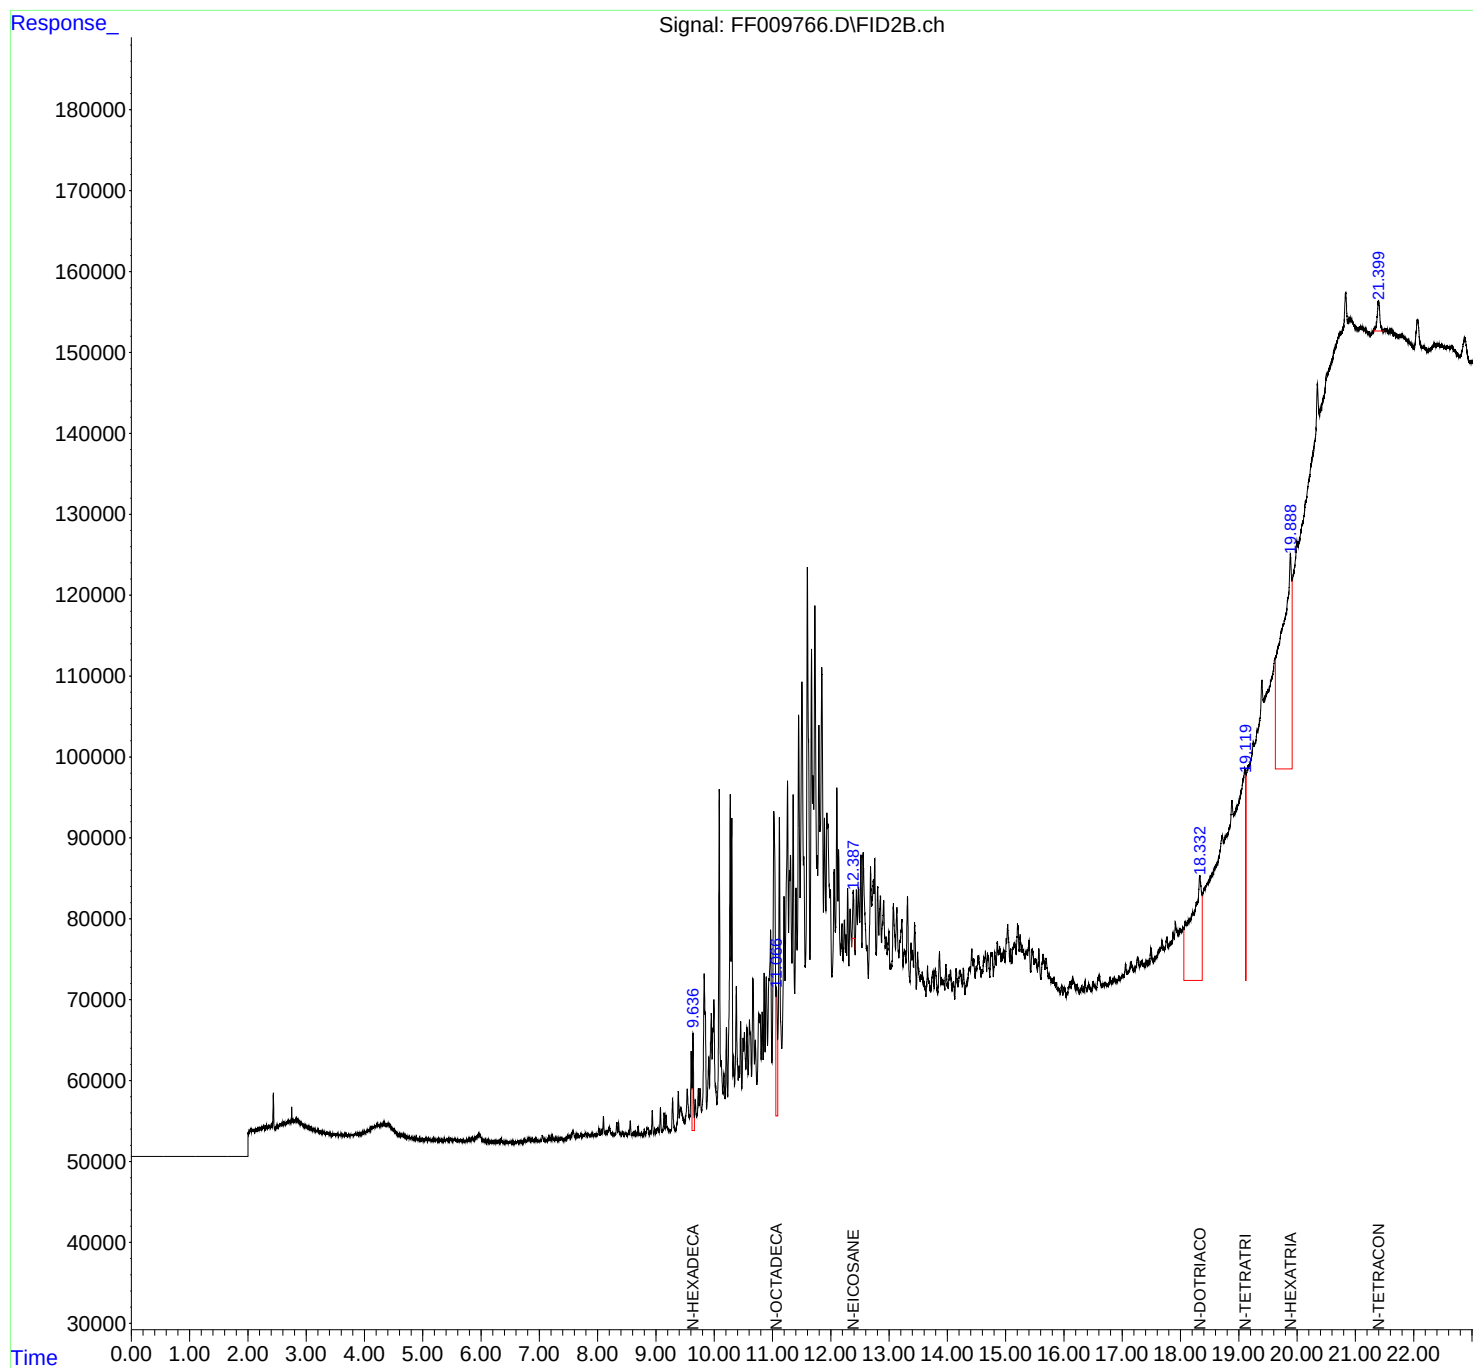


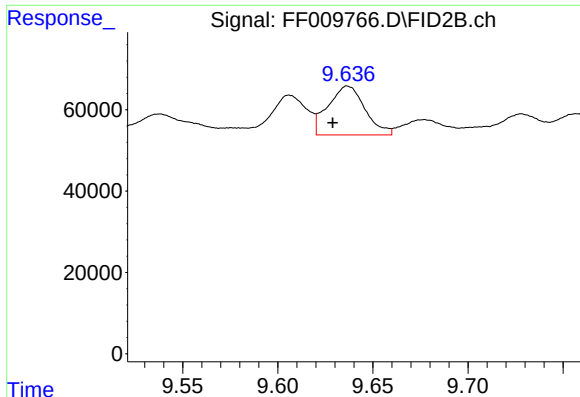

#5 N-HEXADECANE


R.T.: 9.636 min
Delta R.T.: 0.008 min
Response: 162455
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :

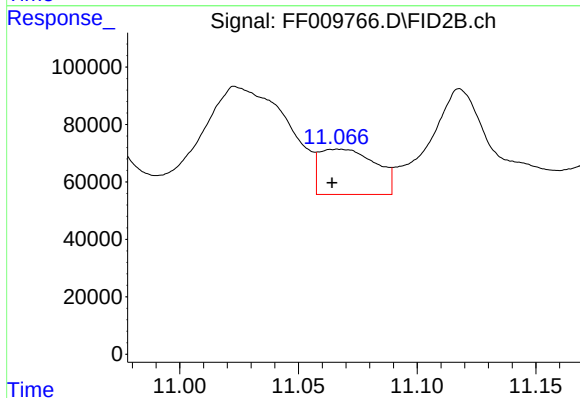


#6 N-OCTADECANE

R.T.: 11.067 min
Delta R.T.: 0.003 min
Response: 260088
Conc: 1.69 ug/ml

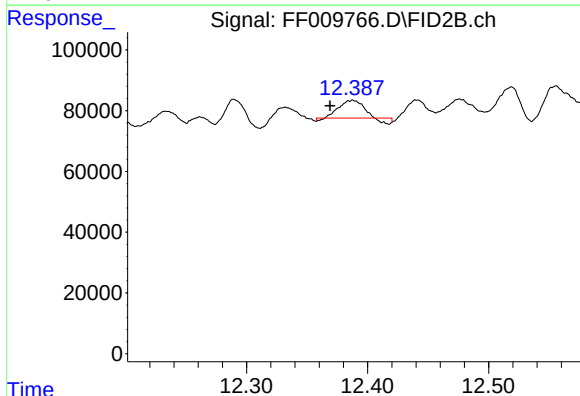


#7 N-EICOSANE

R.T.: 12.388 min
Delta R.T.: 0.019 min
Response: 68329
Conc: 0.45 ug/ml

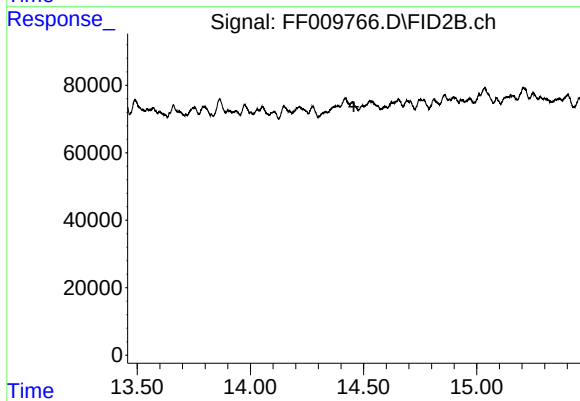

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.421 min
Delta R.T.: -0.036 min
Response: -29519
Conc: N.D.

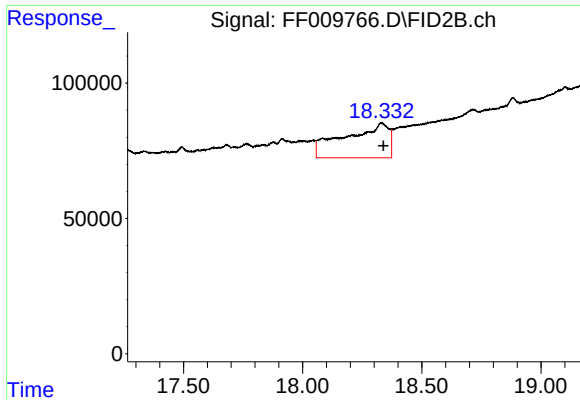

#14 N-DOTRIACONTANE


R.T.: 18.332 min
Delta R.T.: -0.006 min
Response: 1655755
Conc: 12.17 ug/ml

Instrument :
FID_F
ClientSampleId :

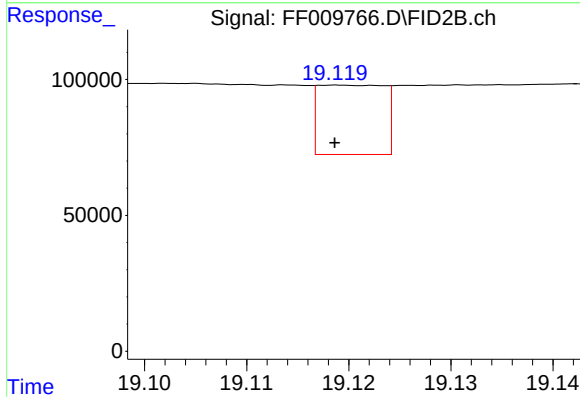


#15 N-TETRATRIACONTANE

R.T.: 19.119 min
Delta R.T.: 0.000 min
Response: 113651
Conc: 0.96 ug/ml

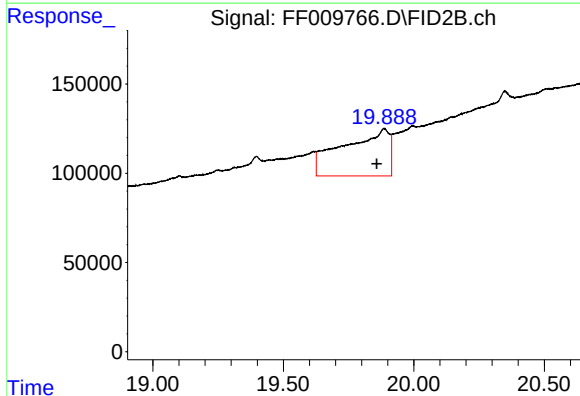

#16 N-HEXATRIACONTANE

R.T.: 19.888 min
Delta R.T.: 0.030 min
Response: 3233081
Conc: 31.36 ug/ml

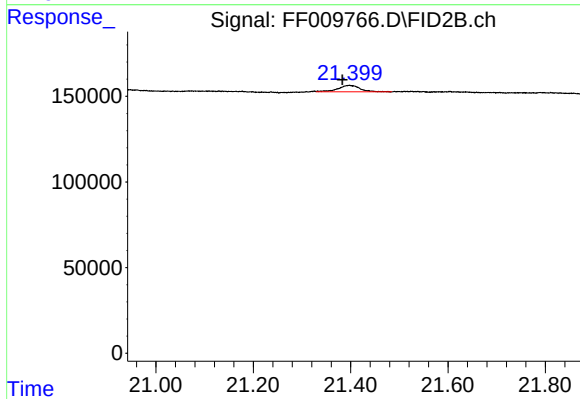

#18 N-TETRACONTANE

R.T.: 21.398 min
Delta R.T.: 0.015 min
Response: 117380
Conc: 1.29 ug/ml