

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
 Data File : FF009769.D
 Signal(s) : FID2B.ch
 Acq On : 22 Jan 2022 02:19
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 22 02:41:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.442	2265258	17.335 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.606	110659	0.762 ug/ml
13) N-TRIACONTANE	17.490	146376	1.023 ug/ml
14) N-DOTRIACONTANE	18.320	497919	3.659 ug/ml
15) N-TETRATRIACONTANE	19.130	97123	0.818 ug/ml
16) N-HEXATRIACONTANE	19.839	937377	9.092 ug/ml
17) N-OCTATRIACONTANE	20.544	67615	0.758 ug/ml
18) N-TETRACONTANE	21.396	121918	1.342 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009769.D
Signal(s) : FID2B.ch
Acq On : 22 Jan 2022 02:19
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 02:41:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

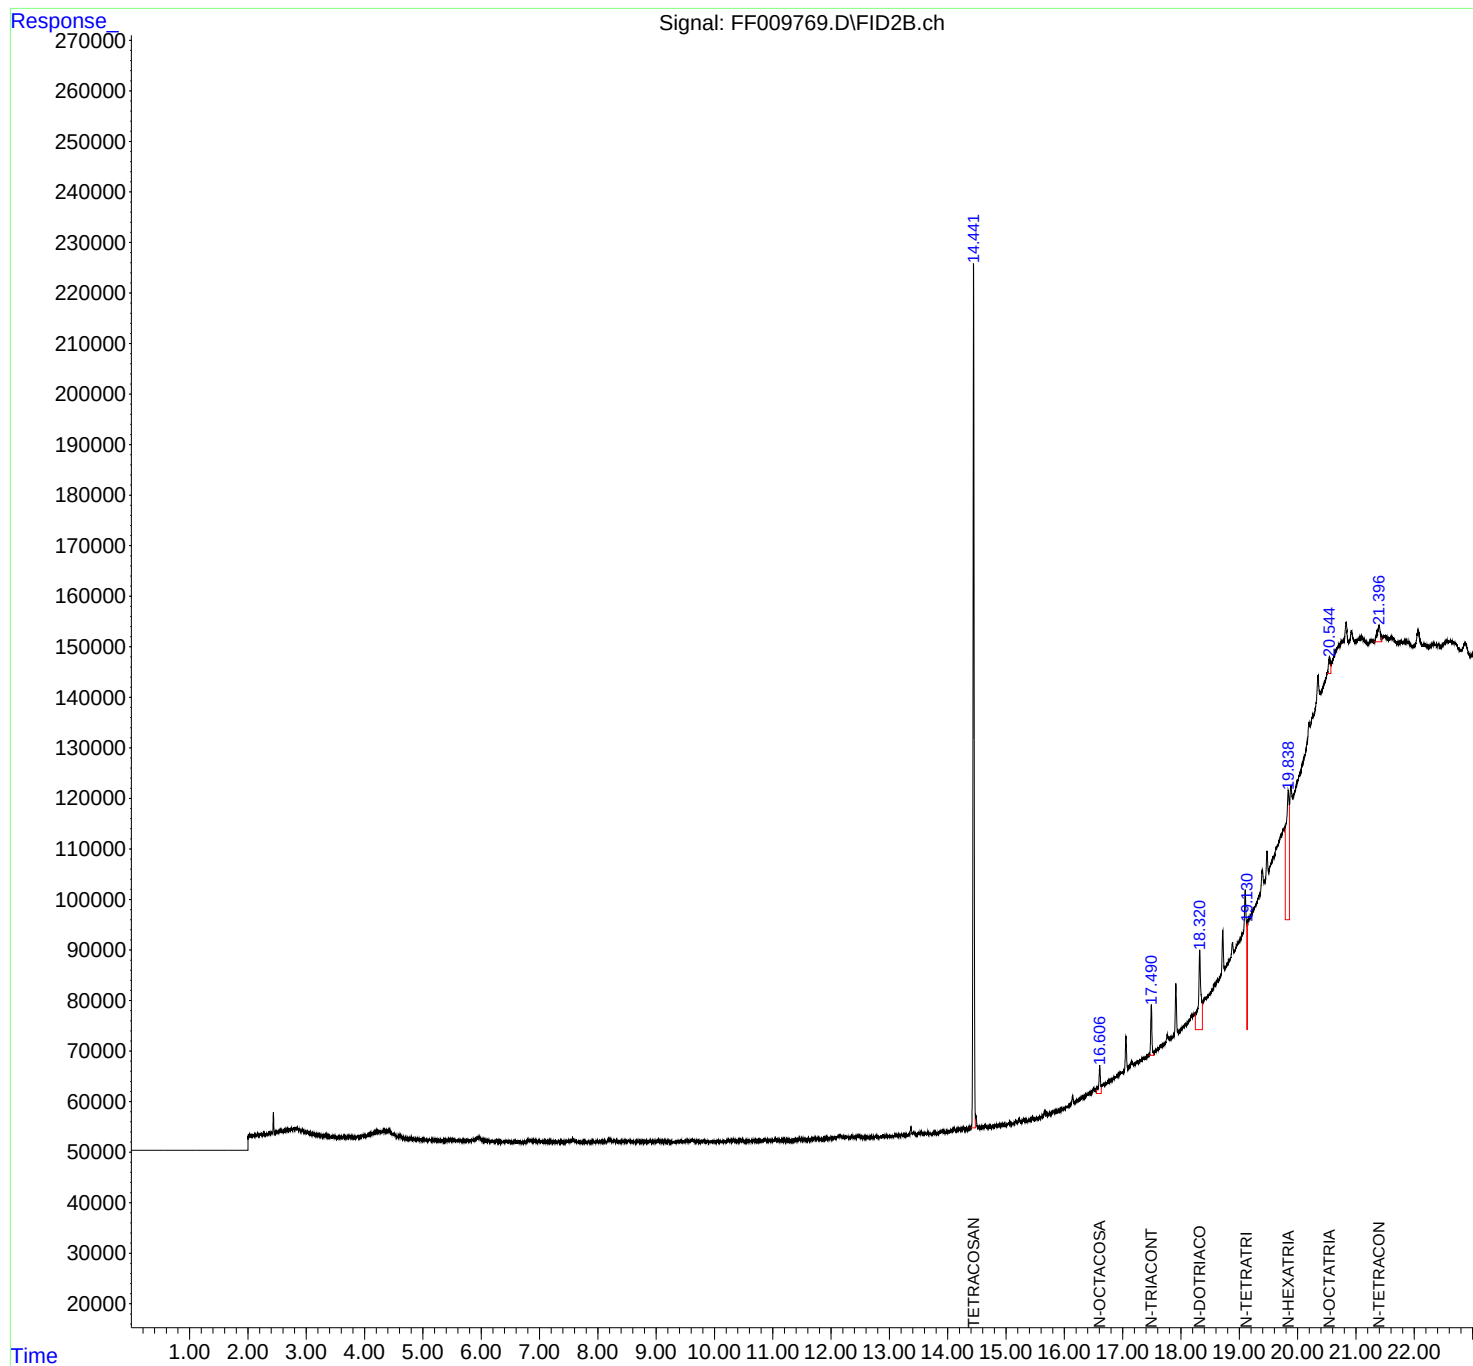


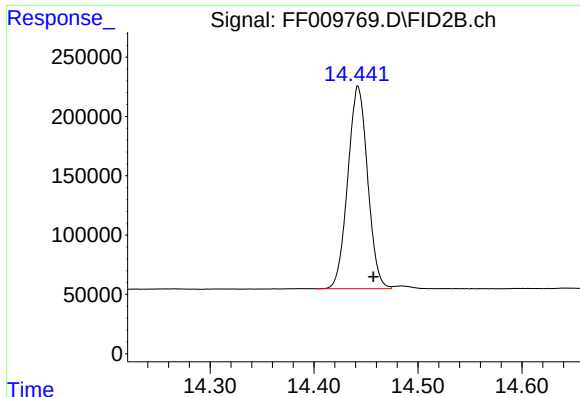

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.442 min
Delta R.T.: -0.015 min
Response: 2265258
Conc: 17.33 ug/ml

Instrument :
FID_F
ClientSampleId :

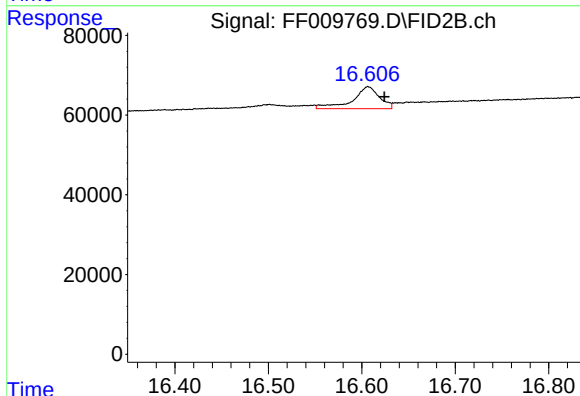


#12 N-OCTACOSANE

R.T.: 16.606 min
Delta R.T.: -0.018 min
Response: 110659
Conc: 0.76 ug/ml

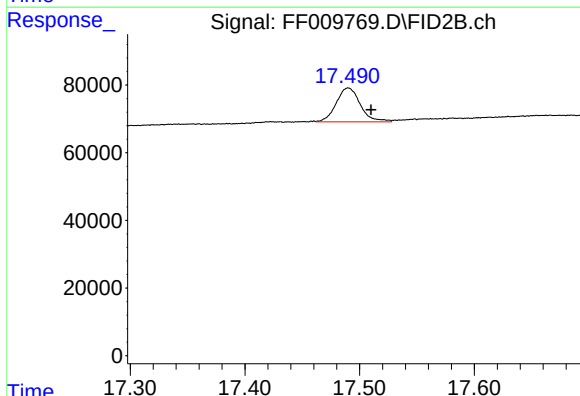


#13 N-TRIACONTANE

R.T.: 17.490 min
Delta R.T.: -0.020 min
Response: 146376
Conc: 1.02 ug/ml

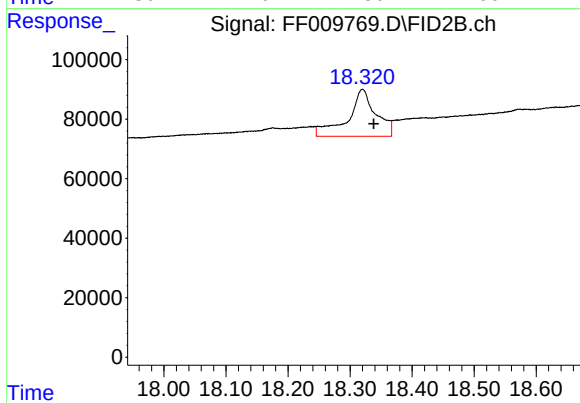

#14 N-DOTRIACONTANE


R.T.: 18.320 min
Delta R.T.: -0.018 min
Response: 497919
Conc: 3.66 ug/ml

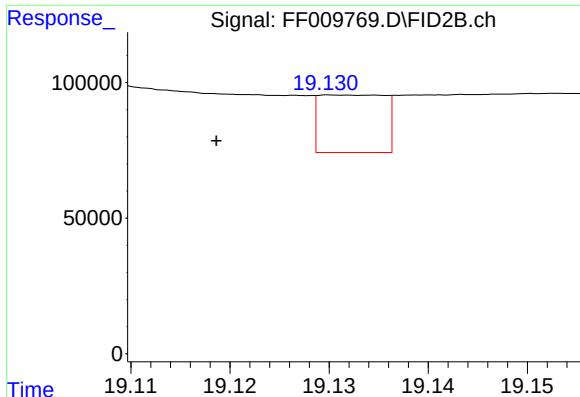

#15 N-TETRATRIACONTANE


R.T.: 19.130 min
Delta R.T.: 0.012 min
Response: 97123
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

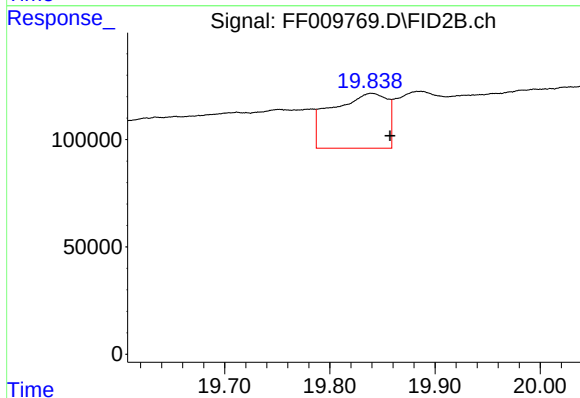


#16 N-HEXATRIACONTANE

R.T.: 19.839 min
Delta R.T.: -0.018 min
Response: 937377
Conc: 9.09 ug/ml

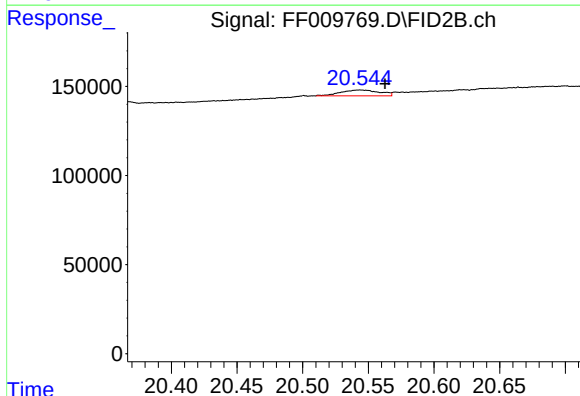

#17 N-OCTATRIACONTANE

R.T.: 20.544 min
Delta R.T.: -0.018 min
Response: 67615
Conc: 0.76 ug/ml

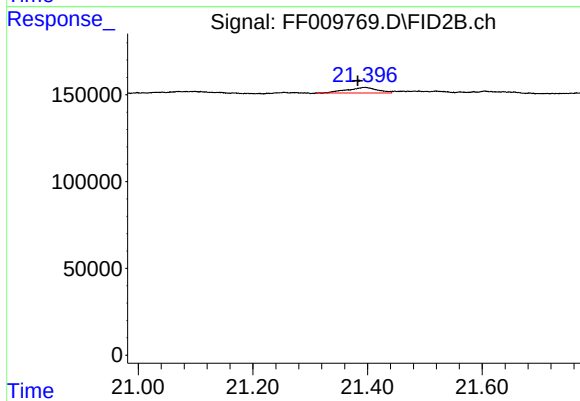

#18 N-TETRACONTANE

R.T.: 21.396 min
Delta R.T.: 0.013 min
Response: 121918
Conc: 1.34 ug/ml