

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009762.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 22:56
Operator : AJ\MA
Sample : N1224-14
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-1-B-5@7-BGS

Integration File: Sample.e
Quant Time: Jan 22 01:27:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.445	2041762	15.624 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012122\
Data File : FF009762.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2022 22:56
Operator : AJ\MA
Sample : N1224-14
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-1-B-5@7-BGS

Integration File: Sample.e
Quant Time: Jan 22 01:27:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

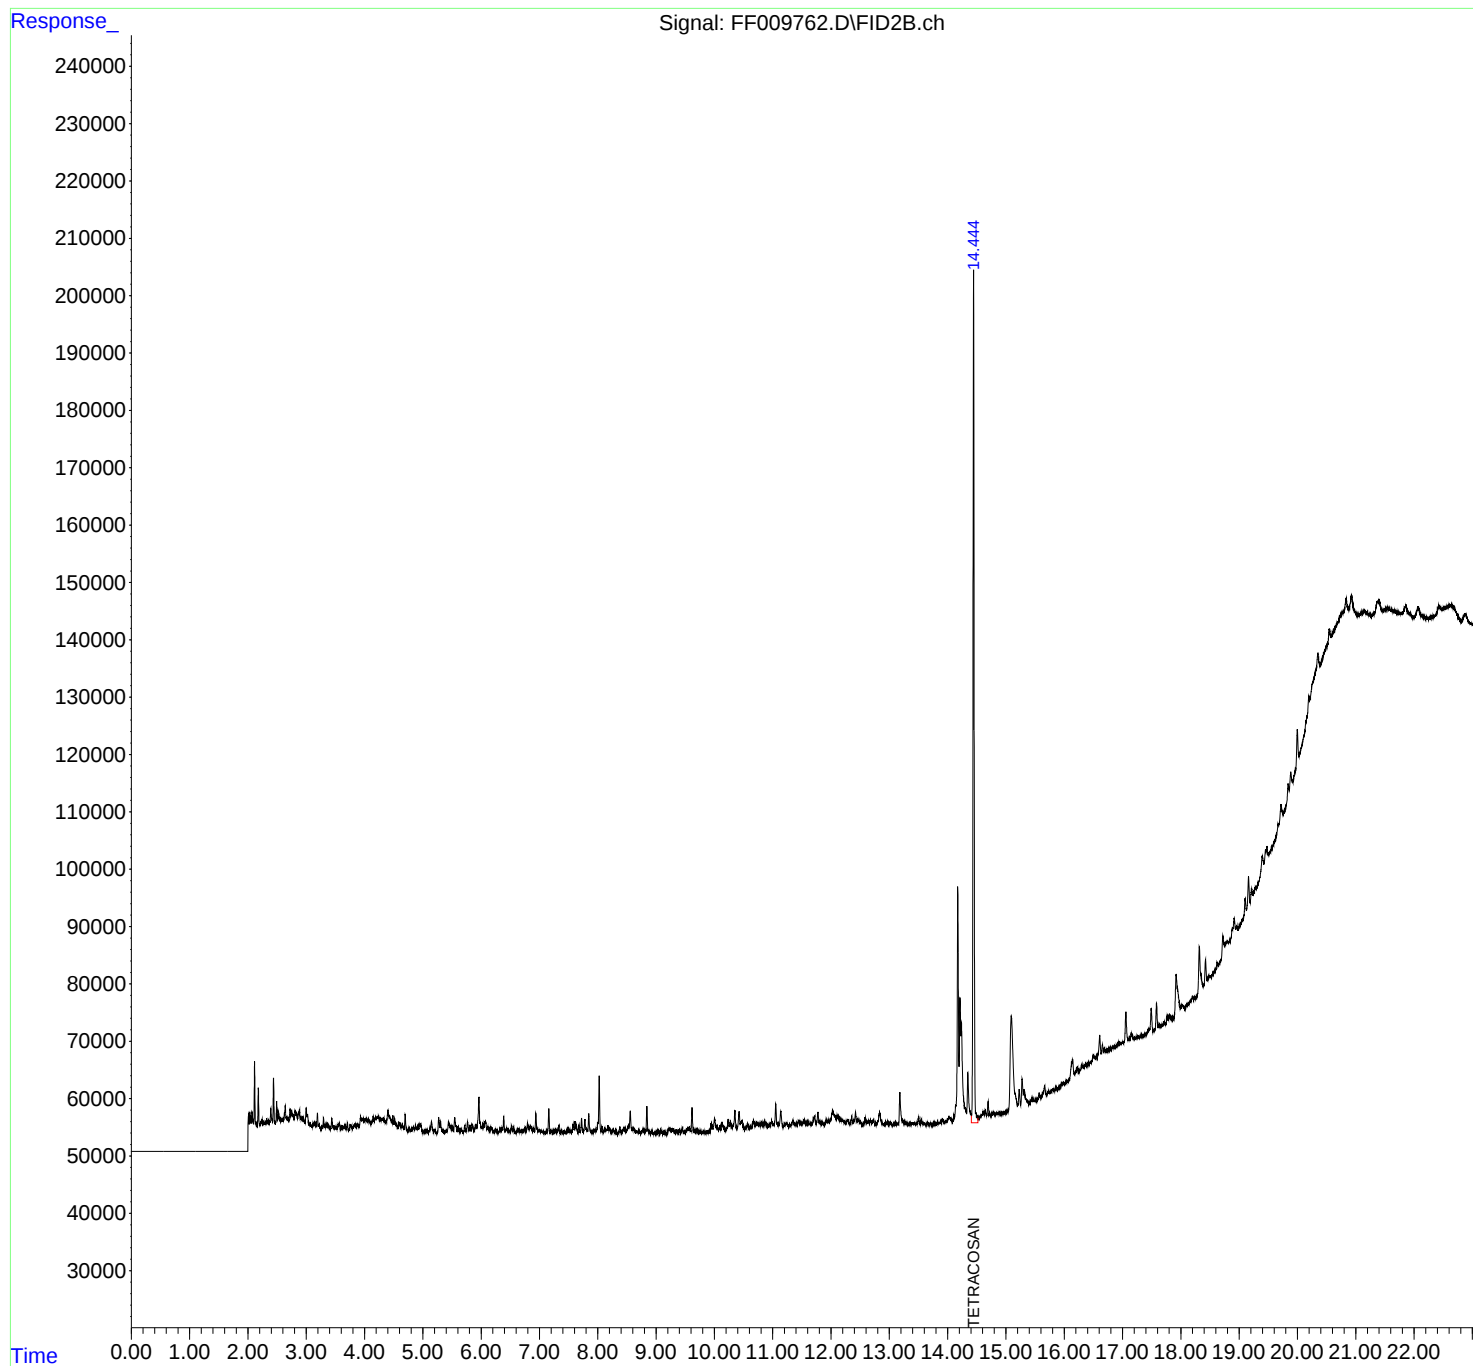

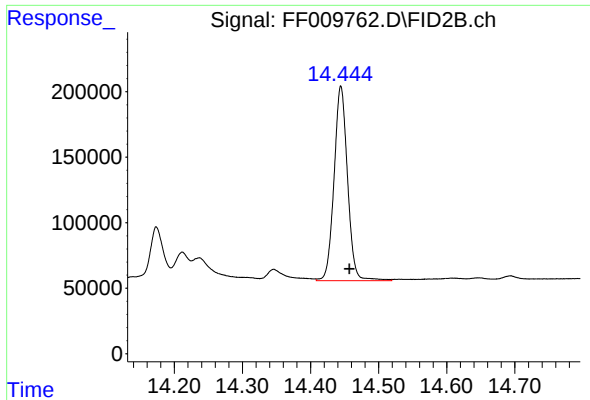

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.445 min
Delta R.T.: -0.013 min
Response: 2041762
Conc: 15.62 ug/ml

Instrument :
FID_F
ClientSampleId :
AREA-1-B-5@7-BGS