

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012125\
Data File : FF015256.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2025 09:20
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 00:30:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.925	62118	0.489 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012125\
Data File : FF015256.D
Signal(s) : FID2B.ch
Acq On : 21 Jan 2025 09:20
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 00:30:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

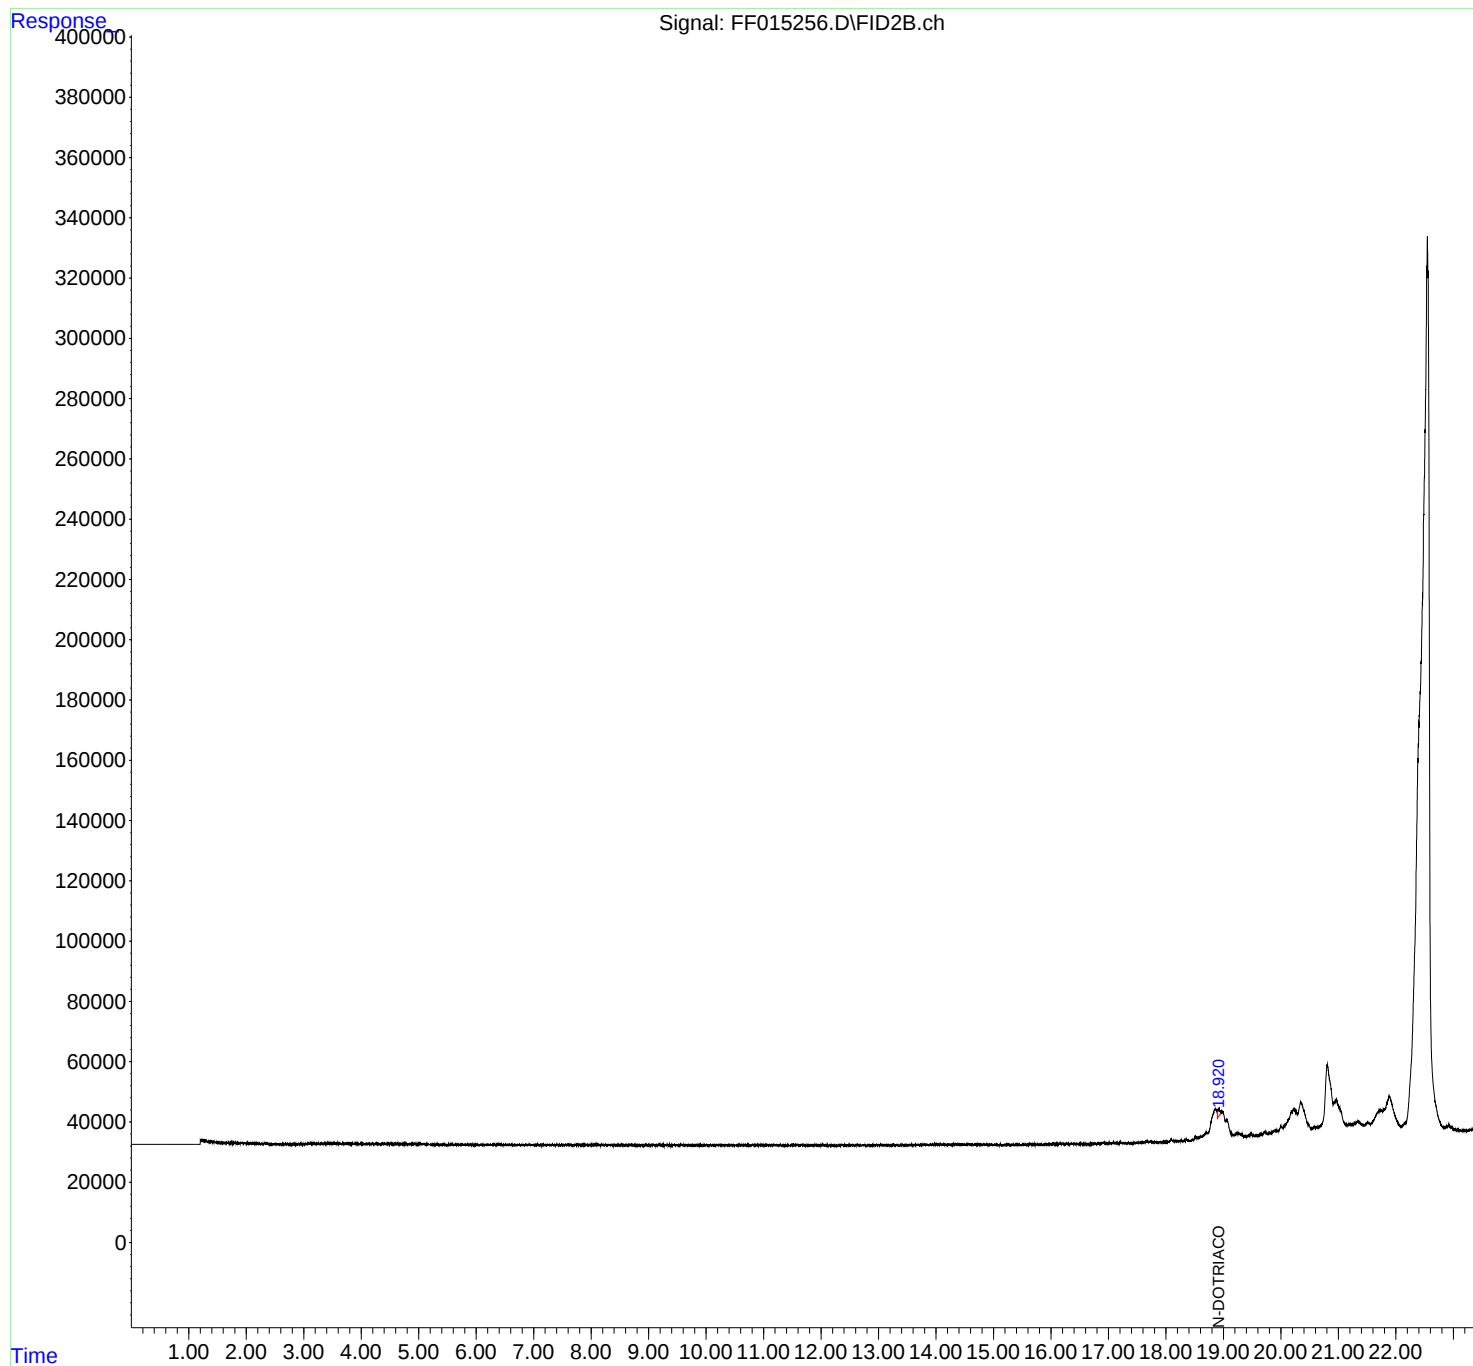


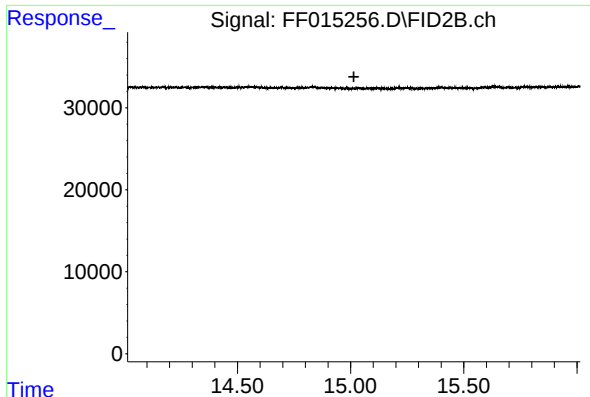

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.015 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

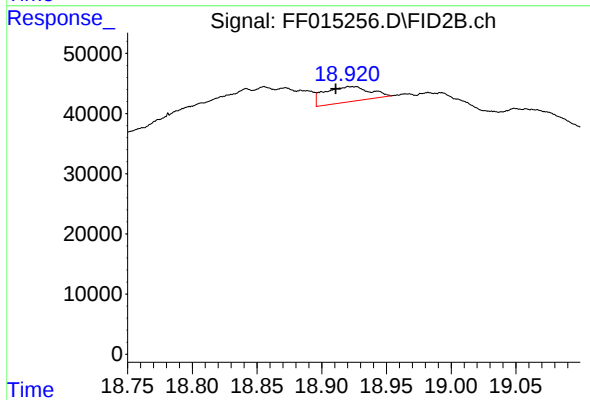

#14 N-DOTRIACONTANE

R.T.: 18.925 min
Delta R.T.: 0.014 min
Response: 62118
Conc: 0.49 ug/ml