

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012320\
 Data File : FF006263.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jan 2020 15:08
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 00:31:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.581	413472	3.816 ug/ml
Target Compounds			
3) N-DODECANE	6.393	3083040	24.414 ug/ml
11) N-HEXACOSANE	15.843	88549	0.720 ug/ml
12) N-OCTACOSANE	16.793	3072124	25.272 ug/ml
13) N-TRIACONTANE	17.675	342762	2.859 ug/ml
14) N-DOTRIACONTANE	18.507	349731	3.026 ug/ml
15) N-TETRATRIACONTANE	19.289	253359	2.249 ug/ml
16) N-HEXATRIACONTANE	20.029	112722	1.054 ug/ml
17) N-OCTATRIACONTANE	20.753	108968	1.178 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012320\
Data File : FF006263.D
Signal(s) : FID2B.ch
Acq On : 23 Jan 2020 15:08
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 00:31:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

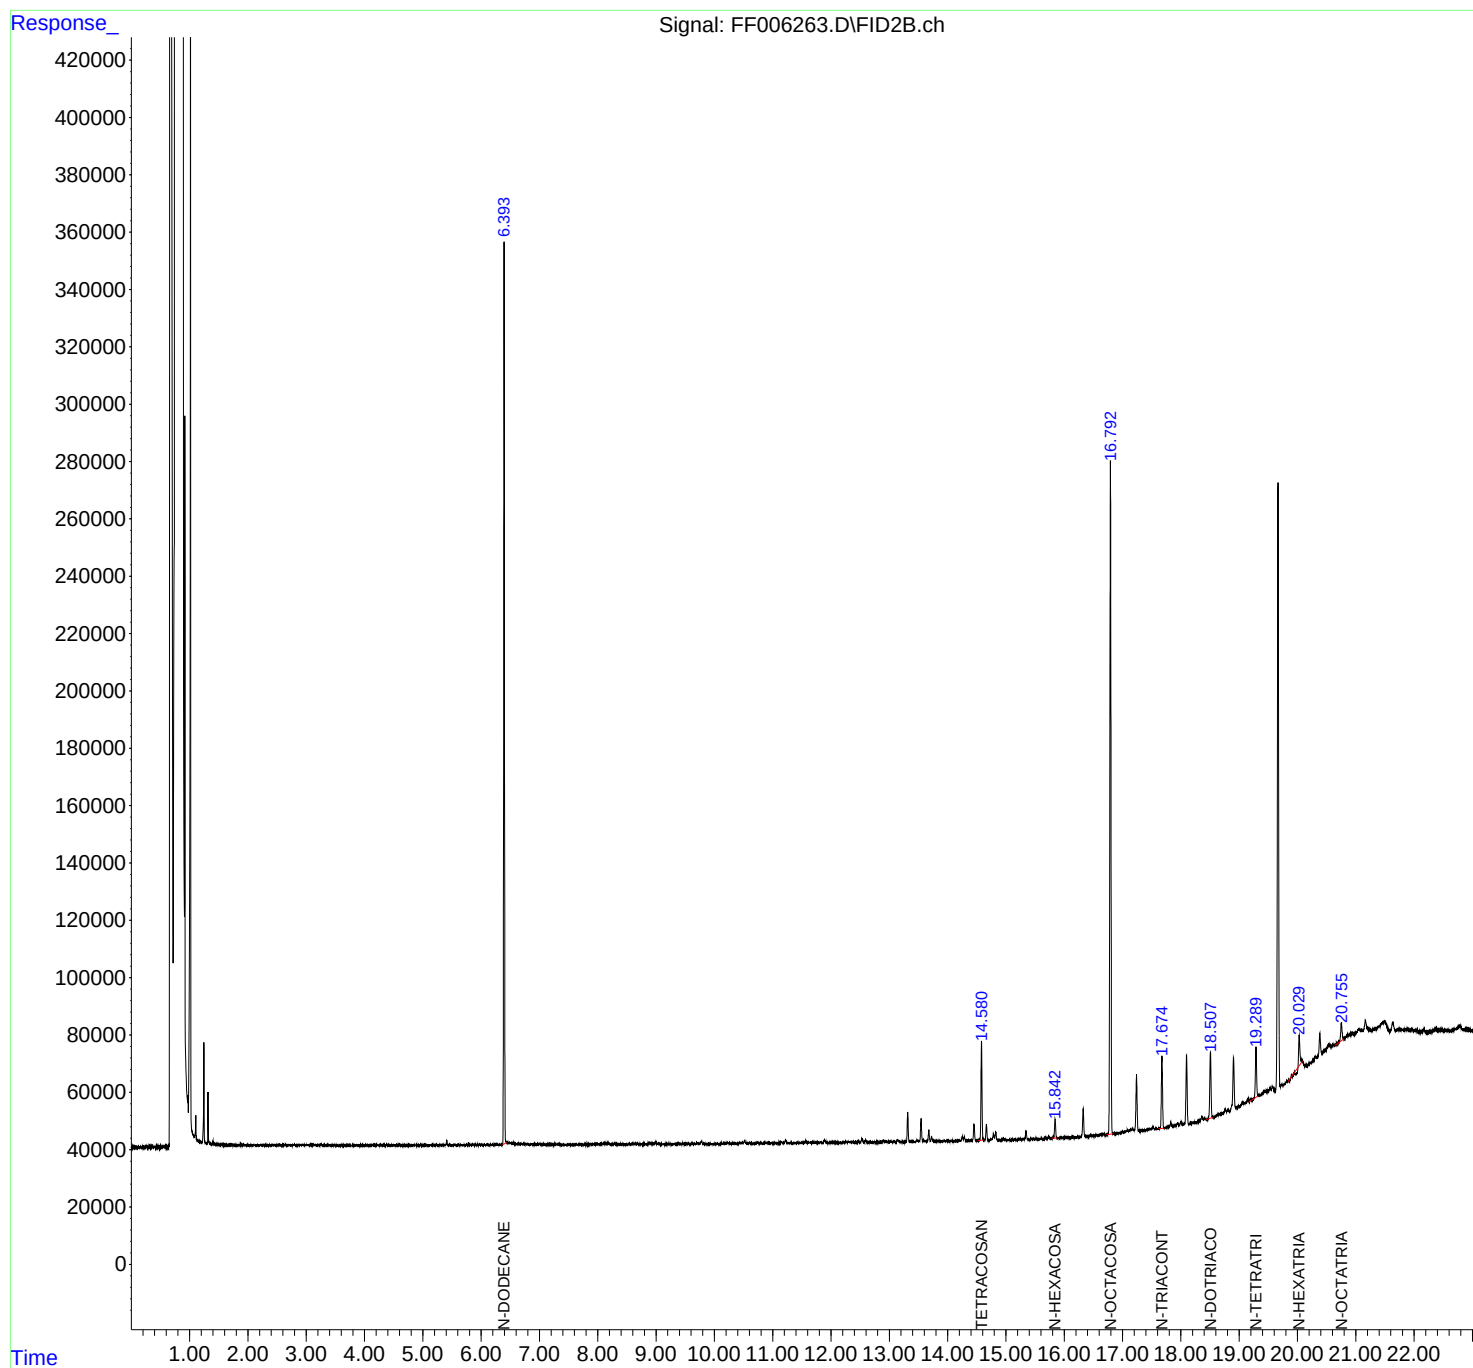


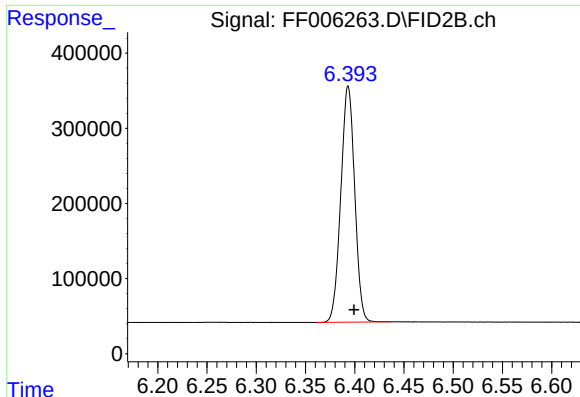

#3 N-DODECANE


R.T.: 6.393 min
Delta R.T.: -0.006 min
Response: 3083040
Conc: 24.41 ug/ml

Instrument :
FID_F
ClientSampleId :

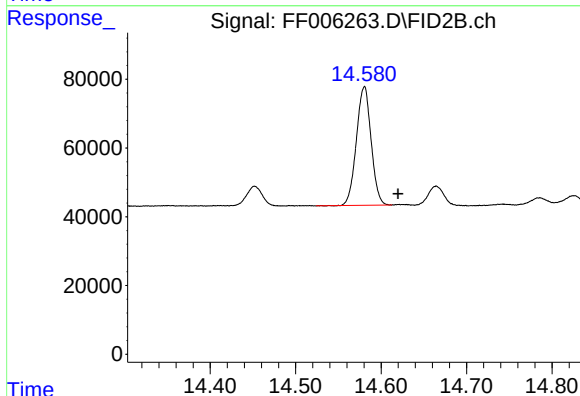


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.581 min
Delta R.T.: -0.040 min
Response: 413472
Conc: 3.82 ug/ml

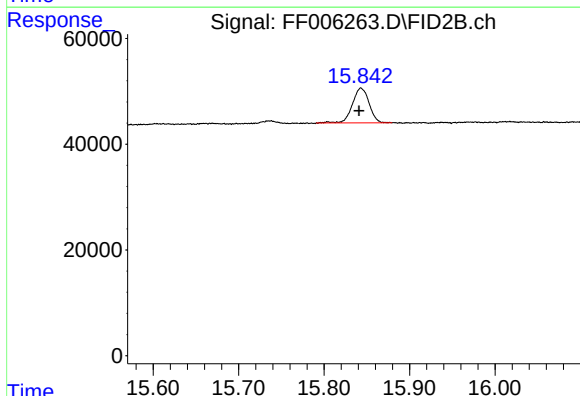


#11 N-HEXACOSANE

R.T.: 15.843 min
Delta R.T.: 0.002 min
Response: 88549
Conc: 0.72 ug/ml

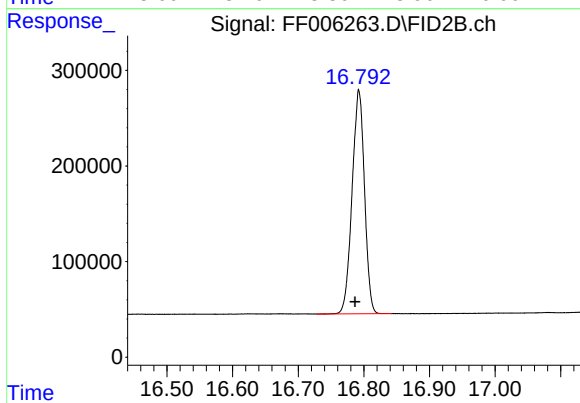

#12 N-OCTACOSANE


R.T.: 16.793 min
Delta R.T.: 0.006 min
Response: 3072124
Conc: 25.27 ug/ml

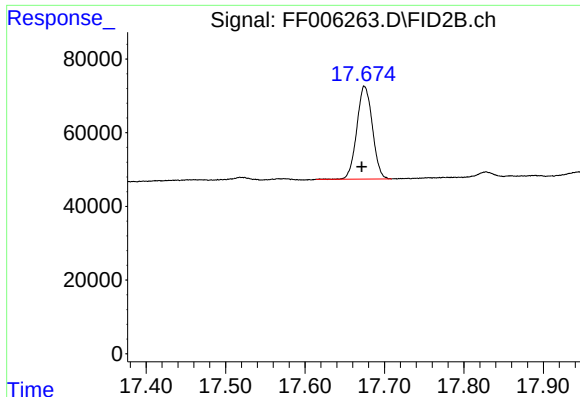

#13 N-TRIACONTANE


R.T.: 17.675 min
Delta R.T.: 0.004 min
Response: 342762
Conc: 2.86 ug/ml

Instrument :
FID_F
ClientSampleId :

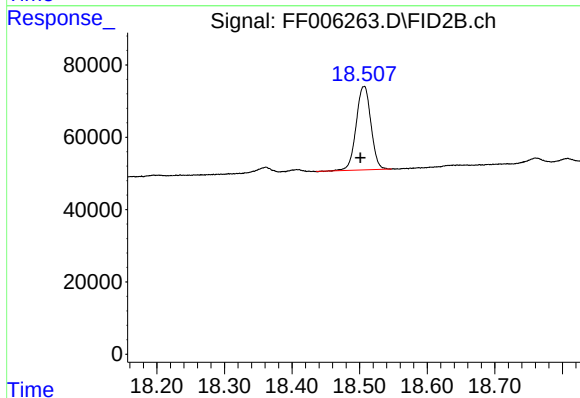


#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: 0.006 min
Response: 349731
Conc: 3.03 ug/ml

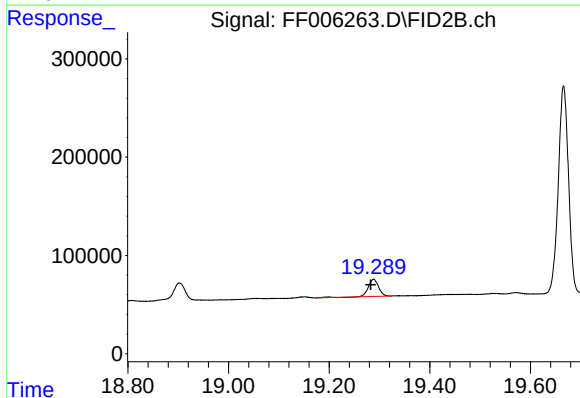


#15 N-TETRATRIACONTANE

R.T.: 19.289 min
Delta R.T.: 0.006 min
Response: 253359
Conc: 2.25 ug/ml

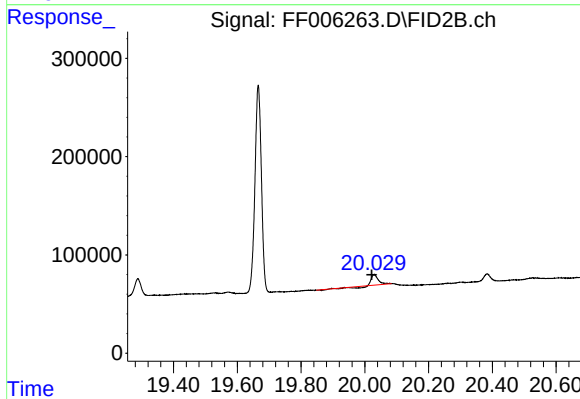

#16 N-HEXATRIACONTANE

R.T.: 20.029 min
Delta R.T.: 0.008 min
Response: 112722
Conc: 1.05 ug/ml

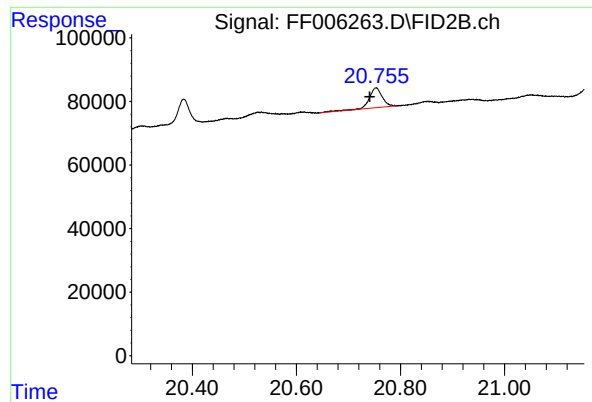

#17 N-OCTATRIACONTANE

R.T.: 20.753 min
Delta R.T.: 0.012 min
Response: 108968
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :