

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012325\
 Data File : FF015280.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jan 2025 15:35
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 05:01:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
 Quant Title :
 QLast Update : Tue Jan 14 11:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.733	2673573	19.545 ug/ml
12) N-OCTACOSANE	17.197	2345447	17.115 ug/ml
13) N-TRIACONTANE	18.084	58577	0.440 ug/ml
14) N-DOTRIACONTANE	18.918	74161	0.584 ug/ml
15) N-TETRATRIACONTANE	19.702	59606	0.538 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012325\
Data File : FF015280.D
Signal(s) : FID2B.ch
Acq On : 23 Jan 2025 15:35
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 05:01:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

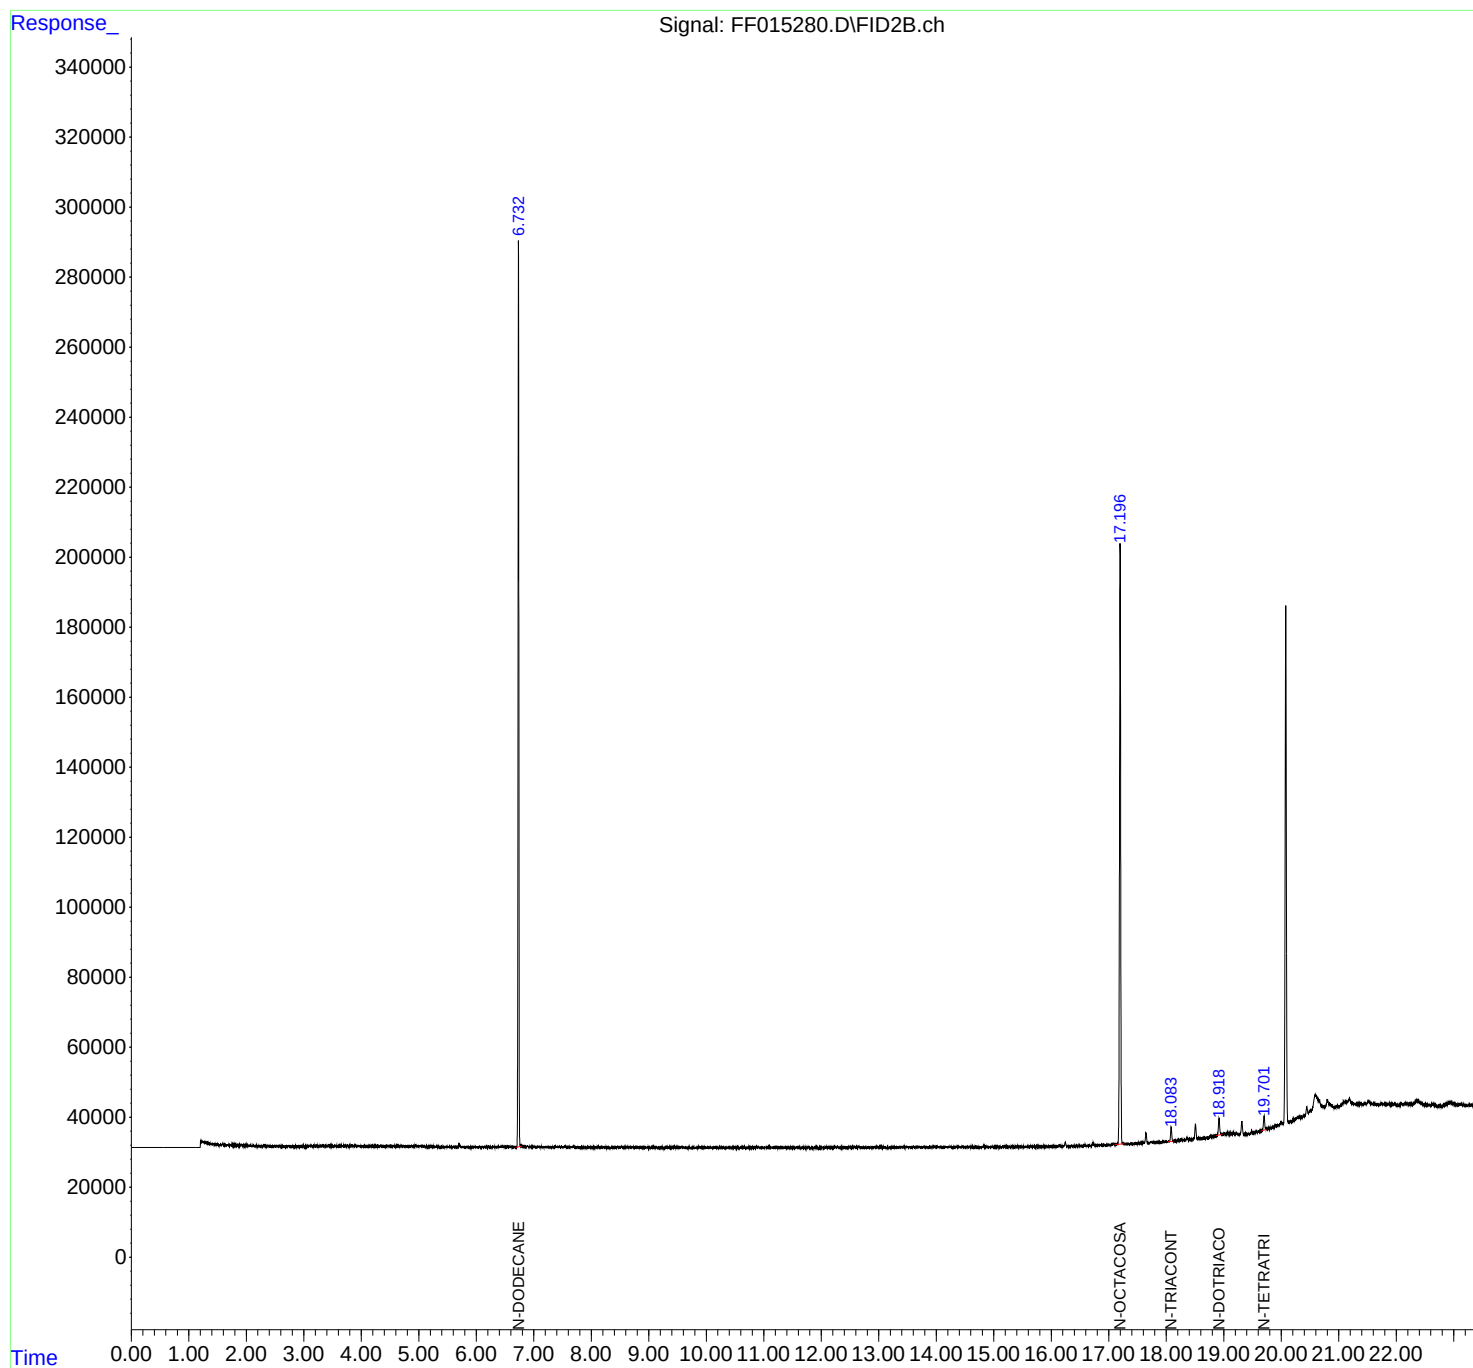


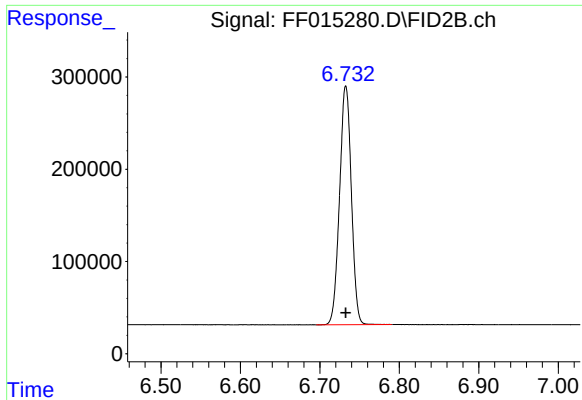

#3 N-DODECANE


R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 2673573
Conc: 19.54 ug/ml

Instrument :
FID_F
ClientSampleId :

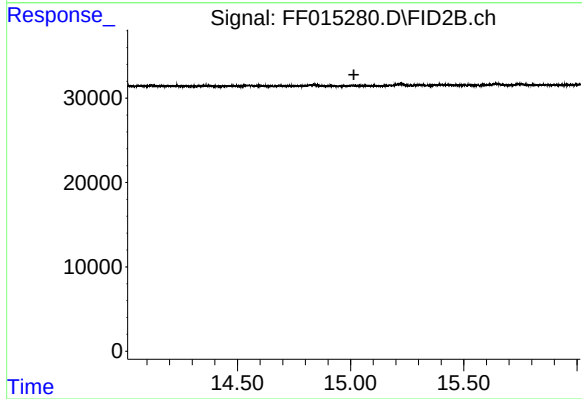


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.015 min
Response: 0
Conc: N.D.

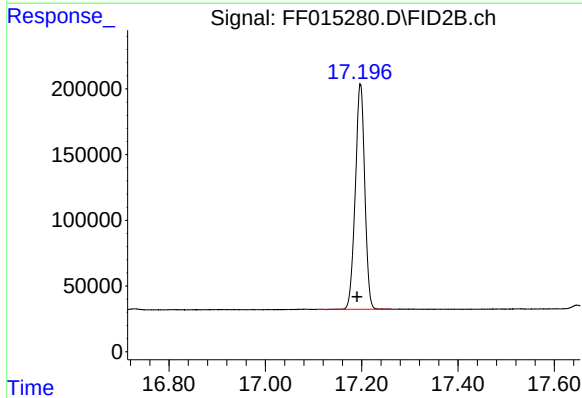


#12 N-OCTACOSANE

R.T.: 17.197 min
Delta R.T.: 0.007 min
Response: 2345447
Conc: 17.11 ug/ml

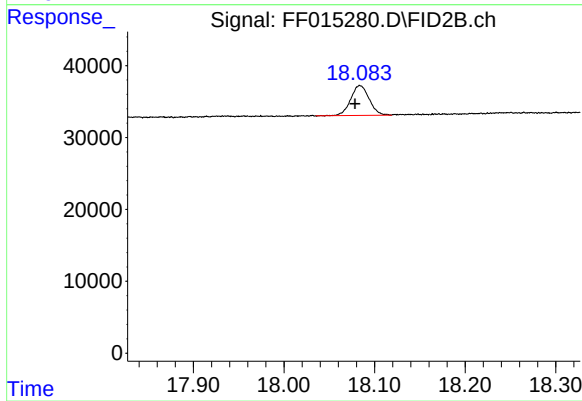

#13 N-TRIACONTANE


R.T.: 18.084 min
Delta R.T.: 0.005 min
Response: 58577
Conc: 0.44 ug/ml

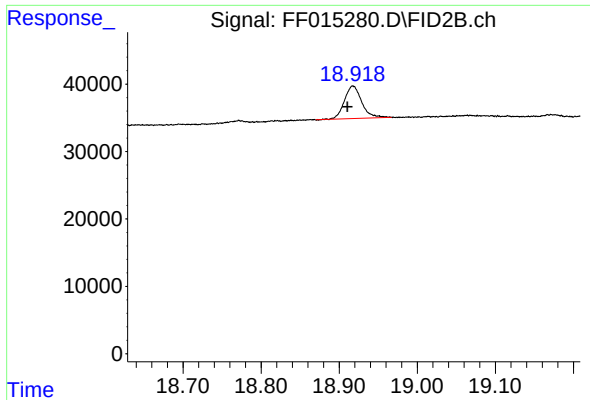

#14 N-DOTRIACONTANE

R.T.: 18.918 min
Delta R.T.: 0.007 min
Response: 74161
Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :

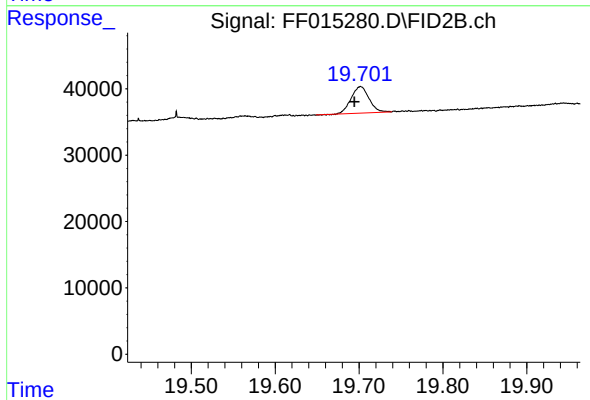

#15 N-TETRATRIACONTANE

R.T.: 19.702 min
Delta R.T.: 0.007 min
Response: 59606
Conc: 0.54 ug/ml