

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006277.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 10:02
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:49:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.579	437962	4.042 ug/ml
Target Compounds			
3) N-DODECANE	6.400	3251689	25.749 ug/ml
11) N-HEXACOSANE	15.842	96621	0.786 ug/ml
12) N-OCTACOSANE	16.790	3284060	27.015 ug/ml
13) N-TRIACONTANE	17.672	419023	3.495 ug/ml
14) N-DOTRIACONTANE	18.502	438412	3.794 ug/ml
15) N-TETRATRIACONTANE	19.283	301597	2.677 ug/ml
16) N-HEXATRIACONTANE	20.025	230717	2.158 ug/ml
17) N-OCTATRIACONTANE	20.745	130493	1.410 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006277.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 10:02
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:49:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

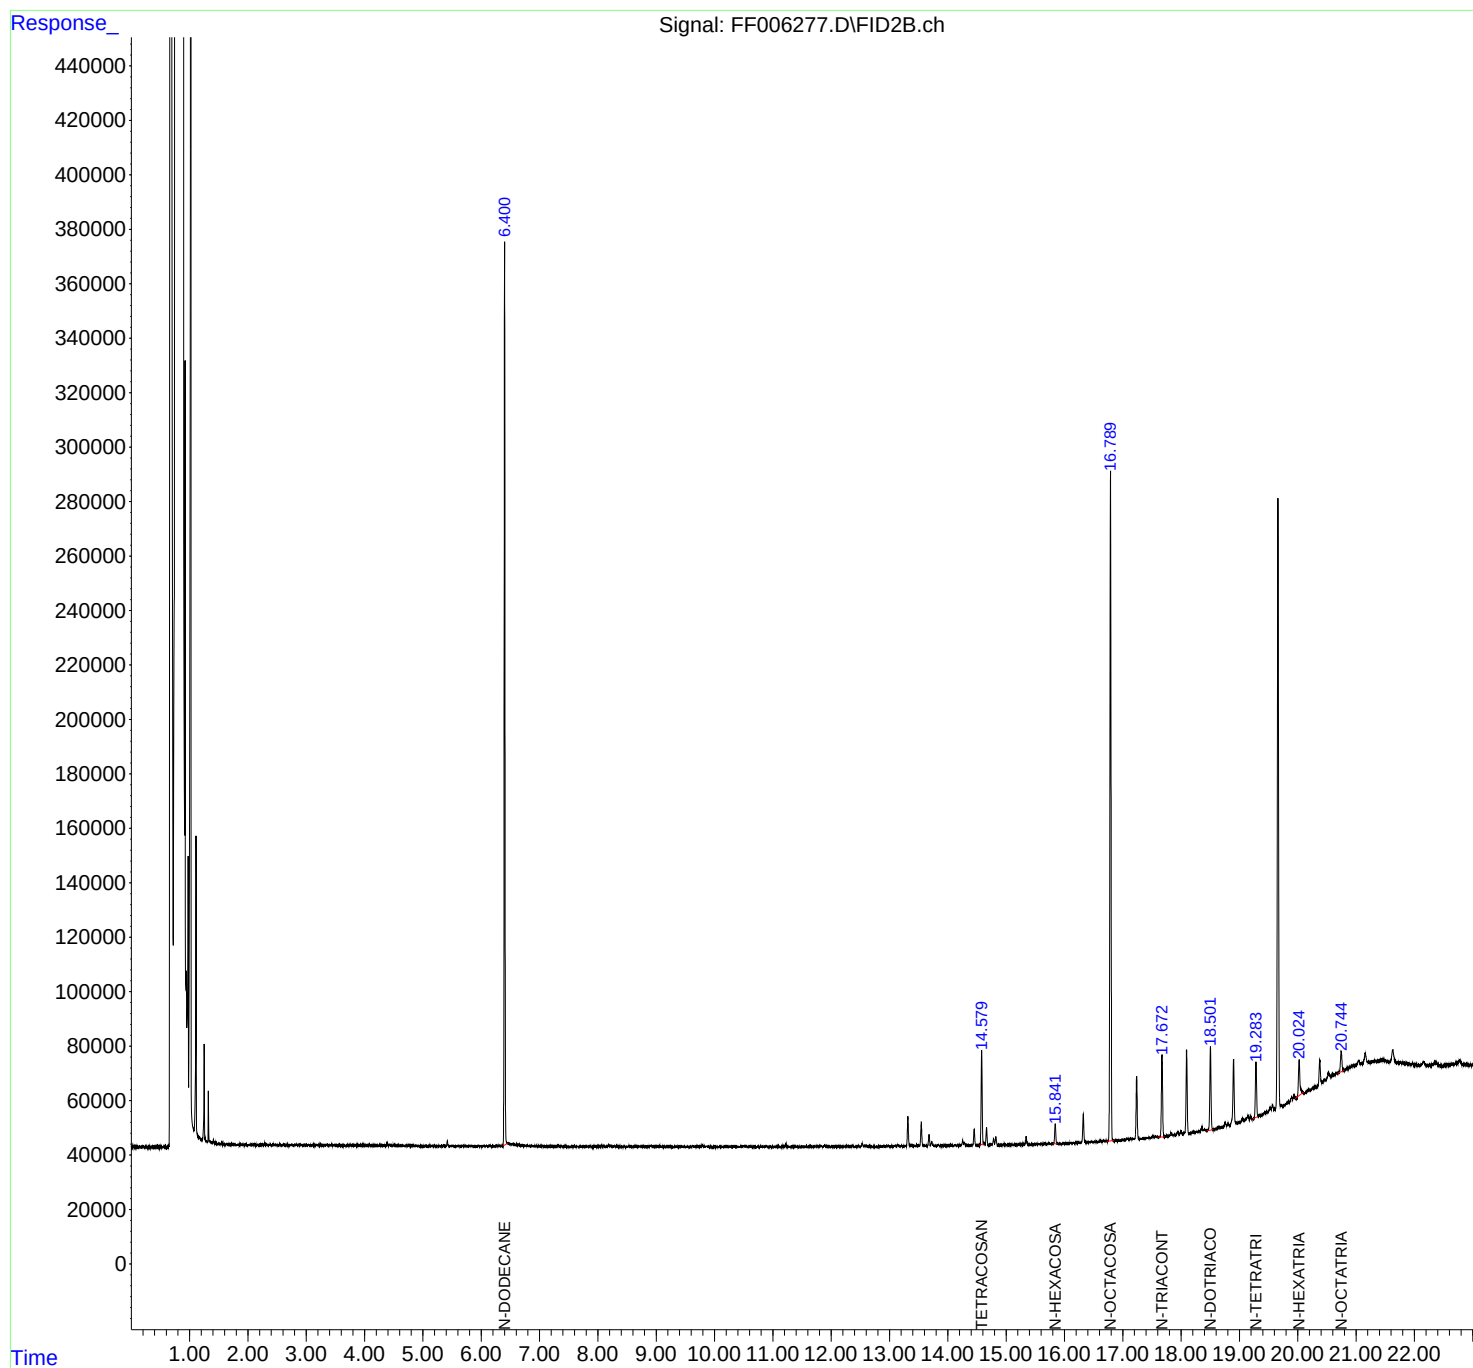


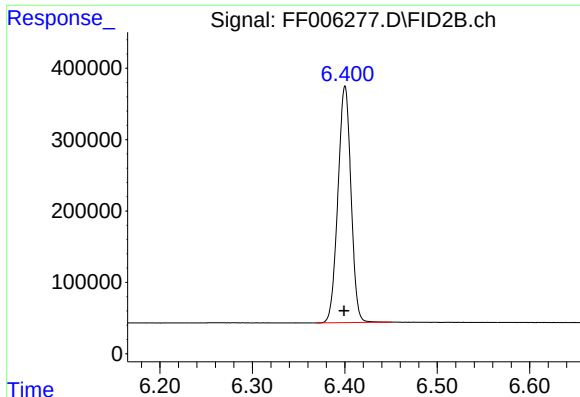

#3 N-DODECANE


R.T.: 6.400 min
Delta R.T.: 0.001 min
Response: 3251689
Conc: 25.75 ug/ml

Instrument :
FID_F
ClientSampleId :

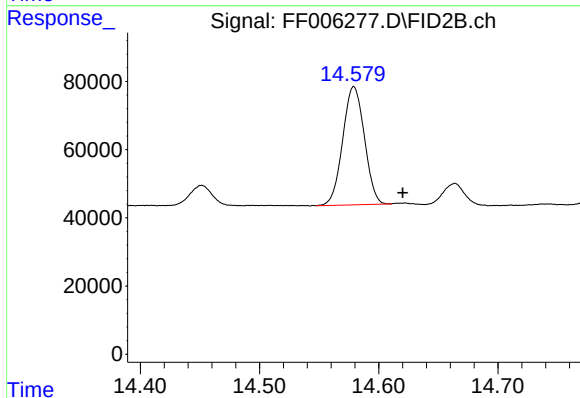


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.579 min
Delta R.T.: -0.041 min
Response: 437962
Conc: 4.04 ug/ml

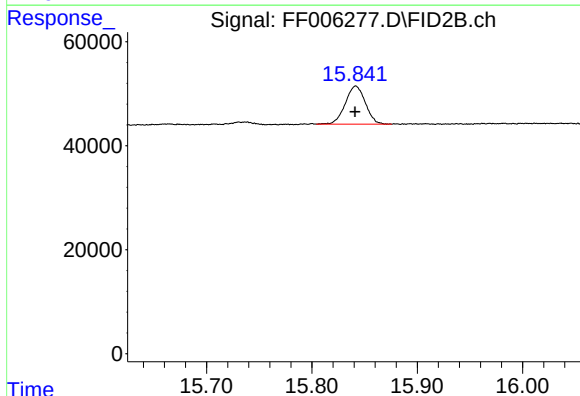


#11 N-HEXACOSANE

R.T.: 15.842 min
Delta R.T.: 0.000 min
Response: 96621
Conc: 0.79 ug/ml

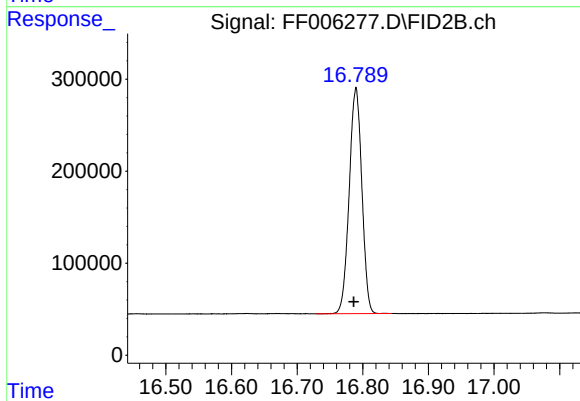

#12 N-OCTACOSANE


R.T.: 16.790 min
Delta R.T.: 0.003 min
Response: 3284060
Conc: 27.02 ug/ml

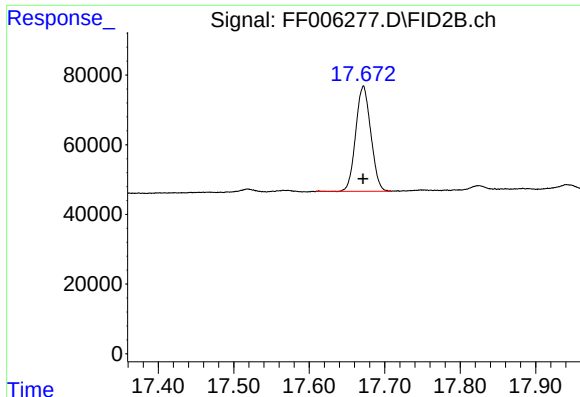

#13 N-TRIACONTANE


R.T.: 17.672 min
Delta R.T.: 0.000 min
Response: 419023
Conc: 3.49 ug/ml

Instrument :
FID_F
ClientSampleId :

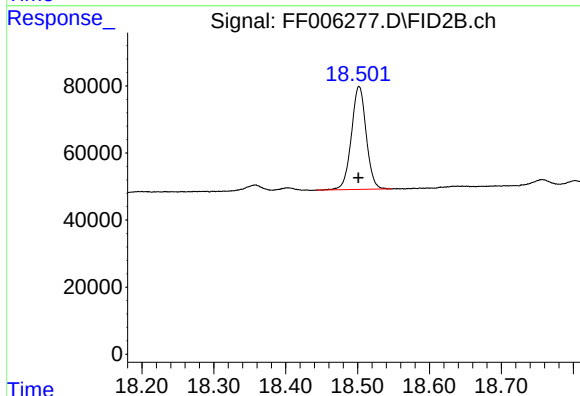


#14 N-DOTRIACONTANE

R.T.: 18.502 min
Delta R.T.: 0.001 min
Response: 438412
Conc: 3.79 ug/ml

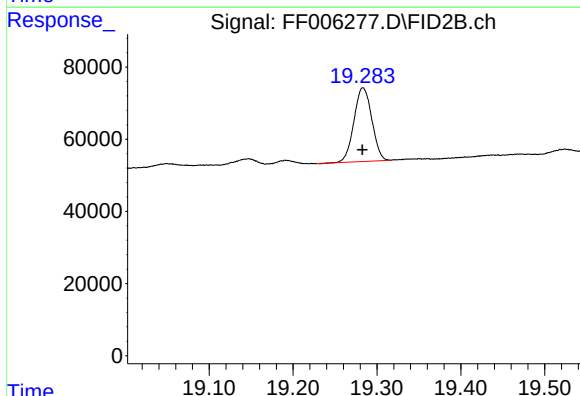


#15 N-TETRATRIACONTANE

R.T.: 19.283 min
Delta R.T.: 0.000 min
Response: 301597
Conc: 2.68 ug/ml

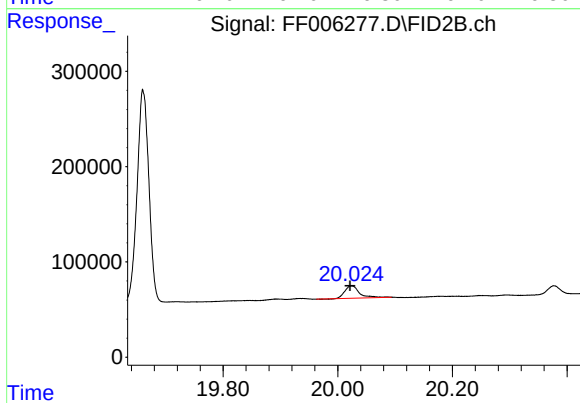

#16 N-HEXATRIACONTANE

R.T.: 20.025 min
Delta R.T.: 0.003 min
Response: 230717
Conc: 2.16 ug/ml

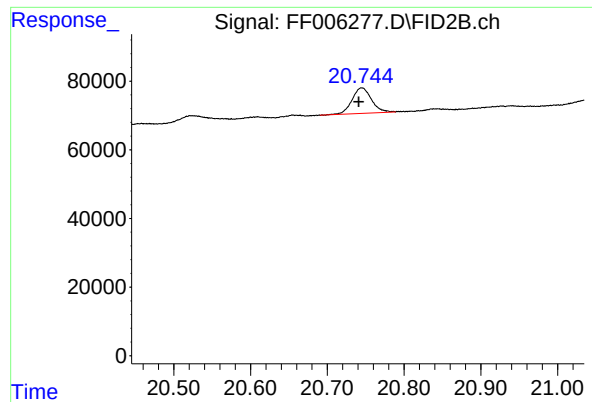

#17 N-OCTATRIACONTANE

R.T.: 20.745 min
Delta R.T.: 0.004 min
Response: 130493
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :