

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012420\  
 Data File : FF006280.D  
 Signal(s) : FID2B.ch  
 Acq On : 24 Jan 2020 15:23  
 Operator : DD\AJ  
 Sample : PB126317BL  
 Misc :  
 ALS Vial : 57 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 24 22:50:05 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011020.M  
 Quant Title :  
 QLast Update : Fri Jan 10 12:35:13 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.628 | 1950942  | 18.004 ug/ml |
| Target Compounds              |        |          |              |
| 11) N-HEXACOSANE              | 15.847 | 247063   | 2.010 ug/ml  |
| 12) N-OCTACOSANE              | 16.795 | 32141    | 0.264 ug/ml  |
| 13) N-TRIACONTANE             | 17.676 | 307979   | 2.569 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.506 | 754773   | 6.531 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.300 | 899256   | 7.982 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.004 | 2309184  | 21.597 ug/ml |
| 17) N-OCTATRIACONTANE         | 20.726 | 3843282  | 41.541 ug/ml |
| 18) N-TETRACONTANE            | 21.657 | 717613   | 7.127 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012420\  
Data File : FF006280.D  
Signal(s) : FID2B.ch  
Acq On : 24 Jan 2020 15:23  
Operator : DD\AJ  
Sample : PB126317BL  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 24 22:50:05 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011020.M  
Quant Title :  
QLast Update : Fri Jan 10 12:35:13 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

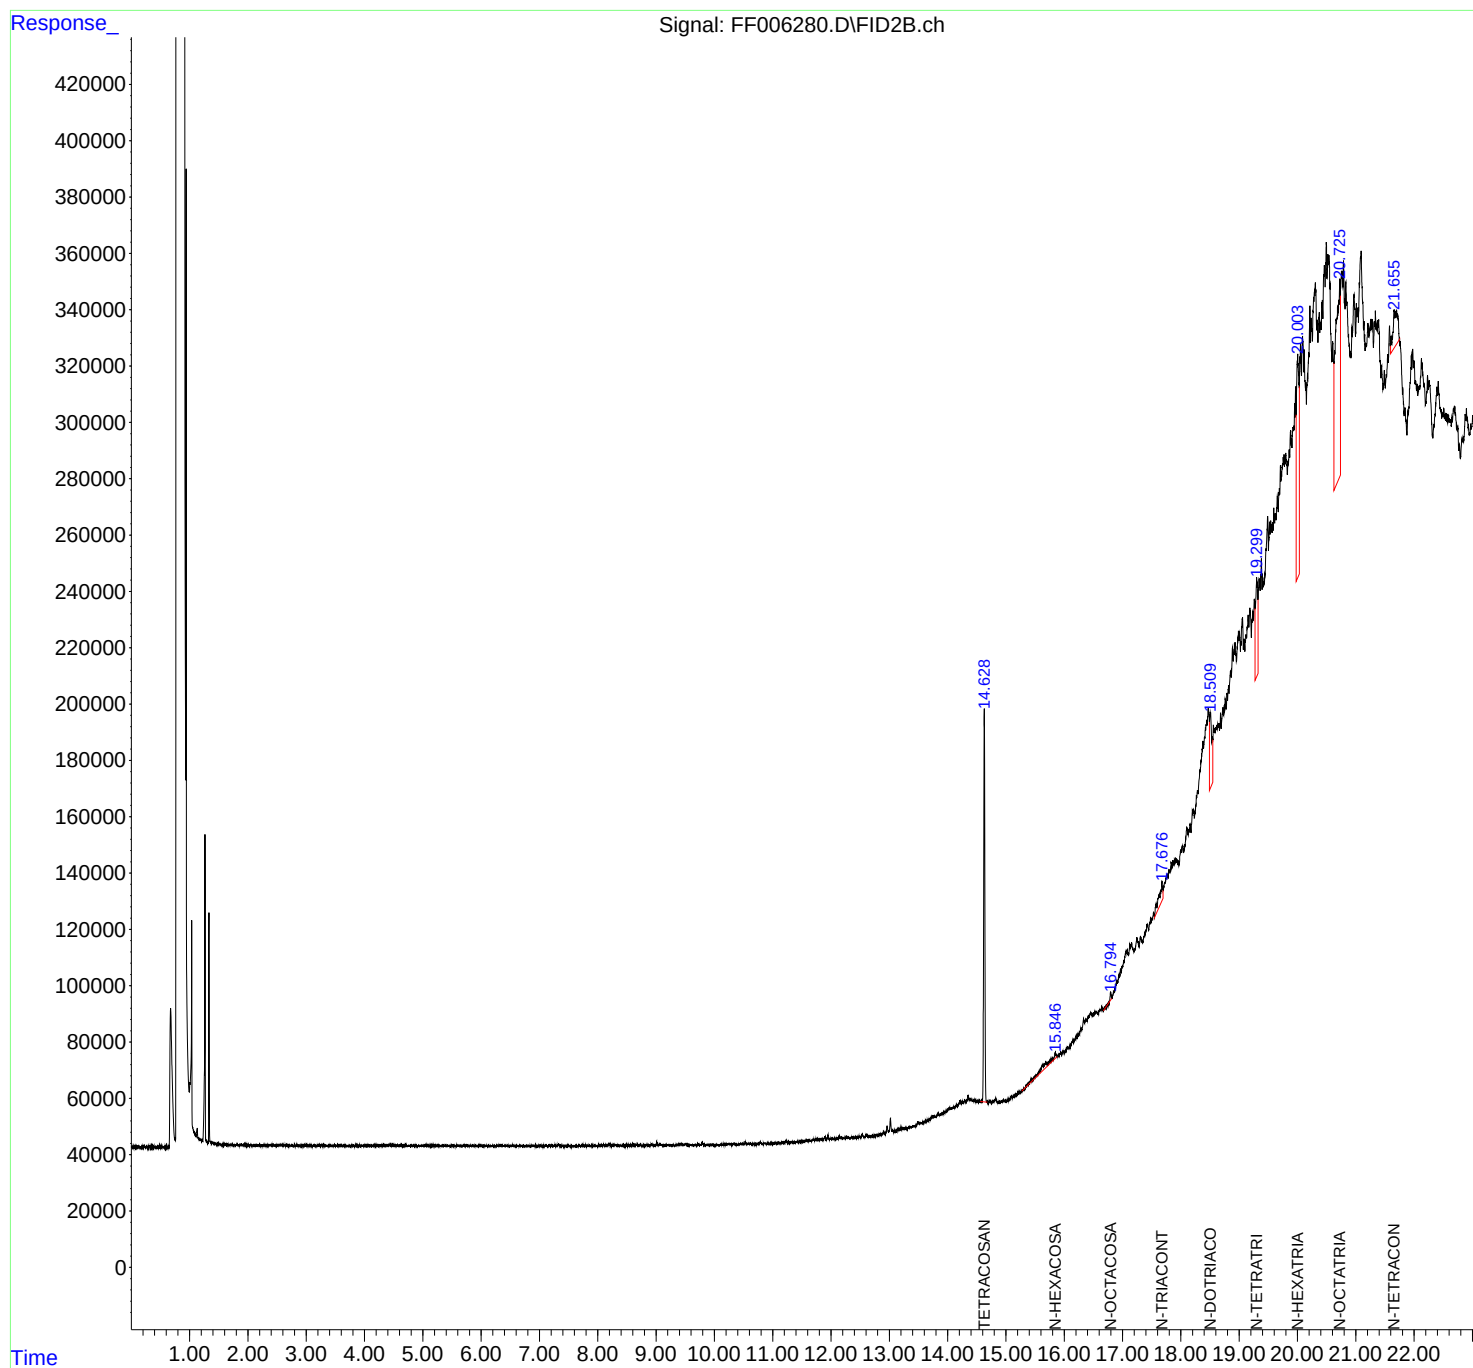


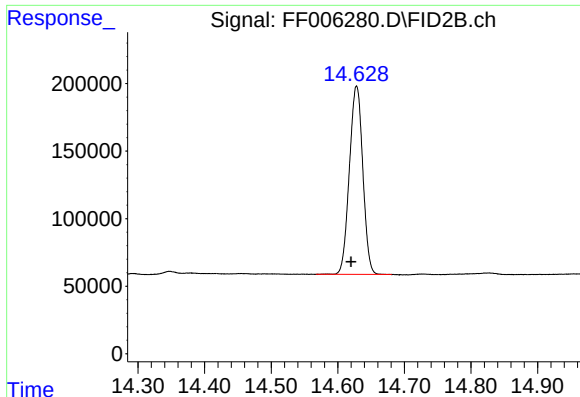

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.628 min  
Delta R.T.: 0.008 min  
Response: 1950942  
Conc: 18.00 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

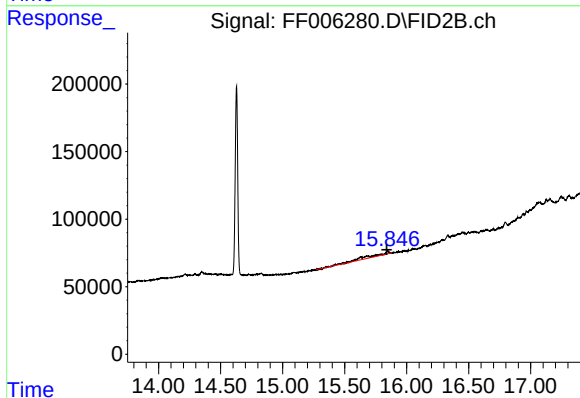


#11 N-HEXACOSANE

R.T.: 15.847 min  
Delta R.T.: 0.006 min  
Response: 247063  
Conc: 2.01 ug/ml

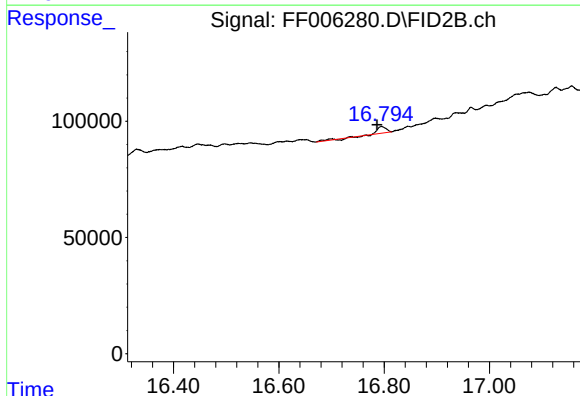


#12 N-OCTACOSANE

R.T.: 16.795 min  
Delta R.T.: 0.009 min  
Response: 32141  
Conc: 0.26 ug/ml

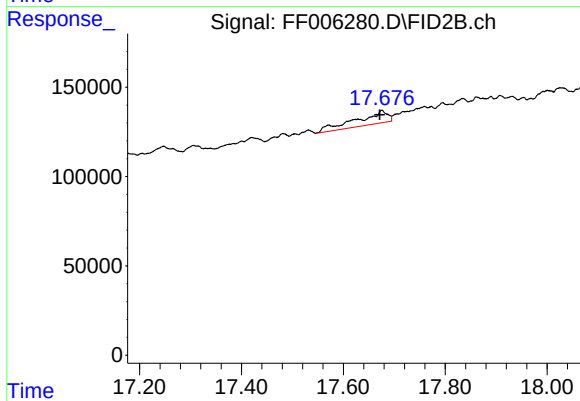

#13 N-TRIACONTANE


R.T.: 17.676 min  
Delta R.T.: 0.004 min  
Response: 307979  
Conc: 2.57 ug/ml

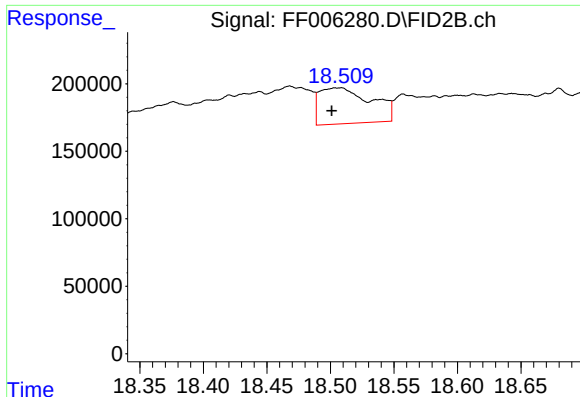

#14 N-DOTRIACONTANE


R.T.: 18.506 min  
Delta R.T.: 0.005 min  
Response: 754773  
Conc: 6.53 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

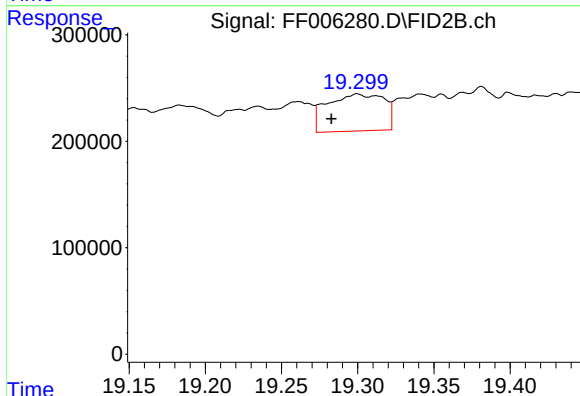


#15 N-TETRATRIACONTANE

R.T.: 19.300 min  
Delta R.T.: 0.017 min  
Response: 899256  
Conc: 7.98 ug/ml

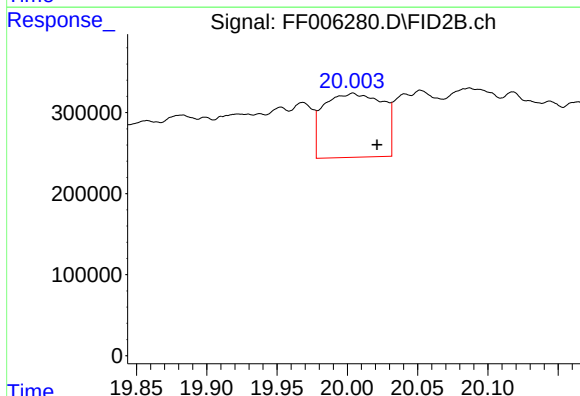


#16 N-HEXATRIACONTANE

R.T.: 20.004 min  
Delta R.T.: -0.017 min  
Response: 2309184  
Conc: 21.60 ug/ml

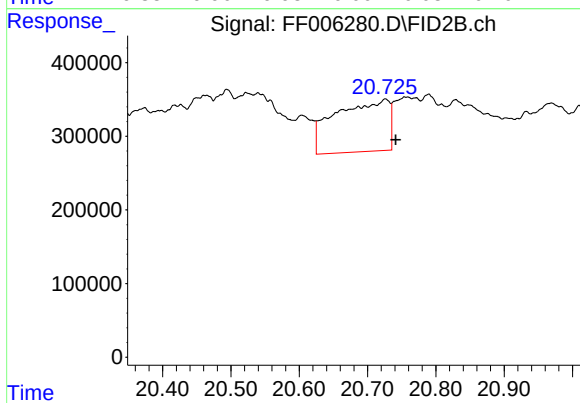

#17 N-OCTATRIACONTANE

R.T.: 20.726 min  
Delta R.T.: -0.015 min  
Response: 3843282  
Conc: 41.54 ug/ml

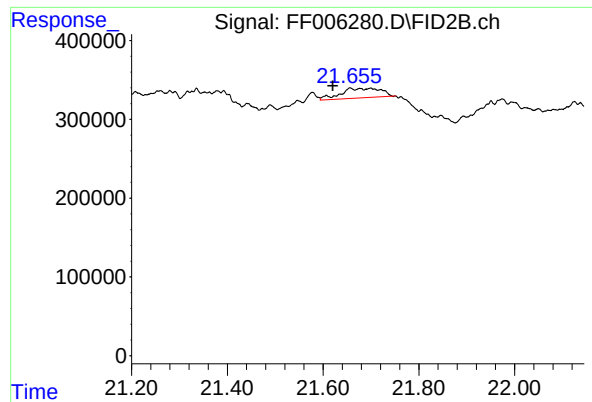

#18 N-TETRACONTANE

R.T.: 21.657 min  
Delta R.T.: 0.036 min  
Response: 717613  
Conc: 7.13 ug/ml

Instrument :  
FID\_F  
ClientSampleId :