

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006282.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 16:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:50:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.629	1939803	17.902 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.512	809568	7.005 ug/ml
15)	N-TETRATRIACONTANE	19.269	65625	0.582 ug/ml
16)	N-HEXATRIACONTANE	20.003	399705	3.738 ug/ml
17)	N-OCTATRIACONTANE	20.760	142356	1.539 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006282.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 16:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:50:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

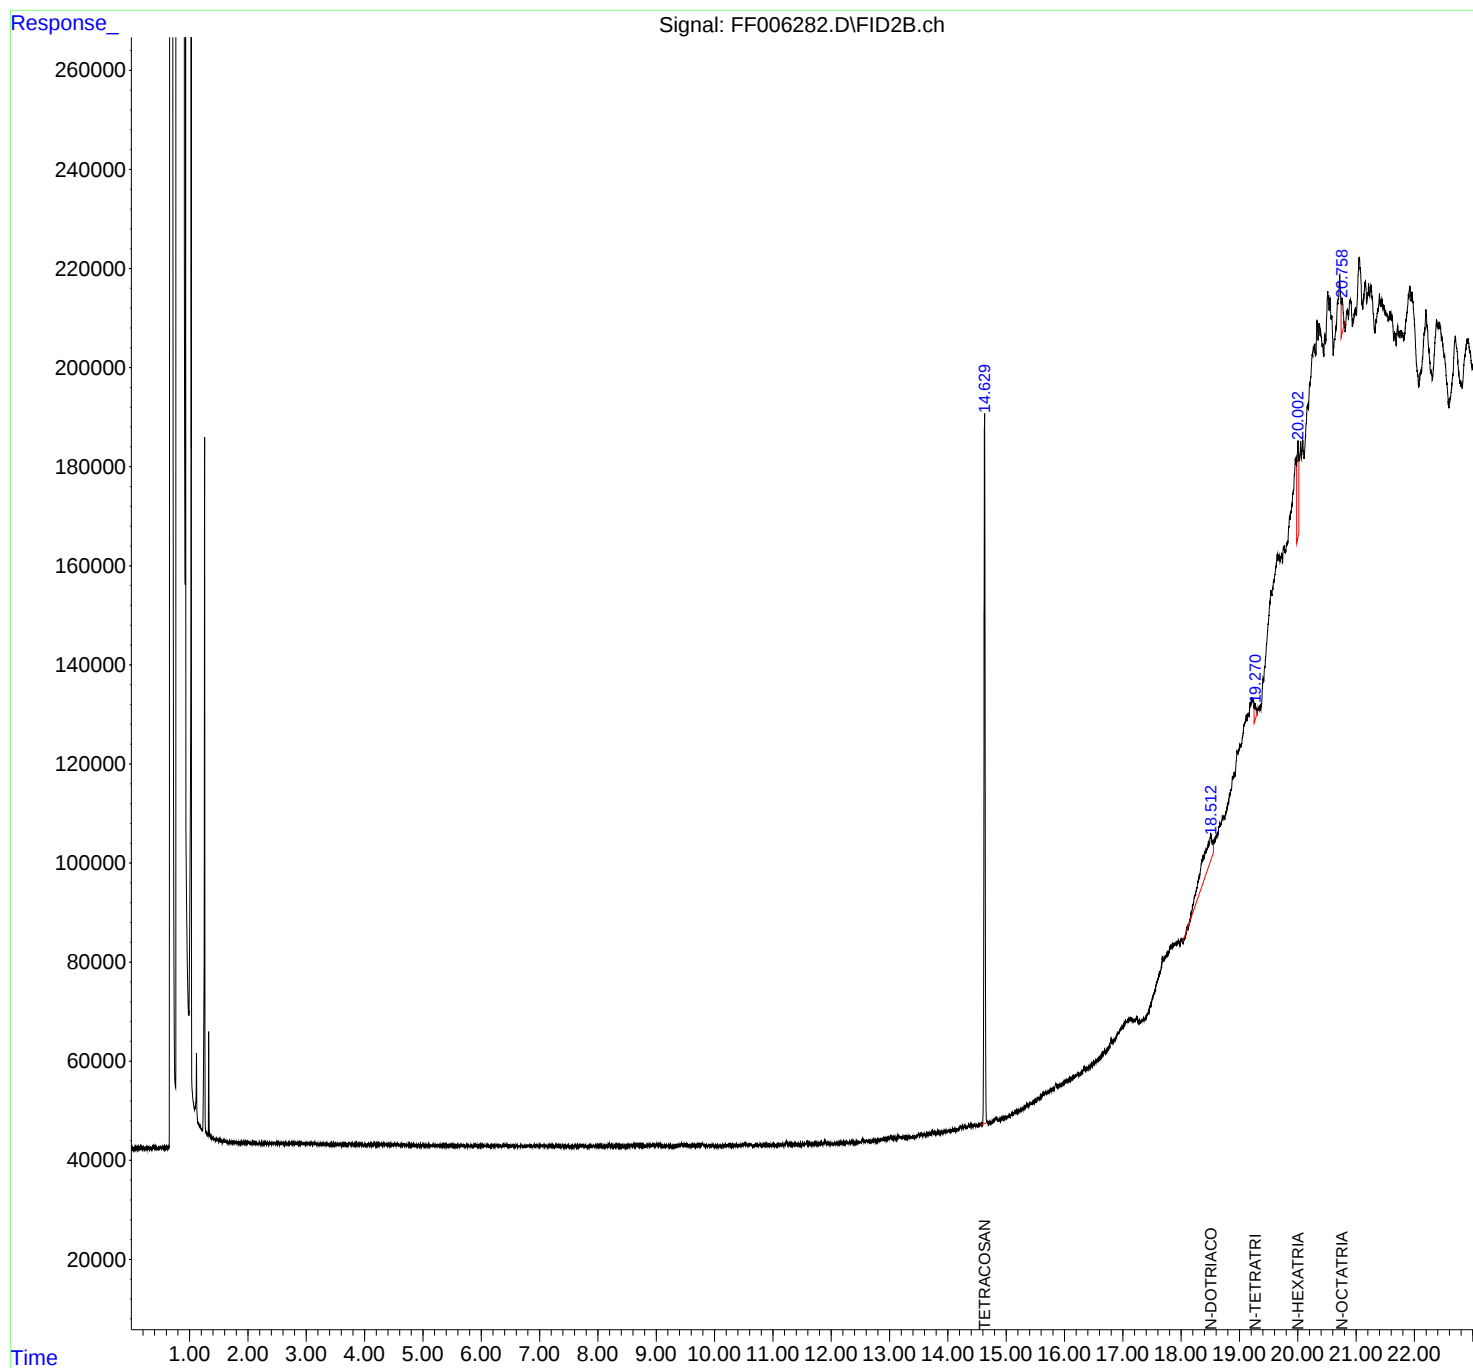


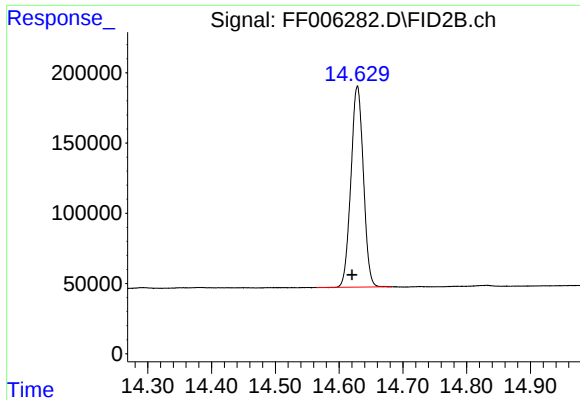

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.629 min
Delta R.T.: 0.009 min
Response: 1939803
Conc: 17.90 ug/ml

Instrument :
FID_F
ClientSampleId :

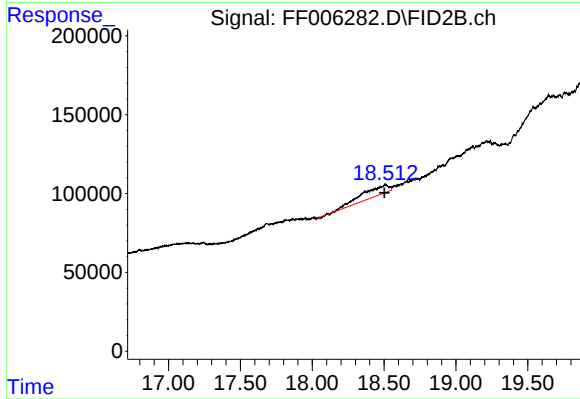


#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: 0.011 min
Response: 809568
Conc: 7.01 ug/ml

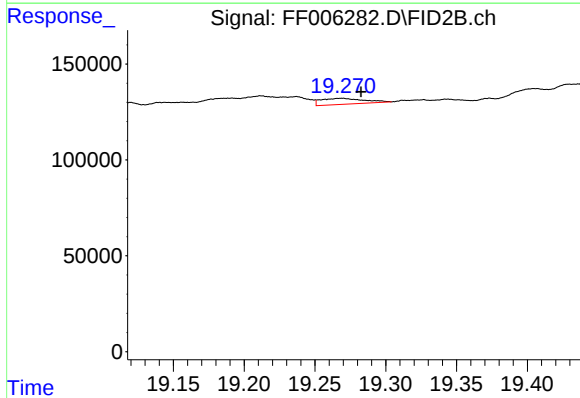


#15 N-TETRATRIACONTANE

R.T.: 19.269 min
Delta R.T.: -0.014 min
Response: 65625
Conc: 0.58 ug/ml

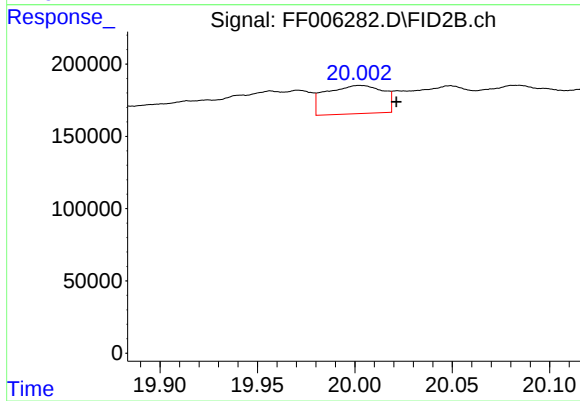

#16 N-HEXATRIACONTANE

R.T.: 20.003 min
Delta R.T.: -0.019 min
Response: 399705
Conc: 3.74 ug/ml

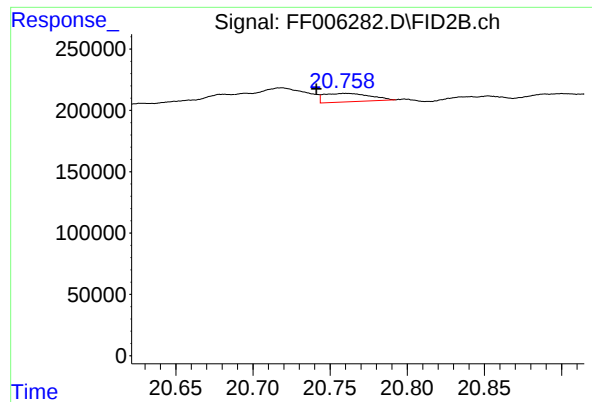

#17 N-OCTATRIACONTANE

R.T.: 20.760 min
Delta R.T.: 0.019 min
Response: 142356
Conc: 1.54 ug/ml

Instrument :
FID_F
ClientSampleId :