

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006284.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 17:23
 Operator : DD\AJ
 Sample : L1247-22
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:51:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	1980603	18.278 ug/ml
Target Compounds			
4) N-TETRADECANE	8.252f	625979	4.959 ug/ml
11) N-HEXACOSANE	15.848	127956	1.041 ug/ml
12) N-OCTACOSANE	16.795	332813	2.738 ug/ml
13) N-TRIACONTANE	17.680	363395	3.031 ug/ml
14) N-DOTRIACONTANE	18.507	540997	4.681 ug/ml
15) N-TETRATRIACONTANE	19.292	109208	0.969 ug/ml
16) N-HEXATRIACONTANE	20.035	568154	5.314 ug/ml
17) N-OCTATRIACONTANE	20.758	170678	1.845 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006284.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 17:23
Operator : DD\AJ
Sample : L1247-22
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 24 22:51:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

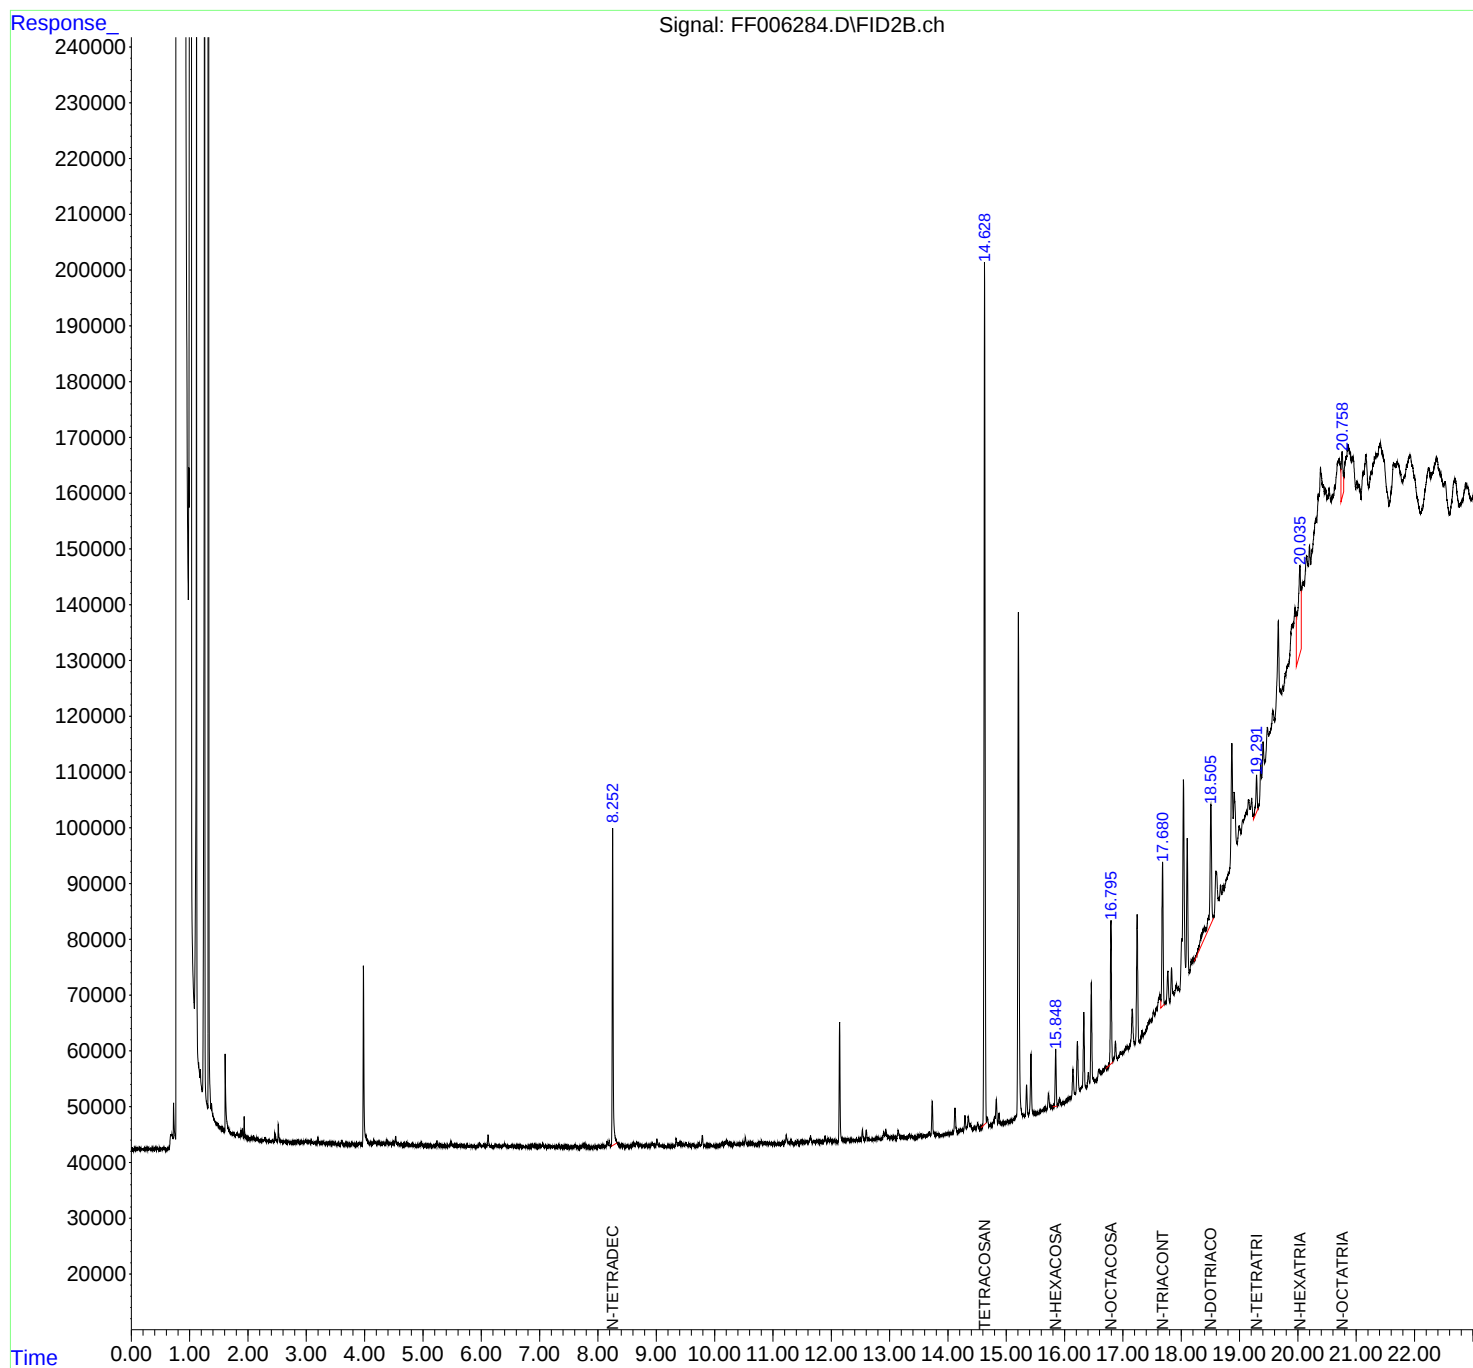


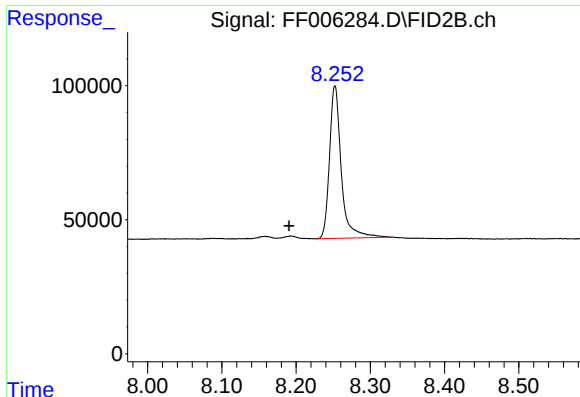

#4 N-TETRADECANE


R.T.: 8.252 min
Delta R.T.: 0.062 min
Response: 625979
Conc: 4.96 ug/ml

Instrument :
FID_F
ClientSampleId :

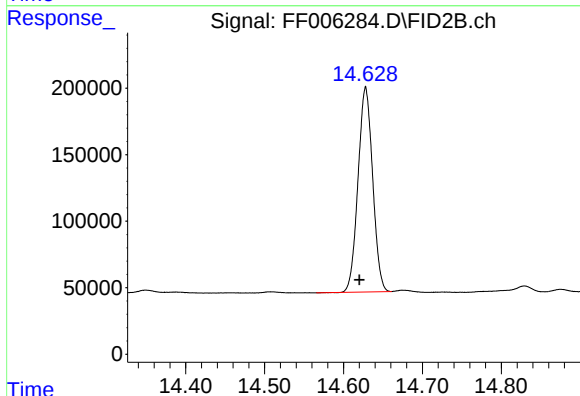


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: 0.008 min
Response: 1980603
Conc: 18.28 ug/ml

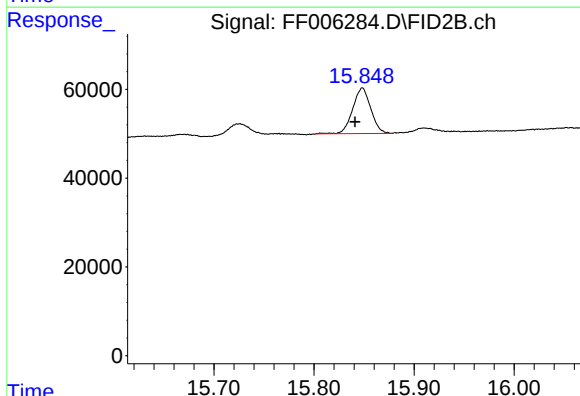


#11 N-HEXACOSANE

R.T.: 15.848 min
Delta R.T.: 0.007 min
Response: 127956
Conc: 1.04 ug/ml

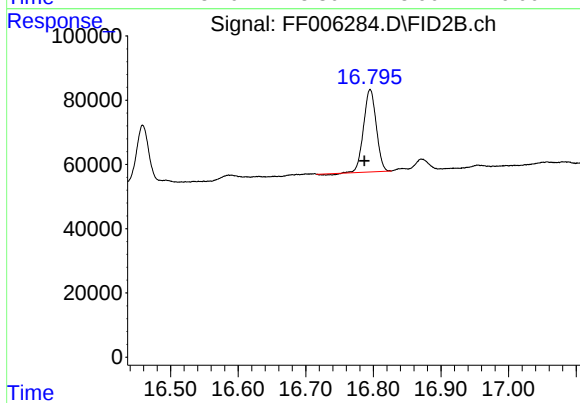

#12 N-OCTACOSANE


R.T.: 16.795 min
Delta R.T.: 0.009 min
Response: 332813
Conc: 2.74 ug/ml

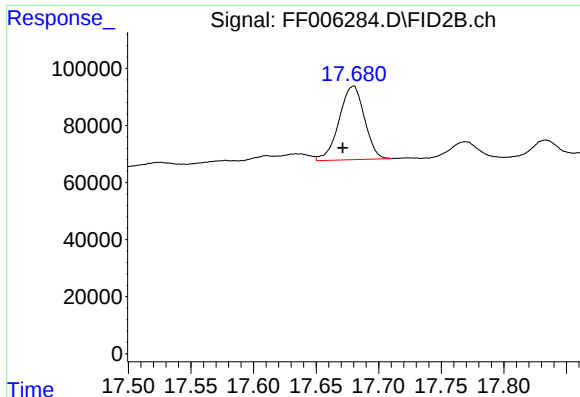

#13 N-TRIACONTANE


R.T.: 17.680 min
Delta R.T.: 0.008 min
Response: 363395
Conc: 3.03 ug/ml

Instrument :
FID_F
ClientSampleId :

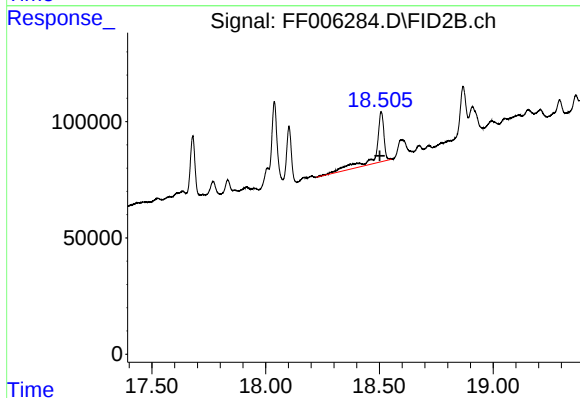


#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: 0.006 min
Response: 540997
Conc: 4.68 ug/ml

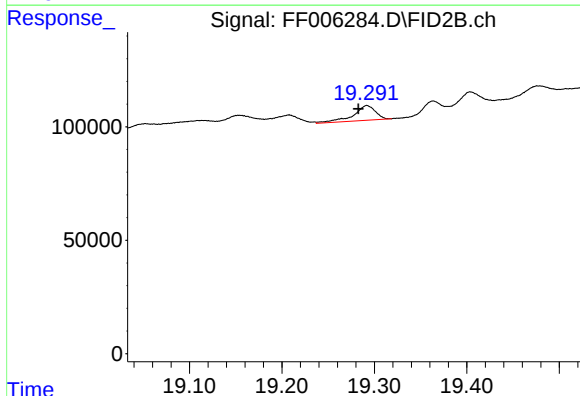


#15 N-TETRATRIACONTANE

R.T.: 19.292 min
Delta R.T.: 0.009 min
Response: 109208
Conc: 0.97 ug/ml

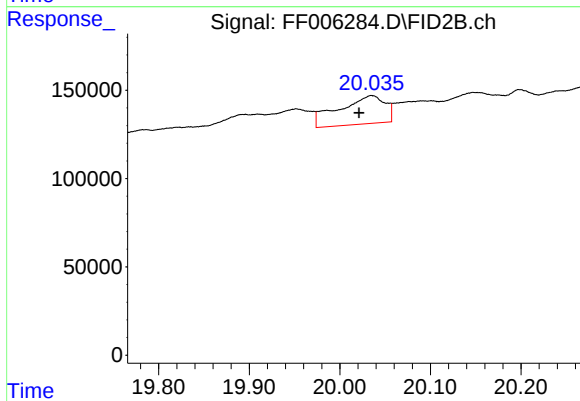

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: 0.014 min
Response: 568154
Conc: 5.31 ug/ml

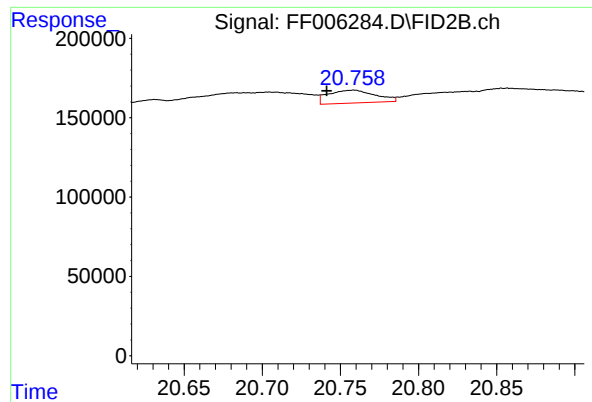

#17 N-OCTATRIACONTANE

R.T.: 20.758 min
Delta R.T.: 0.017 min
Response: 170678
Conc: 1.84 ug/ml

Instrument :
FID_F
ClientSampleId :