

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006285.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 17:53
 Operator : DD\AJ
 Sample : L1247-23
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:51:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	2107211	19.447 ug/ml
Target Compounds			
4) N-TETRADECANE	8.252f	588783	4.665 ug/ml
8) N-DOCOSANE	13.728	107899	0.856 ug/ml
10) N-TETRACOSANE	14.828	155368	1.247 ug/ml
11) N-HEXACOSANE	15.846	185907	1.512 ug/ml
12) N-OCTACOSANE	16.794	394891	3.248 ug/ml
13) N-TRIACONTANE	17.679	383039	3.195 ug/ml
14) N-DOTRIACONTANE	18.505	509322	4.407 ug/ml
15) N-TETRATRIACONTANE	19.292	72164	0.641 ug/ml
16) N-HEXATRIACONTANE	20.058	502024	4.695 ug/ml
18) N-TETRACONTANE	21.645	167117	1.660 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006285.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 17:53
Operator : DD\AJ
Sample : L1247-23
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:51:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

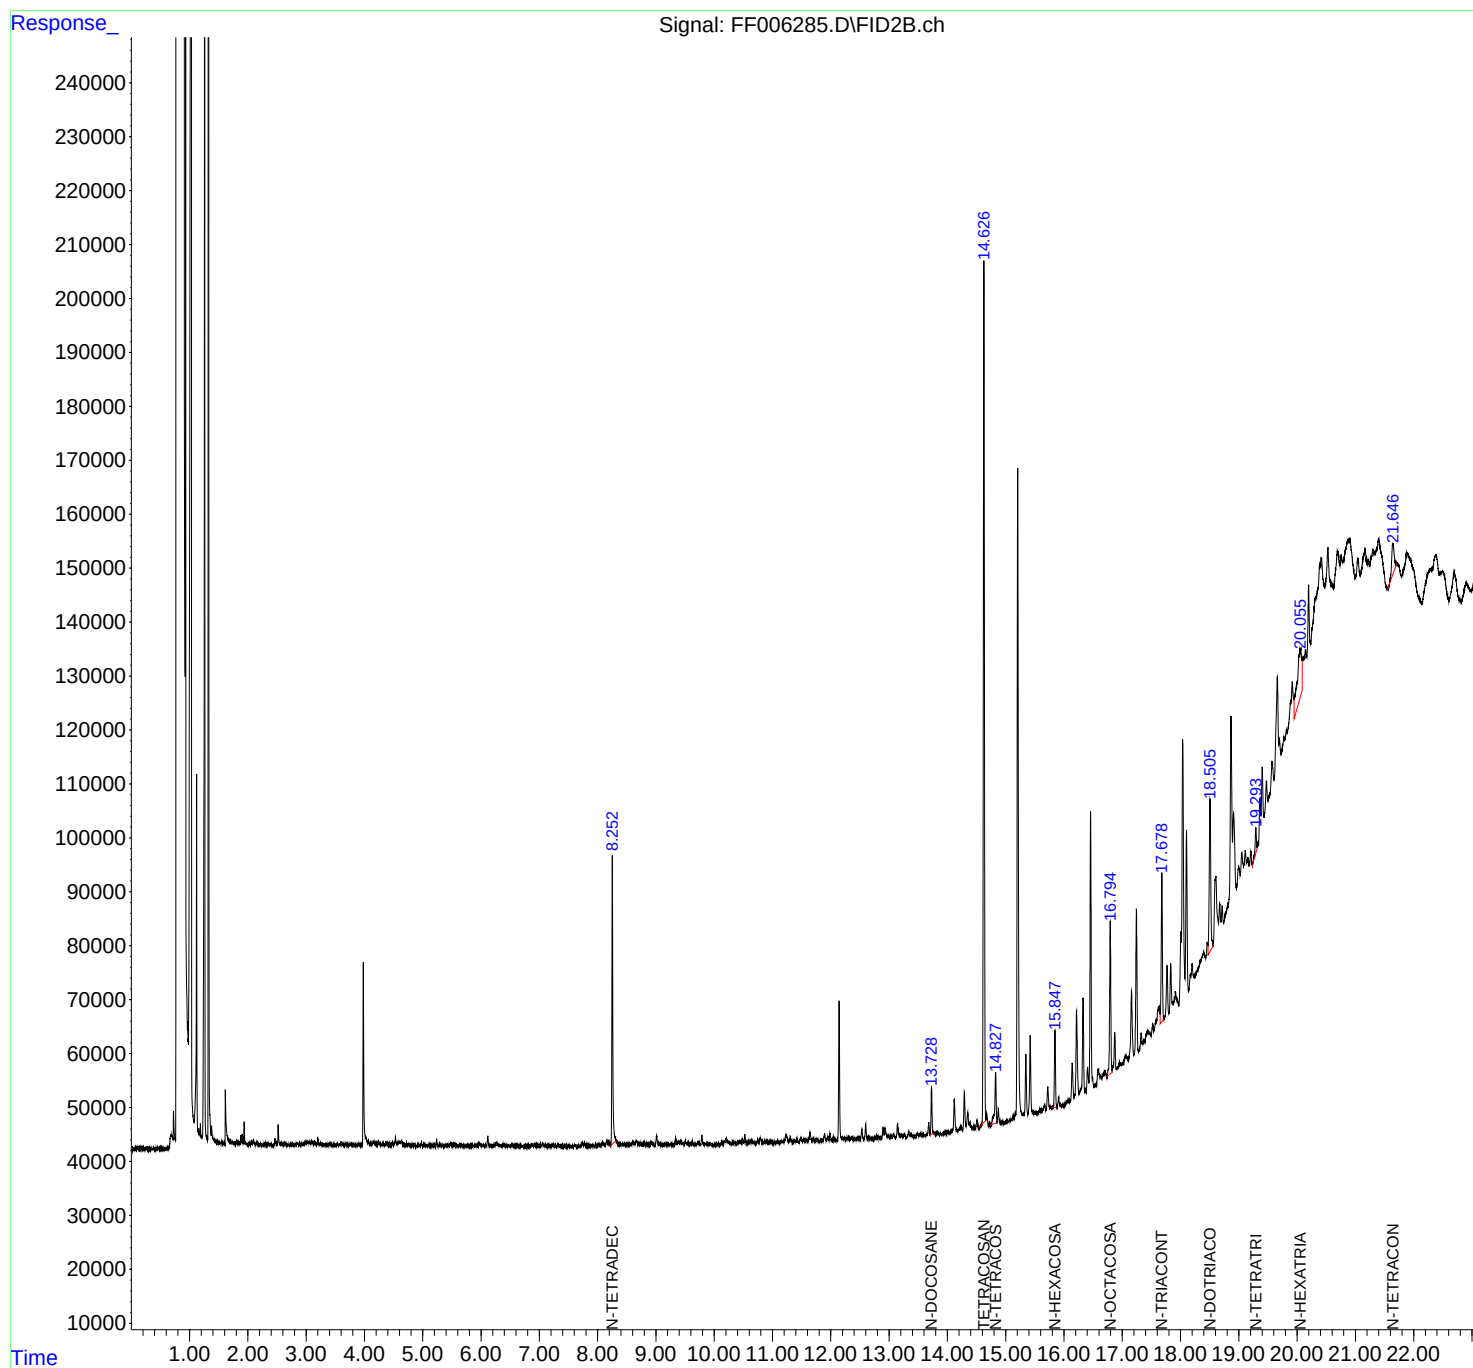


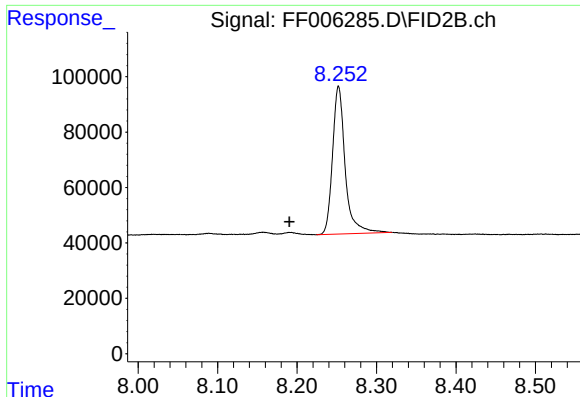

#4 N-TETRADECANE


R.T.: 8.252 min
Delta R.T.: 0.062 min
Response: 588783
Conc: 4.66 ug/ml

Instrument :
FID_F
ClientSampleId :

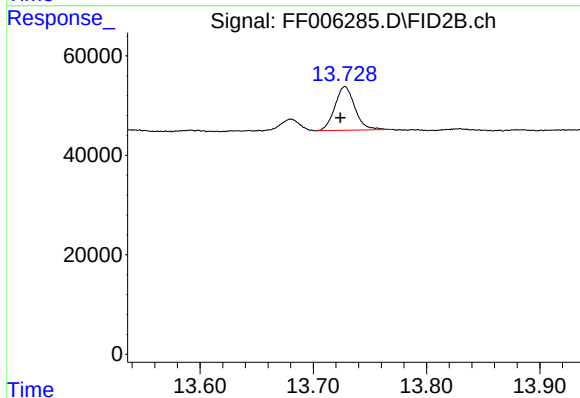


#8 N-DOCOSANE

R.T.: 13.728 min
Delta R.T.: 0.004 min
Response: 107899
Conc: 0.86 ug/ml

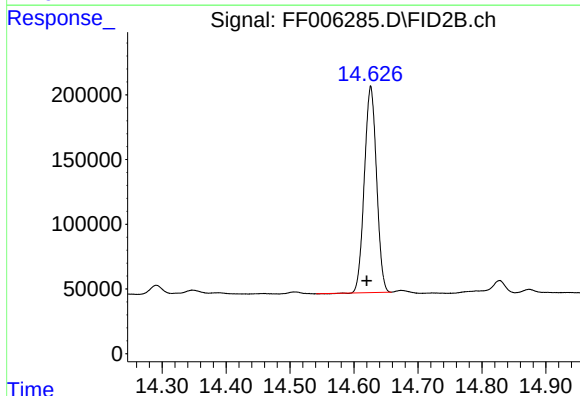


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: 0.006 min
Response: 2107211
Conc: 19.45 ug/ml

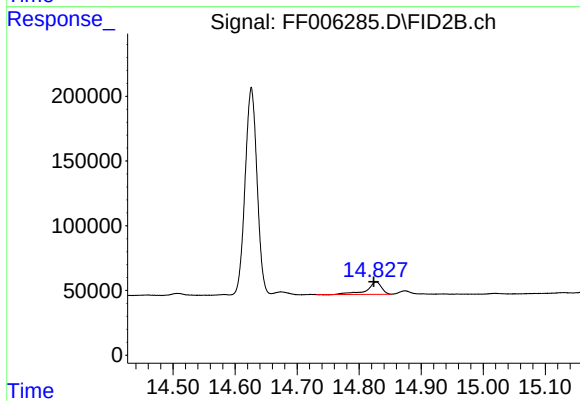

#10 N-TETRACOSANE


R.T.: 14.828 min
Delta R.T.: 0.004 min
Response: 155368
Conc: 1.25 ug/ml

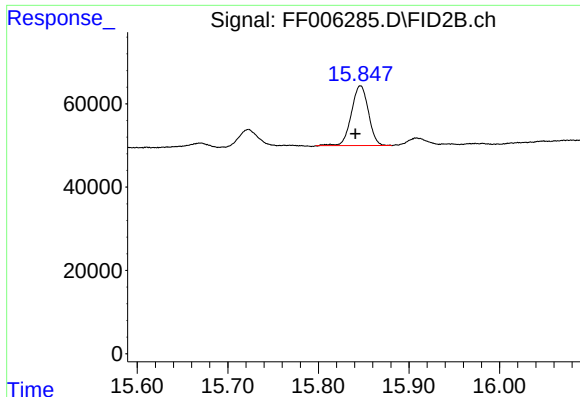

#11 N-HEXACOSANE


R.T.: 15.846 min
Delta R.T.: 0.005 min
Response: 185907
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :

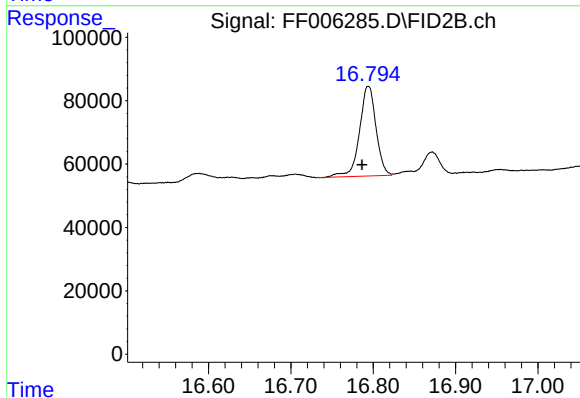


#12 N-OCTACOSANE

R.T.: 16.794 min
Delta R.T.: 0.008 min
Response: 394891
Conc: 3.25 ug/ml

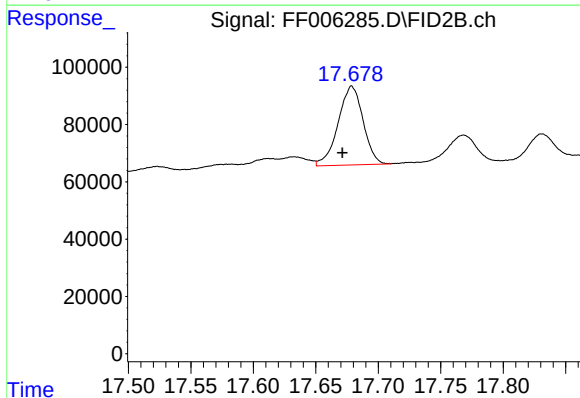


#13 N-TRIACONTANE

R.T.: 17.679 min
Delta R.T.: 0.008 min
Response: 383039
Conc: 3.19 ug/ml

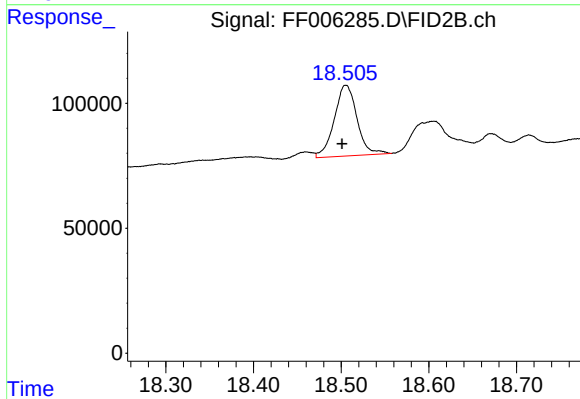

#14 N-DOTRIACONTANE


R.T.: 18.505 min
Delta R.T.: 0.004 min
Response: 509322
Conc: 4.41 ug/ml

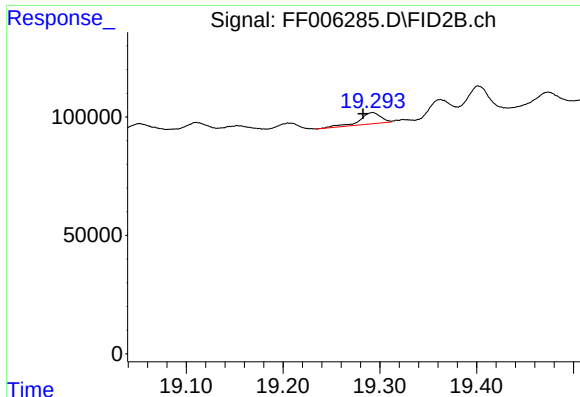

#15 N-TETRATRIACONTANE


R.T.: 19.292 min
Delta R.T.: 0.010 min
Response: 72164
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

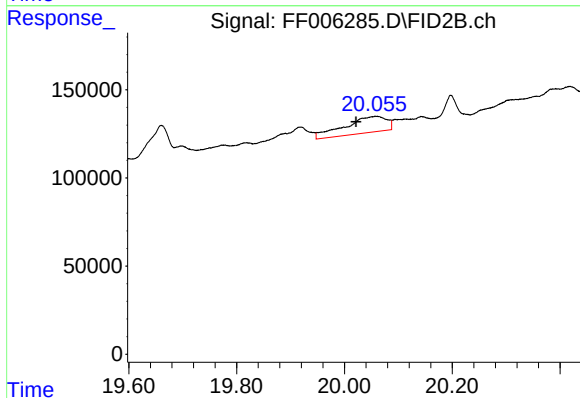

#16 N-HEXATRIACONTANE

R.T.: 20.058 min
Delta R.T.: 0.036 min
Response: 502024
Conc: 4.70 ug/ml

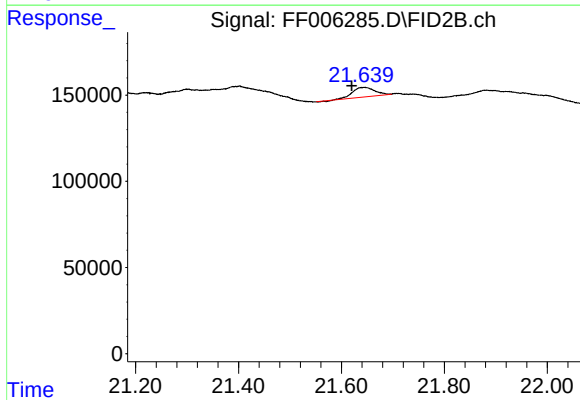

#18 N-TETRACONTANE

R.T.: 21.645 min
Delta R.T.: 0.024 min
Response: 167117
Conc: 1.66 ug/ml