

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006286.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 18:24
 Operator : DD\AJ
 Sample : L1247-29
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:51:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	2160192	19.935 ug/ml
Target Compounds			
4) N-TETRADECANE	8.251f	550389	4.360 ug/ml
8) N-DOCOSANE	13.728	121498	0.964 ug/ml
10) N-TETRACOSANE	14.826	187027	1.501 ug/ml
11) N-HEXACOSANE	15.845	317846	2.585 ug/ml
12) N-OCTACOSANE	16.792	613126	5.044 ug/ml
13) N-TRIACONTANE	17.676	592337	4.940 ug/ml
14) N-DOTRIACONTANE	18.505	515889	4.464 ug/ml
15) N-TETRATRIACONTANE	19.289	81267	0.721 ug/ml
17) N-OCTATRIACONTANE	20.692	49125	0.531 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006286.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 18:24
Operator : DD\AJ
Sample : L1247-29
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:51:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

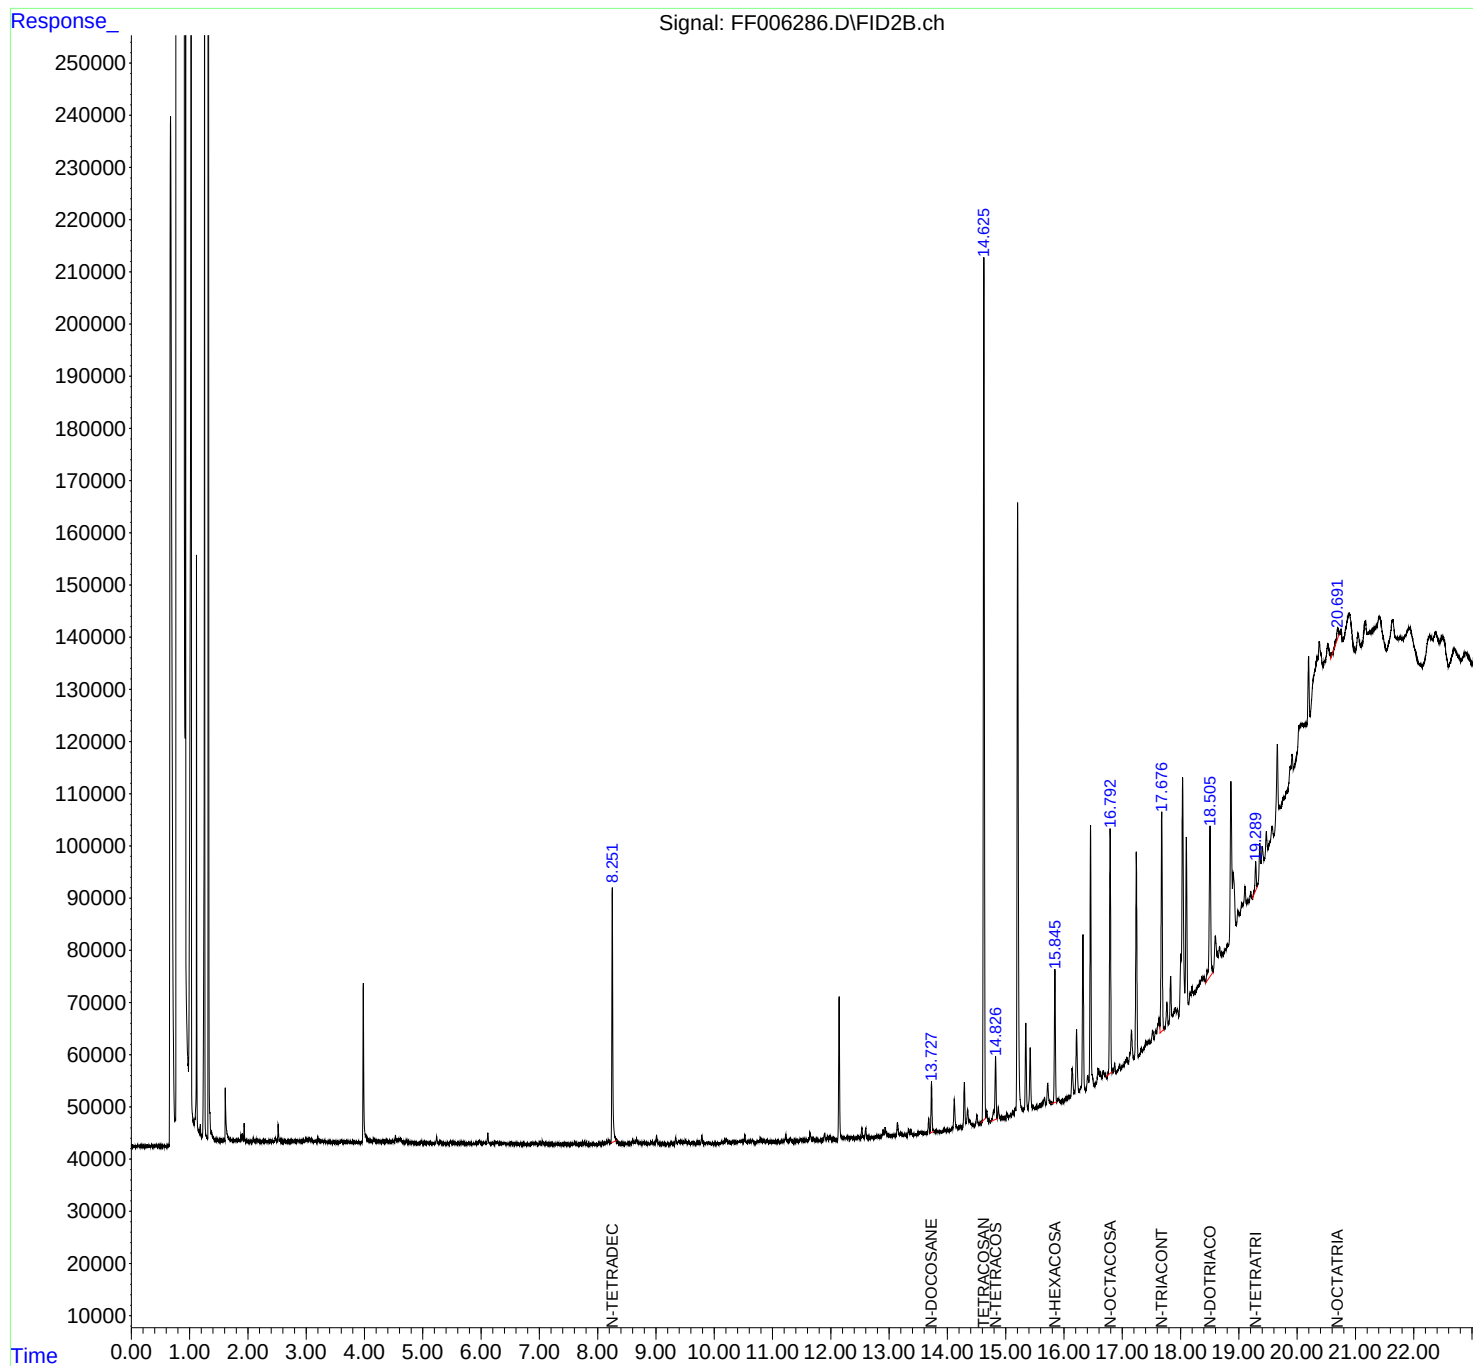


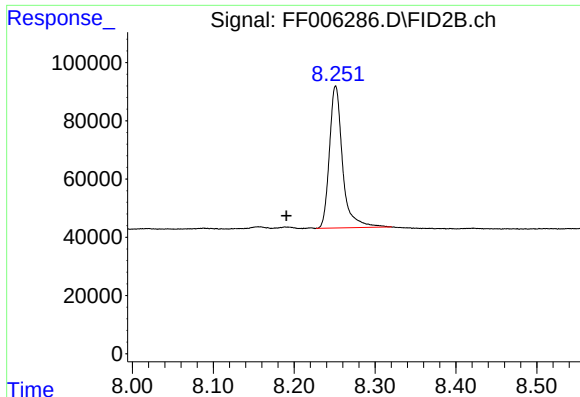

#4 N-TETRADECANE


R.T.: 8.251 min
Delta R.T.: 0.061 min
Response: 550389
Conc: 4.36 ug/ml

Instrument :
FID_F
ClientSampleId :

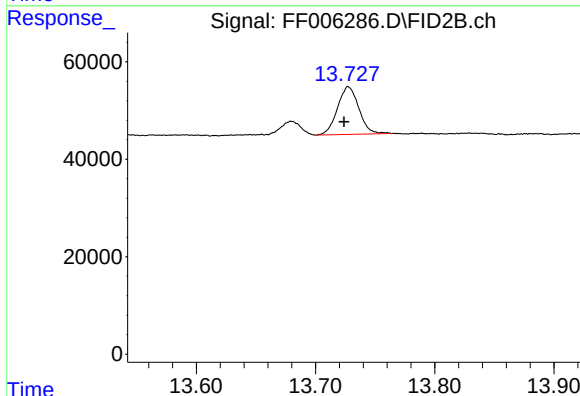


#8 N-DOCOSANE

R.T.: 13.728 min
Delta R.T.: 0.004 min
Response: 121498
Conc: 0.96 ug/ml

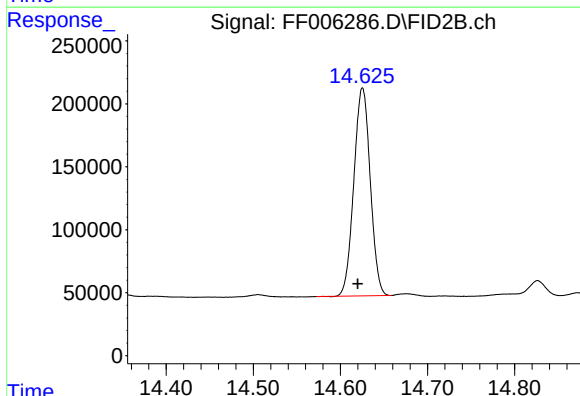


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: 0.005 min
Response: 2160192
Conc: 19.94 ug/ml

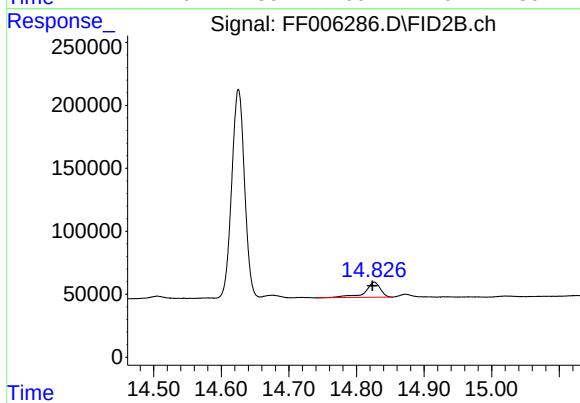

#10 N-TETRACOSANE


R.T.: 14.826 min
Delta R.T.: 0.003 min
Response: 187027
Conc: 1.50 ug/ml

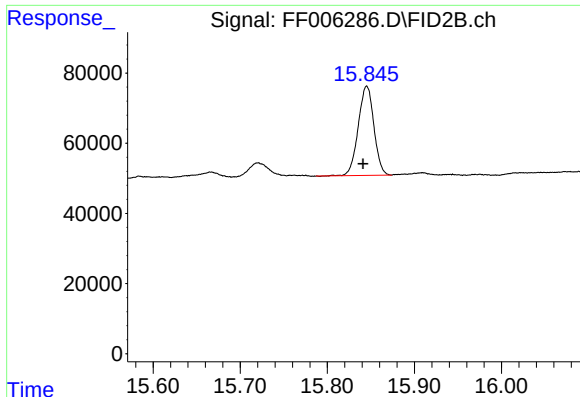

#11 N-HEXACOSANE


R.T.: 15.845 min
Delta R.T.: 0.004 min
Response: 317846
Conc: 2.59 ug/ml

Instrument :
FID_F
ClientSampleId :

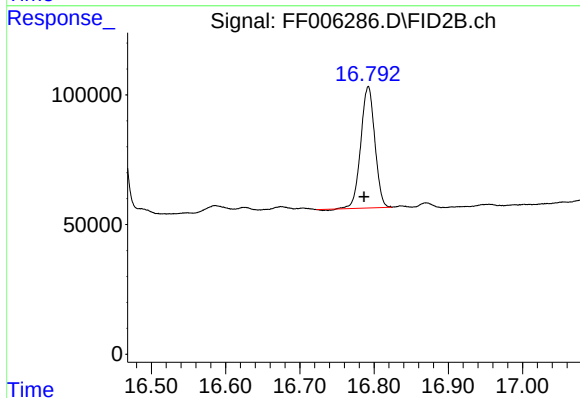


#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: 0.006 min
Response: 613126
Conc: 5.04 ug/ml

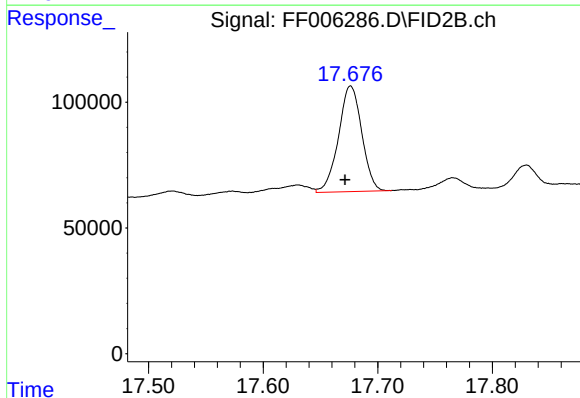


#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: 0.005 min
Response: 592337
Conc: 4.94 ug/ml

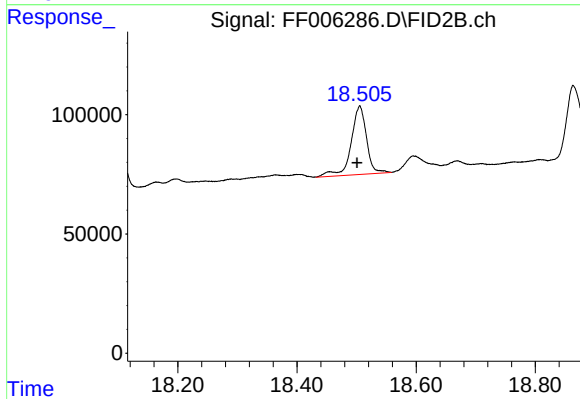

#14 N-DOTRIACONTANE


R.T.: 18.505 min
Delta R.T.: 0.004 min
Response: 515889
Conc: 4.46 ug/ml

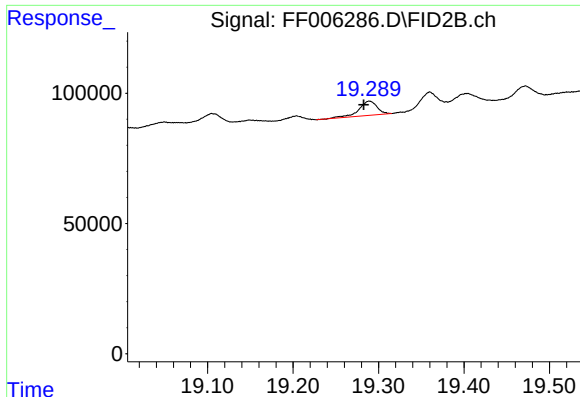

#15 N-TETRATRIACONTANE

R.T.: 19.289 min
Delta R.T.: 0.007 min
Response: 81267
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

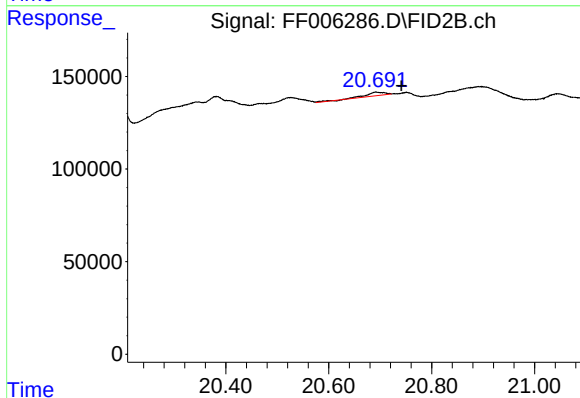

#17 N-OCTATRIACONTANE

R.T.: 20.692 min
Delta R.T.: -0.050 min
Response: 49125
Conc: 0.53 ug/ml