

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006287.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 18:54
 Operator : DD\AJ
 Sample : L1247-30
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:51:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	2536886	23.412 ug/ml
Target Compounds			
4) N-TETRADECANE	8.251f	553258	4.383 ug/ml
8) N-DOCOSANE	13.728	91838	0.728 ug/ml
10) N-TETRACOSANE	14.827	118912	0.955 ug/ml
11) N-HEXACOSANE	15.846	126849	1.032 ug/ml
12) N-OCTACOSANE	16.793	304666	2.506 ug/ml
13) N-TRIACONTANE	17.677	292655	2.441 ug/ml
14) N-DOTRIACONTANE	18.502	336544	2.912 ug/ml
16) N-HEXATRIACONTANE	20.037	224988	2.104 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006287.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 18:54
Operator : DD\AJ
Sample : L1247-30
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:51:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

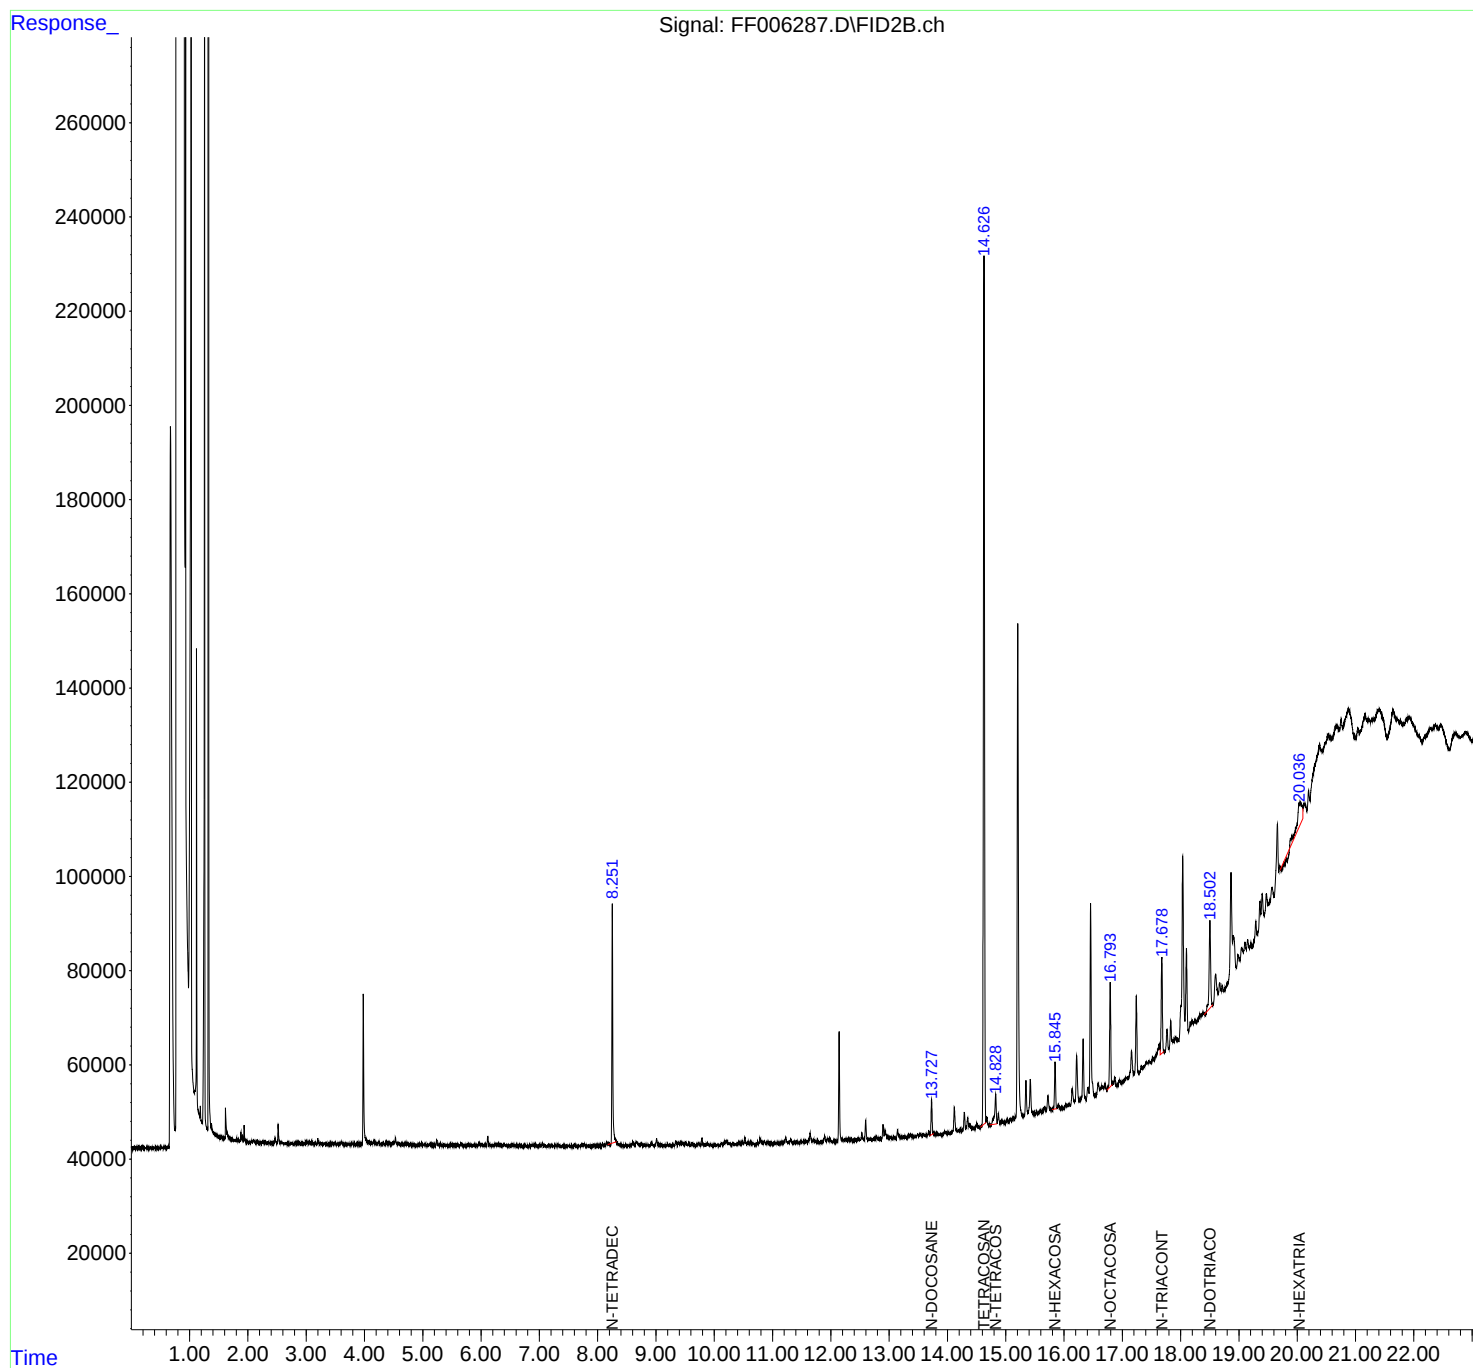


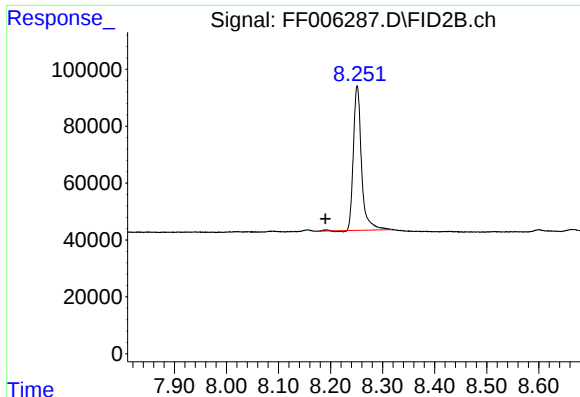

#4 N-TETRADECANE


R.T.: 8.251 min
Delta R.T.: 0.061 min
Response: 553258
Conc: 4.38 ug/ml

Instrument :
FID_F
ClientSampleId :

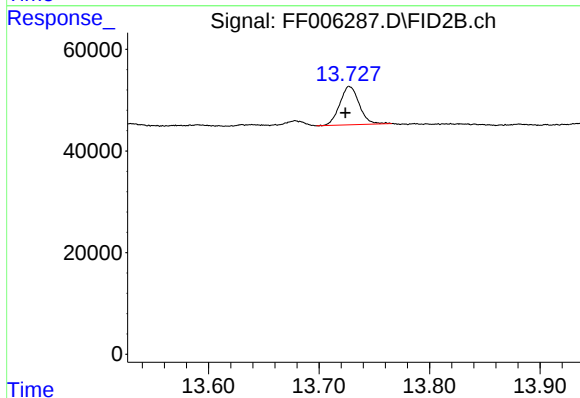


#8 N-DOCOSANE

R.T.: 13.728 min
Delta R.T.: 0.004 min
Response: 91838
Conc: 0.73 ug/ml

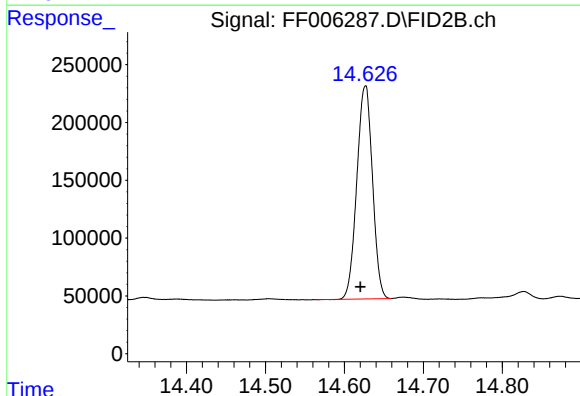


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: 0.007 min
Response: 2536886
Conc: 23.41 ug/ml

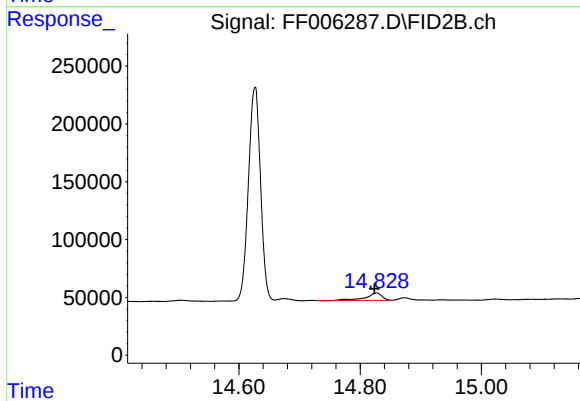

#10 N-TETRACOSANE


R.T.: 14.827 min
Delta R.T.: 0.004 min
Response: 118912
Conc: 0.95 ug/ml

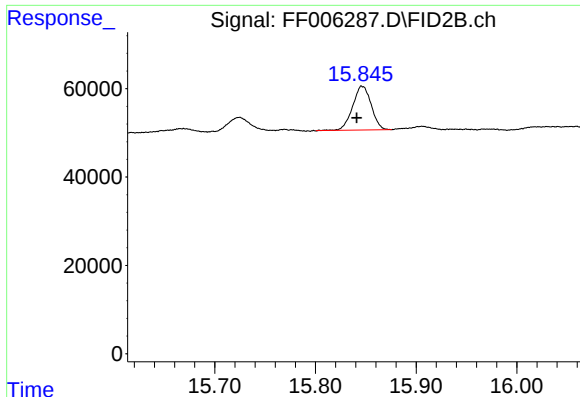

#11 N-HEXACOSANE


R.T.: 15.846 min
Delta R.T.: 0.005 min
Response: 126849
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

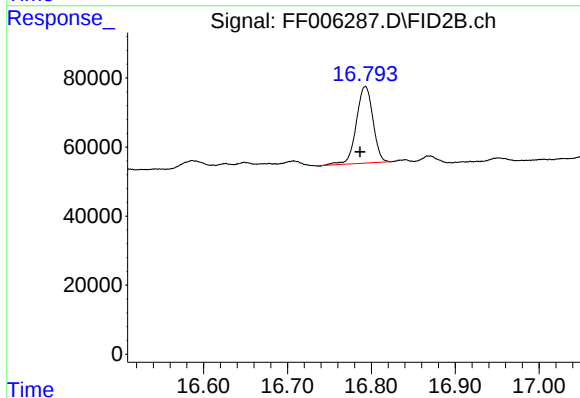


#12 N-OCTACOSANE

R.T.: 16.793 min
Delta R.T.: 0.006 min
Response: 304666
Conc: 2.51 ug/ml

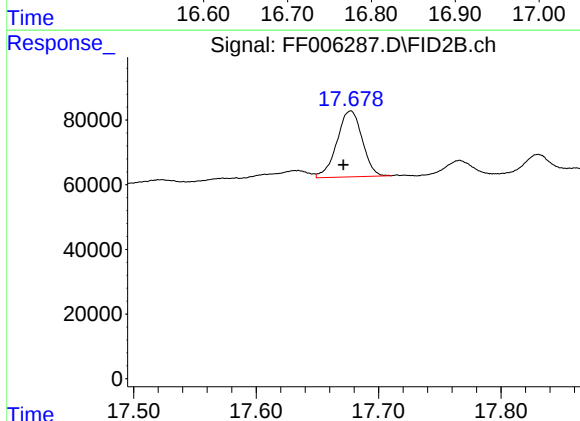


#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: 0.006 min
Response: 292655
Conc: 2.44 ug/ml

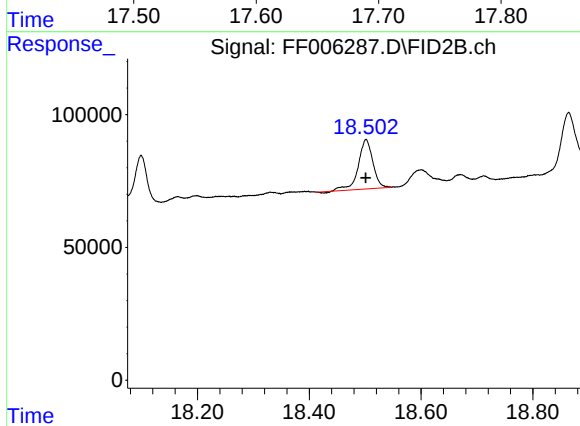

#14 N-DOTRIACONTANE

R.T.: 18.502 min
Delta R.T.: 0.000 min
Response: 336544
Conc: 2.91 ug/ml

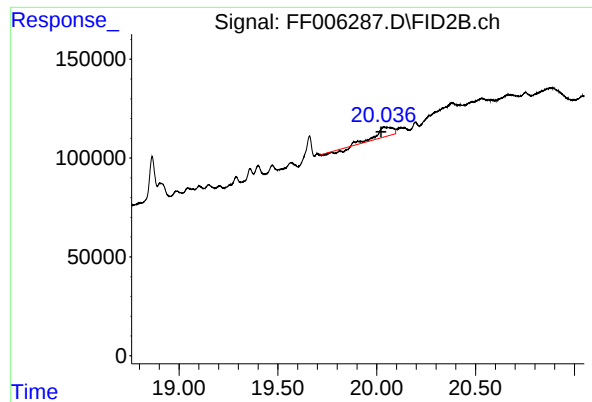

#16 N-HEXATRIACONTANE

R.T.: 20.037 min
Delta R.T.: 0.015 min
Response: 224988
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :