

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006290.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 20:24
 Operator : DD\AJ
 Sample : L1247-38
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:52:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	2236106	20.636 ug/ml
Target Compounds			
4) N-TETRADECANE	8.250f	597029	4.730 ug/ml
8) N-DOCOSANE	13.727	110234	0.874 ug/ml
10) N-TETRACOSANE	14.826	172057	1.381 ug/ml
11) N-HEXACOSANE	15.843	261094	2.124 ug/ml
12) N-OCTACOSANE	16.791	458332	3.770 ug/ml
13) N-TRIACONTANE	17.676	455554	3.799 ug/ml
14) N-DOTRIACONTANE	18.504	377294	3.265 ug/ml
15) N-TETRATRIACONTANE	19.289	78004	0.692 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006290.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 20:24
Operator : DD\AJ
Sample : L1247-38
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:52:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

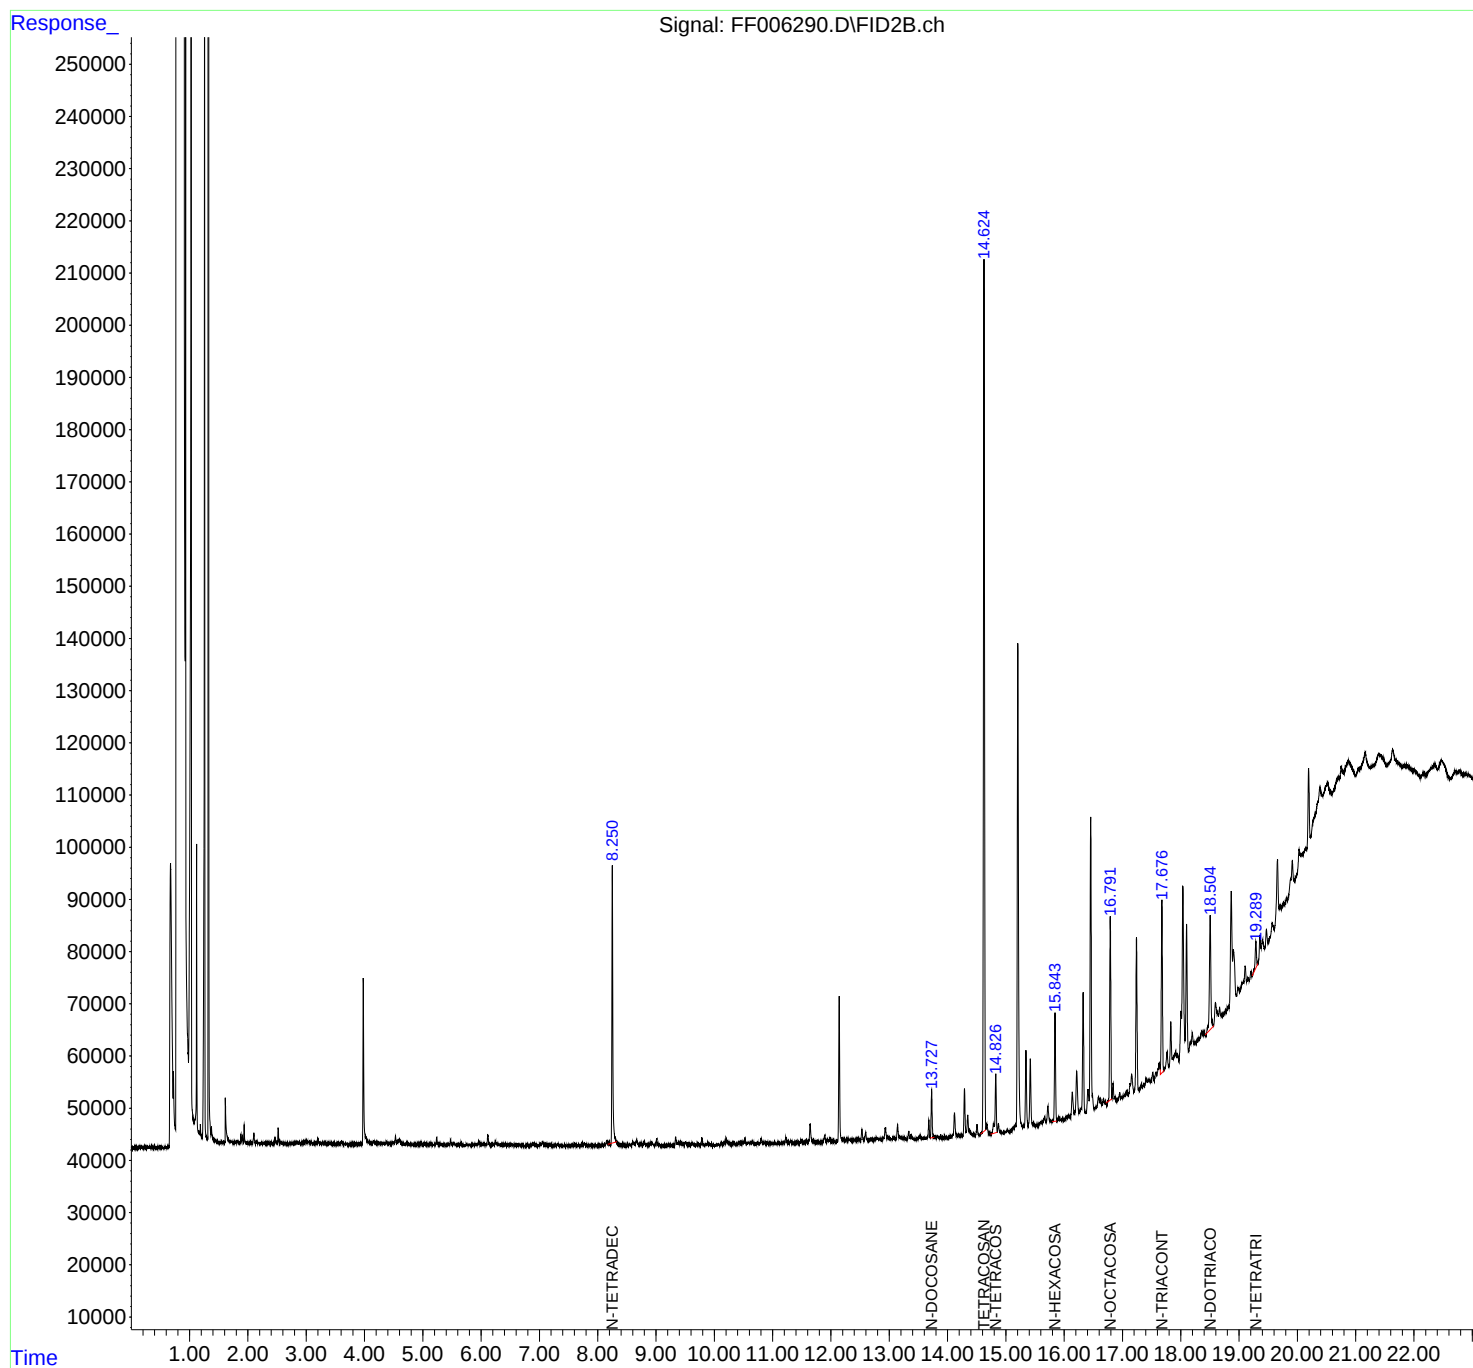


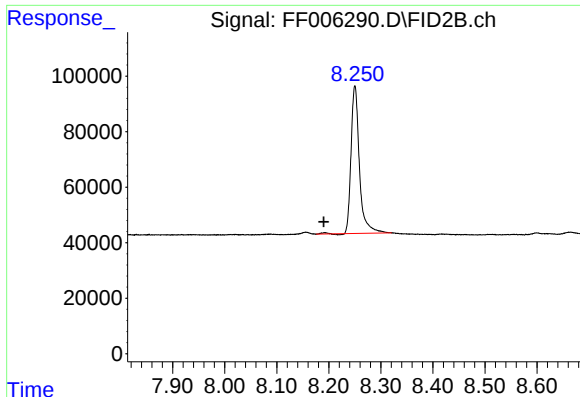

#4 N-TETRADECANE


R.T.: 8.250 min
Delta R.T.: 0.060 min
Response: 597029
Conc: 4.73 ug/ml

Instrument :
FID_F
ClientSampleId :

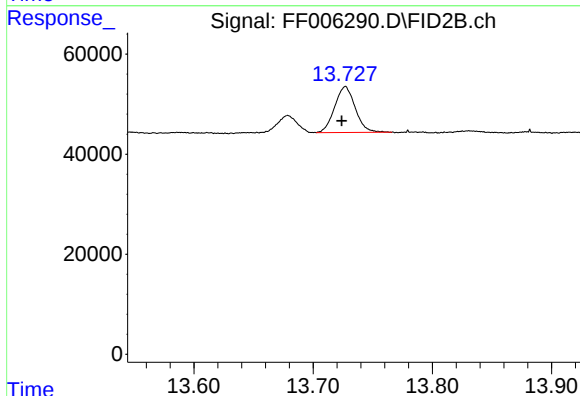


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.003 min
Response: 110234
Conc: 0.87 ug/ml

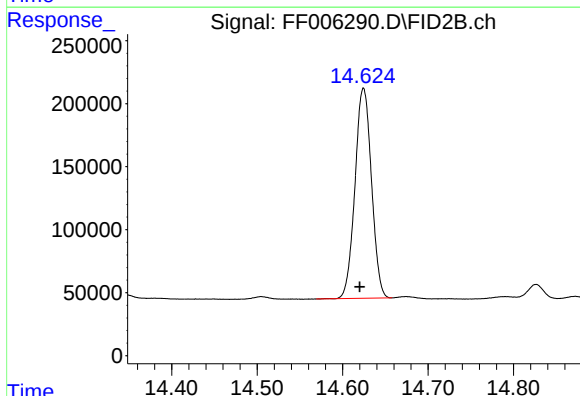


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.624 min
Delta R.T.: 0.004 min
Response: 2236106
Conc: 20.64 ug/ml

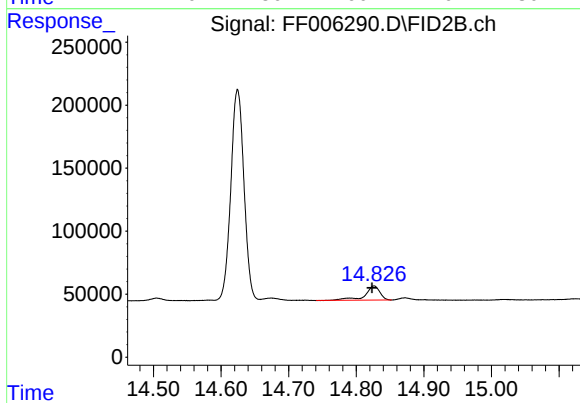

#10 N-TETRACOSANE


R.T.: 14.826 min
Delta R.T.: 0.003 min
Response: 172057
Conc: 1.38 ug/ml

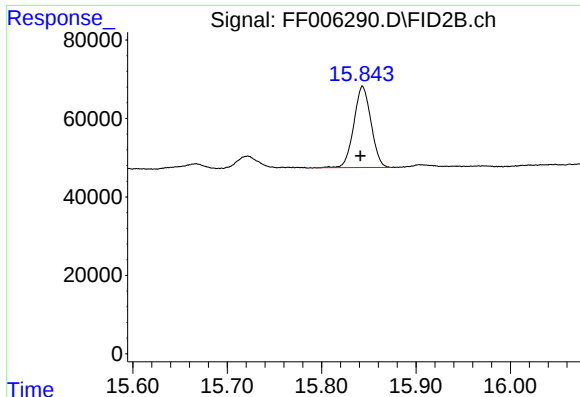

#11 N-HEXACOSANE


R.T.: 15.843 min
Delta R.T.: 0.002 min
Response: 261094
Conc: 2.12 ug/ml

Instrument :
FID_F
ClientSampleId :

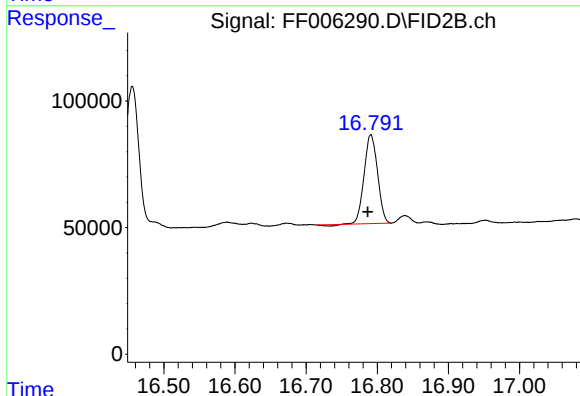


#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: 0.005 min
Response: 458332
Conc: 3.77 ug/ml

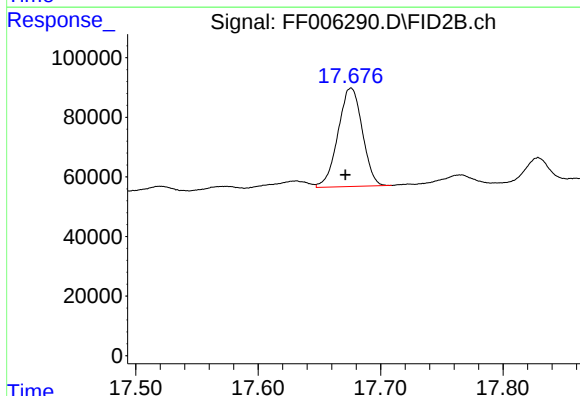


#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: 0.004 min
Response: 455554
Conc: 3.80 ug/ml

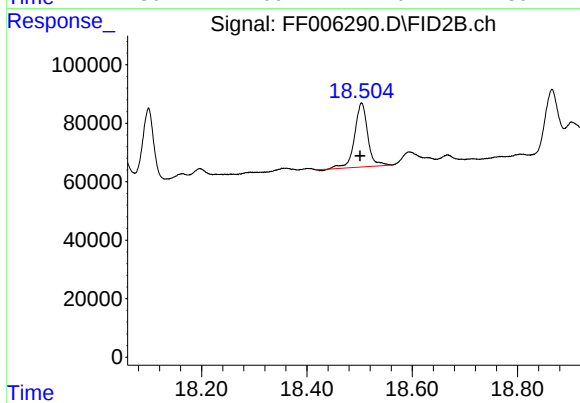

#14 N-DOTRIACONTANE

R.T.: 18.504 min
Delta R.T.: 0.003 min
Response: 377294
Conc: 3.26 ug/ml

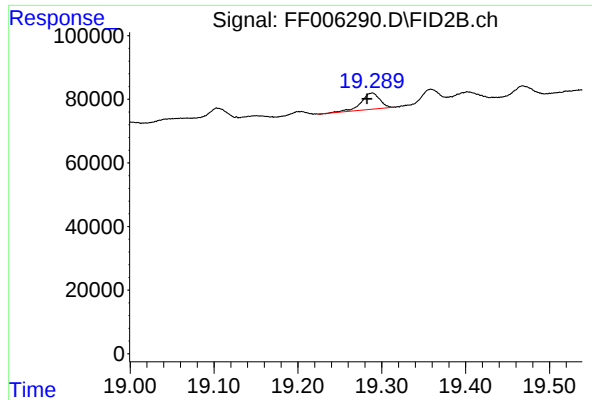

#15 N-TETRATRIACONTANE

R.T.: 19.289 min
Delta R.T.: 0.006 min
Response: 78004
Conc: 0.69 ug/ml

Instrument :
FID_F
ClientSampleId :