

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006291.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 20:55
 Operator : DD\AJ
 Sample : L1247-39
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 22:52:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	2463022	22.730 ug/ml
Target Compounds			
4) N-TETRADECANE	8.250f	456517	3.617 ug/ml
8) N-DOCOSANE	13.727	104406	0.828 ug/ml
11) N-HEXACOSANE	15.844	121421	0.988 ug/ml
12) N-OCTACOSANE	16.791	330361	2.718 ug/ml
13) N-TRIACONTANE	17.677	320918	2.677 ug/ml
14) N-DOTRIACONTANE	18.502	340265	2.944 ug/ml
15) N-TETRATRIACONTANE	19.288	55804	0.495 ug/ml
16) N-HEXATRIACONTANE	20.056	106652	0.997 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006291.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 20:55
Operator : DD\AJ
Sample : L1247-39
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 22:52:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

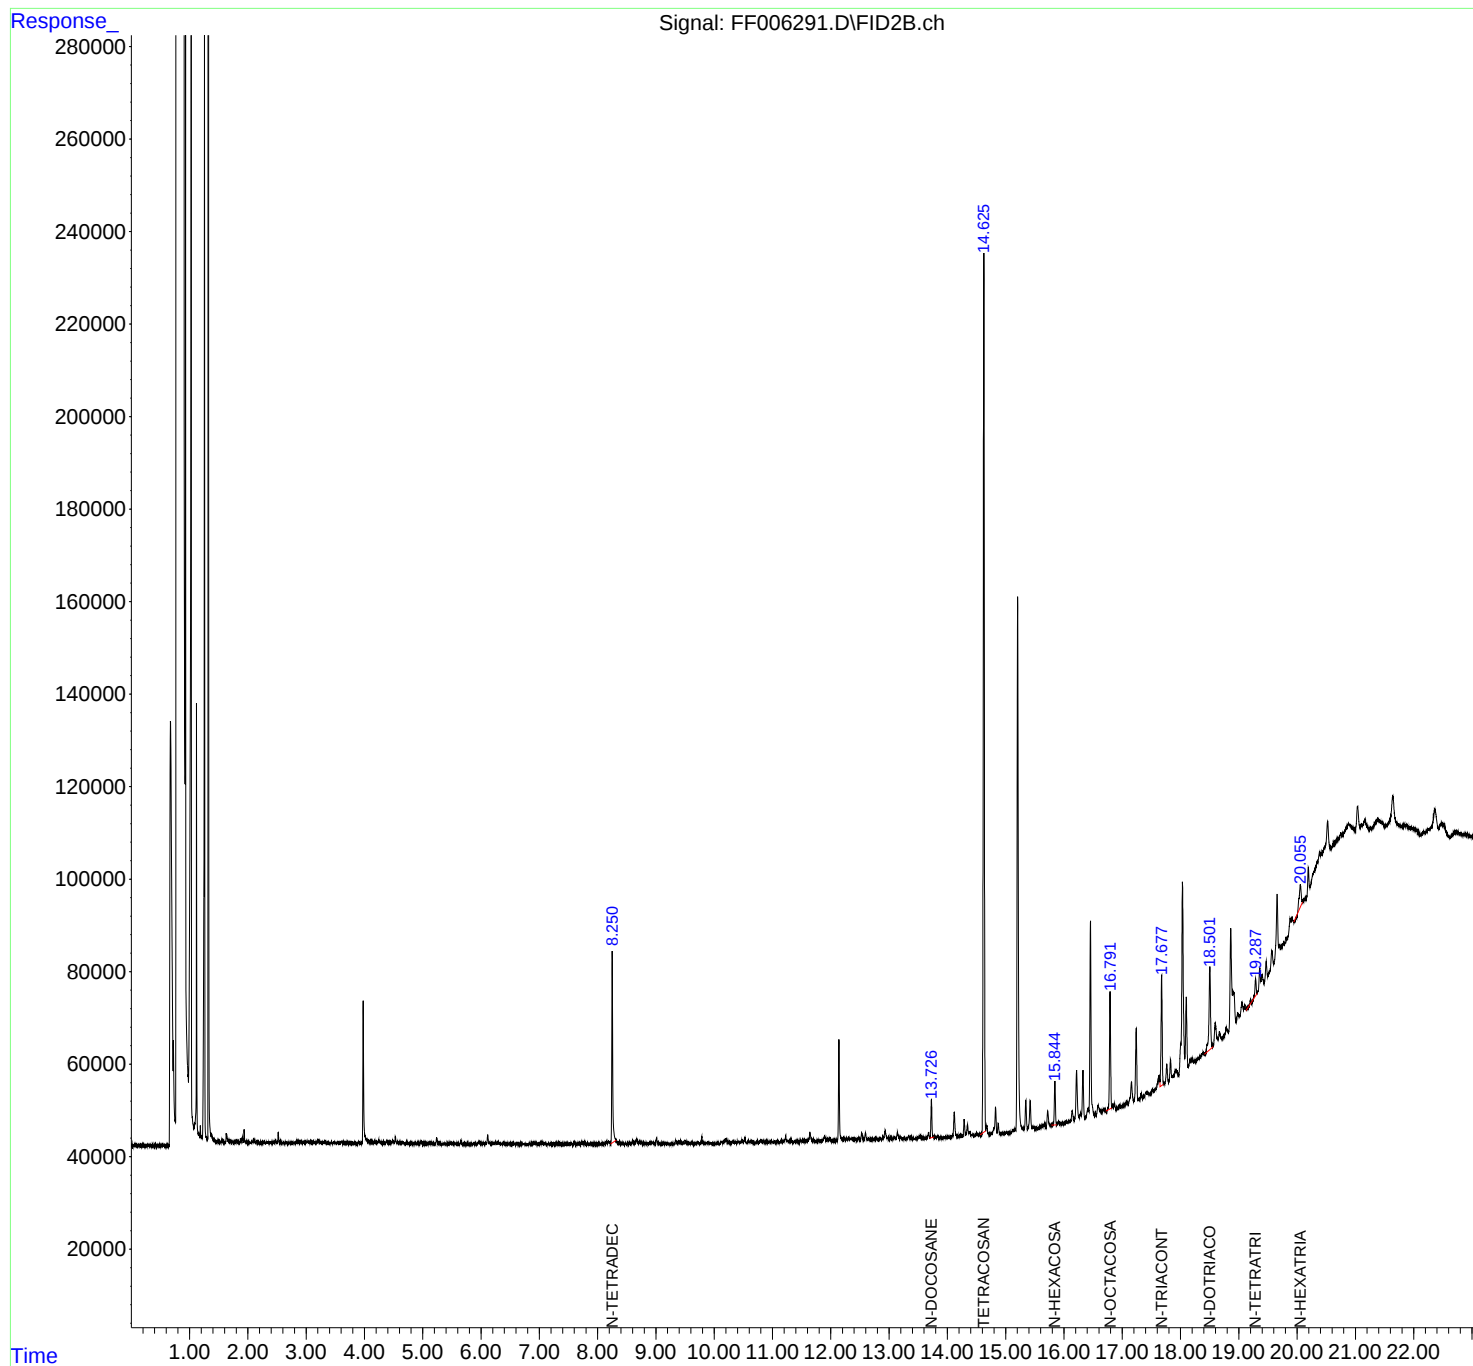


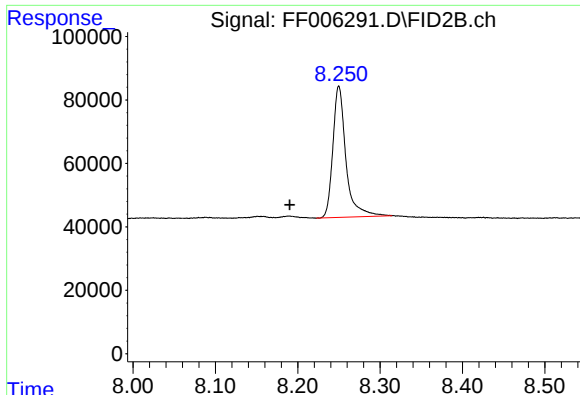

#4 N-TETRADECANE


R.T.: 8.250 min
Delta R.T.: 0.060 min
Response: 456517
Conc: 3.62 ug/ml

Instrument :
FID_F
ClientSampleId :

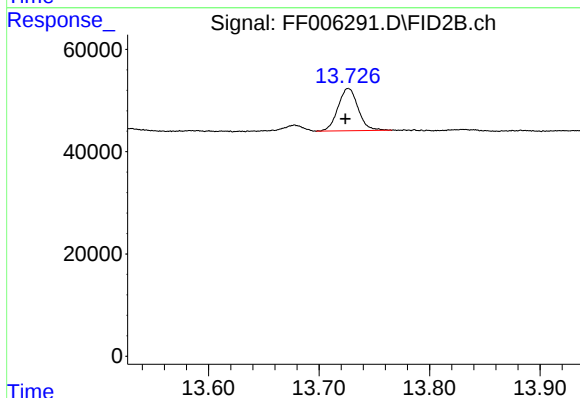


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.003 min
Response: 104406
Conc: 0.83 ug/ml

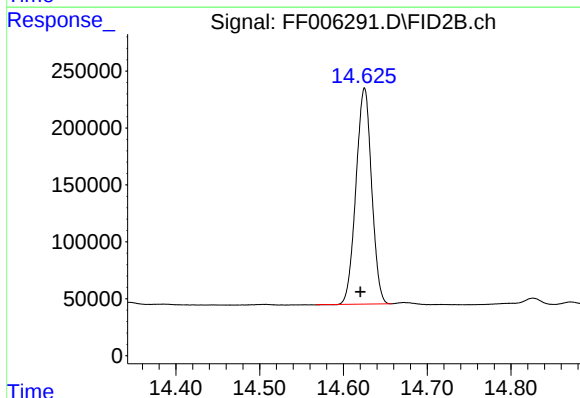


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: 0.005 min
Response: 2463022
Conc: 22.73 ug/ml

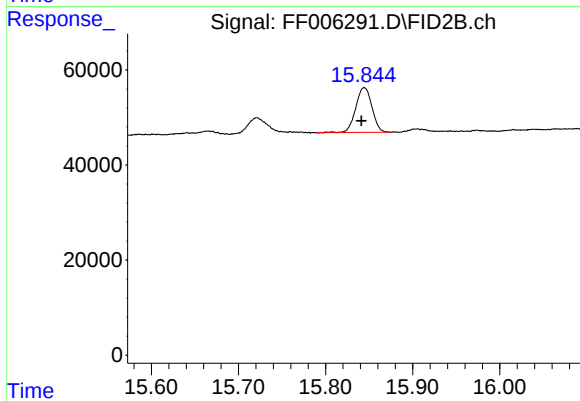

#11 N-HEXACOSANE


R.T.: 15.844 min
Delta R.T.: 0.003 min
Response: 121421
Conc: 0.99 ug/ml

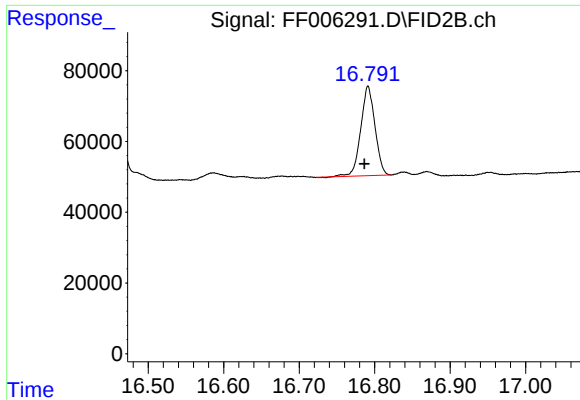

#12 N-OCTACOSANE


R.T.: 16.791 min
Delta R.T.: 0.005 min
Response: 330361
Conc: 2.72 ug/ml

Instrument :
FID_F
ClientSampleId :

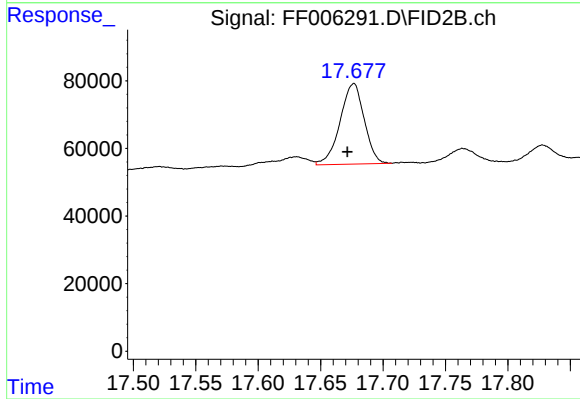


#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: 0.005 min
Response: 320918
Conc: 2.68 ug/ml

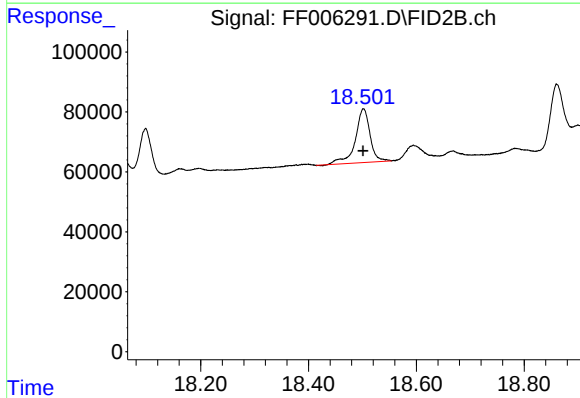


#14 N-DOTRIACONTANE

R.T.: 18.502 min
Delta R.T.: 0.001 min
Response: 340265
Conc: 2.94 ug/ml

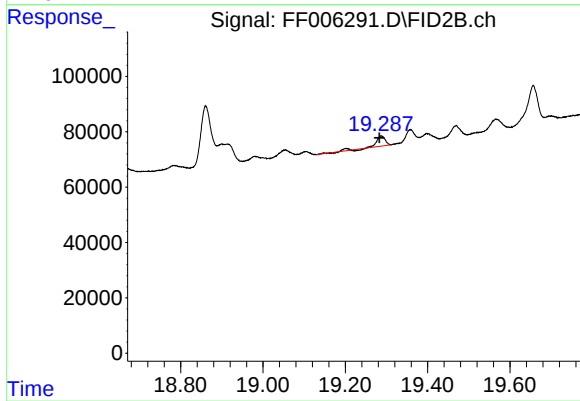

#15 N-TETRATRIACONTANE

R.T.: 19.288 min
Delta R.T.: 0.005 min
Response: 55804
Conc: 0.50 ug/ml

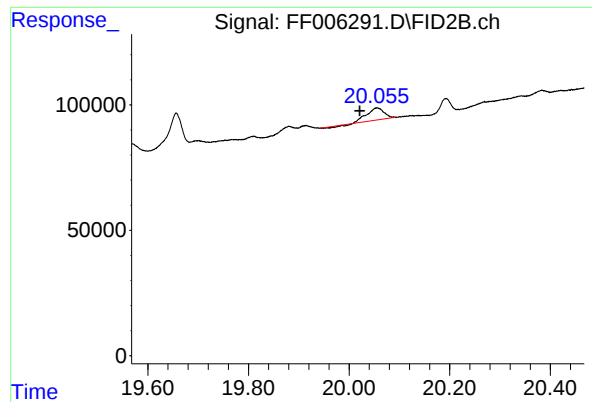

#16 N-HEXATRIACONTANE

R.T.: 20.056 min
Delta R.T.: 0.034 min
Response: 106652
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :