

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006294.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2020 22:25
 Operator : DD\AJ
 Sample : L1007-01 20X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 23:21:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.399	128360	1.016 ug/ml
4)	N-TETRADECANE	8.190	257144	2.037 ug/ml
5)	N-HEXADECANE	9.787	335260	2.623 ug/ml
6)	N-OCTADECANE	11.224	268541	2.117 ug/ml
7)	N-EICOSANE	12.530	200271	1.567 ug/ml
8)	N-DOCOSANE	13.727	187307	1.485 ug/ml
10)	N-TETRACOSANE	14.811	620232	4.979 ug/ml
12)	N-OCTACOSANE	16.795	152729	1.256 ug/ml
13)	N-TRIACONTANE	17.674	156538	1.306 ug/ml
14)	N-DOTRIACONTANE	18.504	175911	1.522 ug/ml
15)	N-TETRATRIACONTANE	19.285	35321	0.314 ug/ml
16)	N-HEXATRIACONTANE	20.028	100340	0.938 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006294.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2020 22:25
Operator : DD\AJ
Sample : L1007-01 20X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 23:21:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

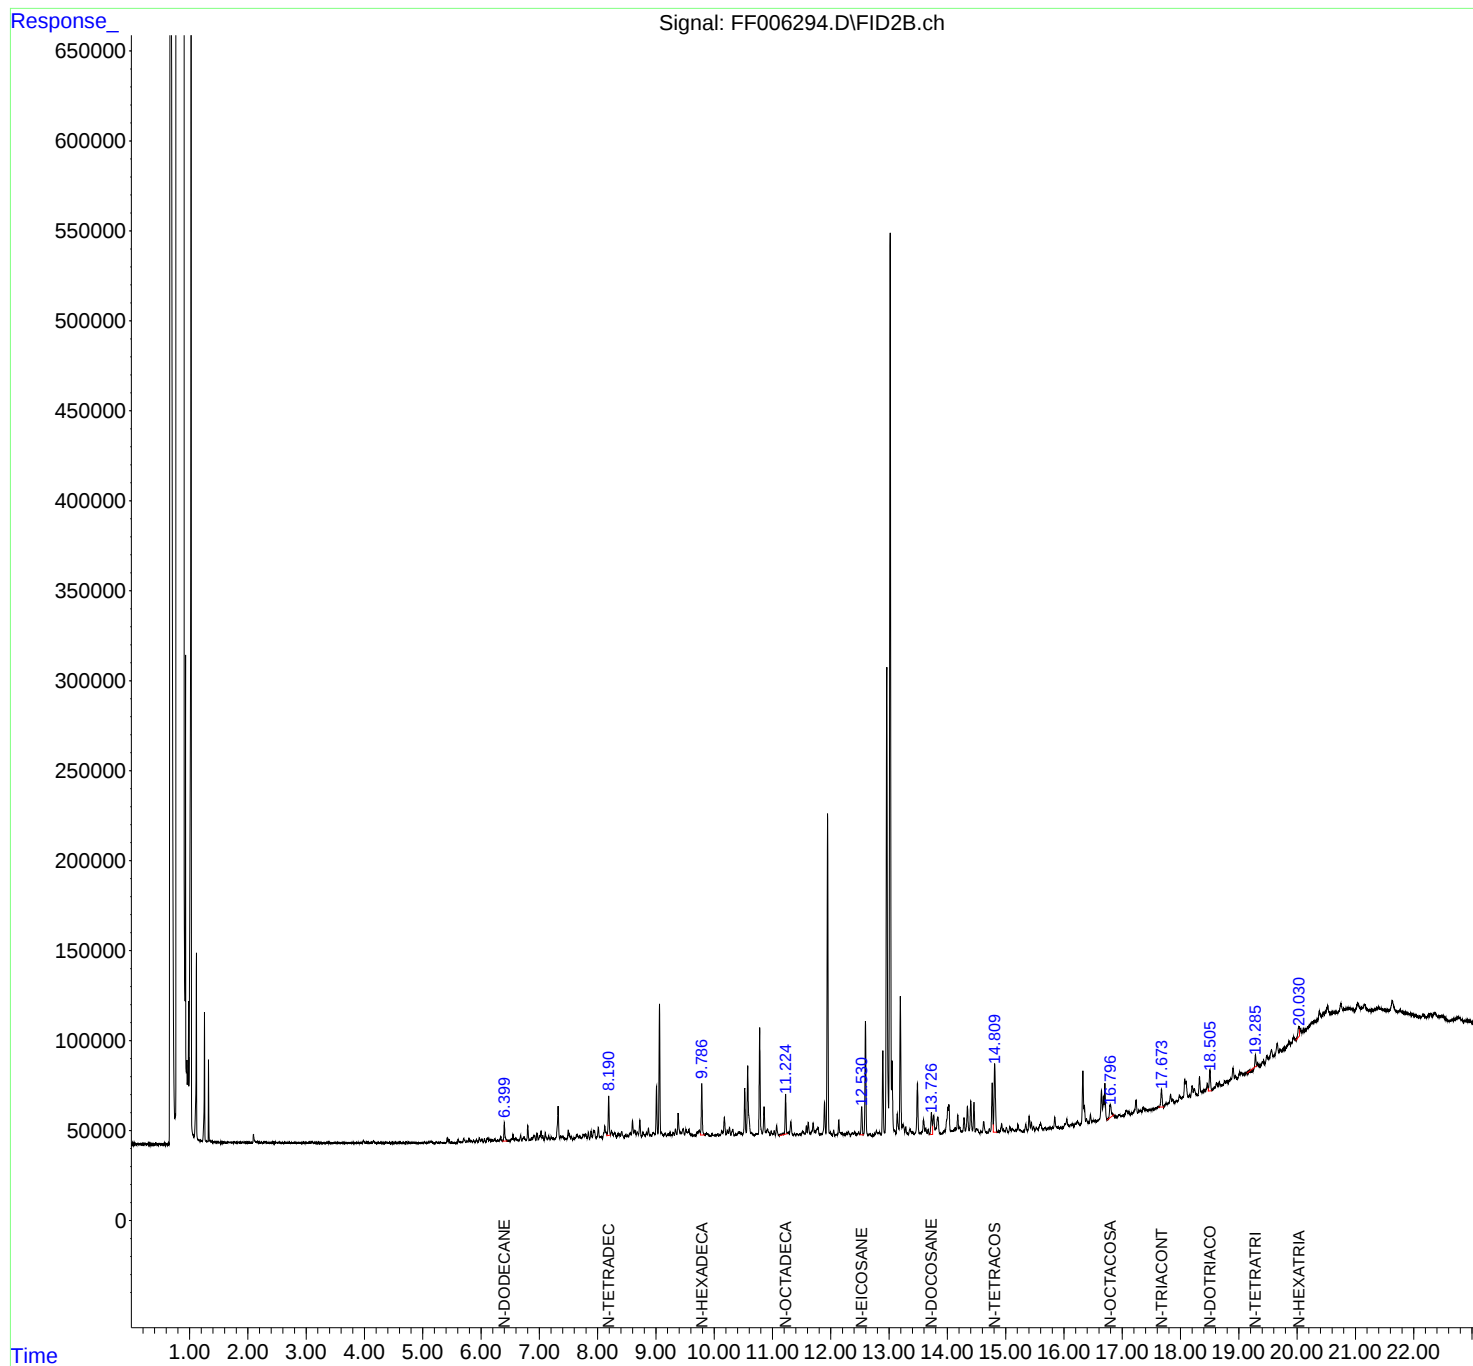


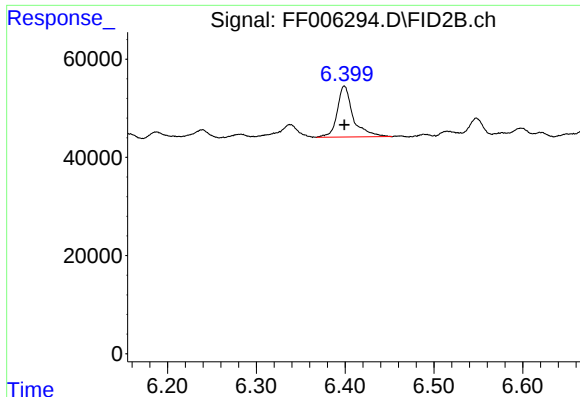

#3 N-DODECANE


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 128360
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :

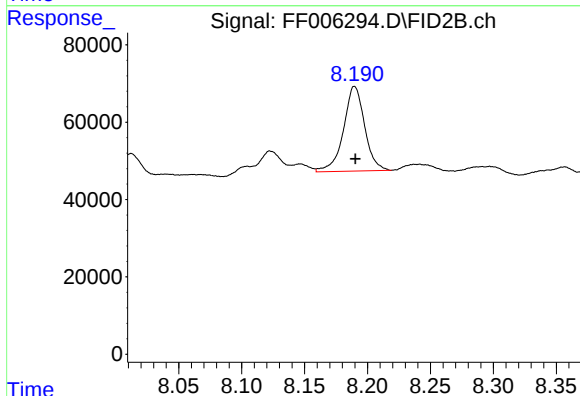


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 257144
Conc: 2.04 ug/ml

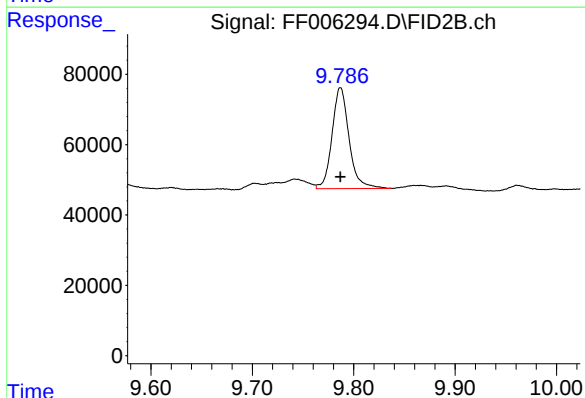


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: 0.000 min
Response: 335260
Conc: 2.62 ug/ml

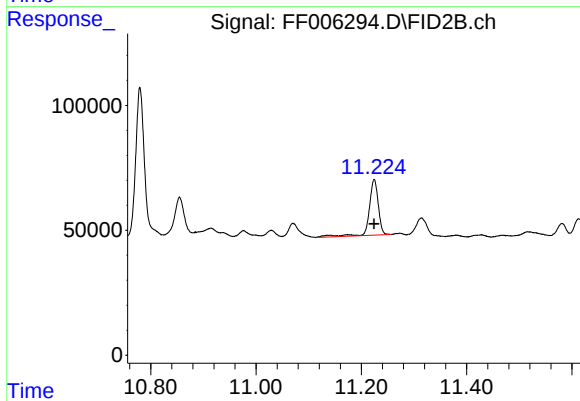

#6 N-OCTADECANE


R.T.: 11.224 min
Delta R.T.: 0.000 min
Response: 268541
Conc: 2.12 ug/ml

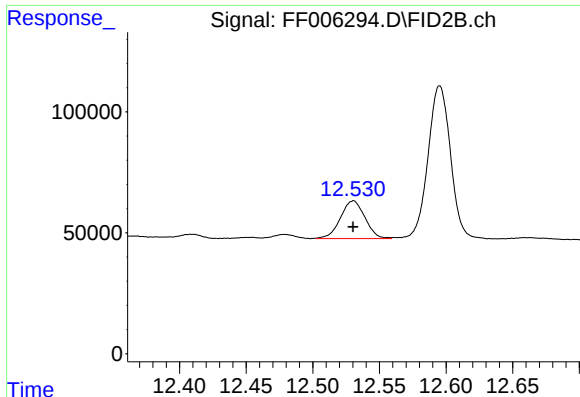

#7 N-EICOSANE


R.T.: 12.530 min
Delta R.T.: 0.000 min
Response: 200271
Conc: 1.57 ug/ml

Instrument :
FID_F
ClientSampleId :

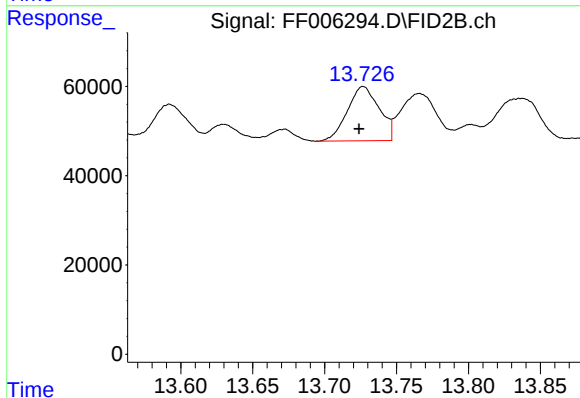


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.003 min
Response: 187307
Conc: 1.49 ug/ml

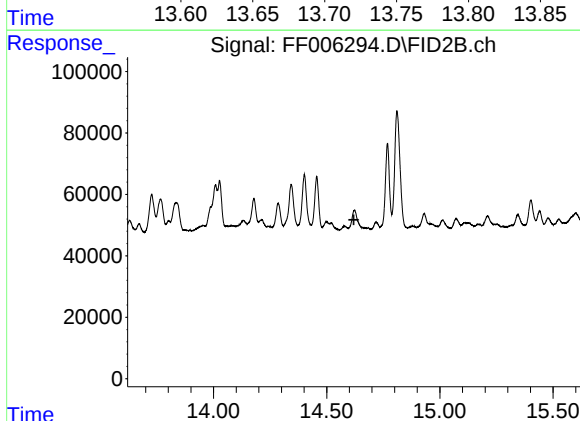


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.620 min
Response: 0
Conc: N.D.

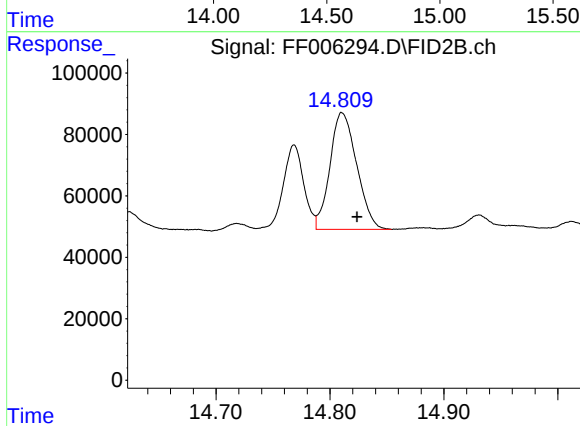

#10 N-TETRACOSANE


R.T.: 14.811 min
Delta R.T.: -0.013 min
Response: 620232
Conc: 4.98 ug/ml

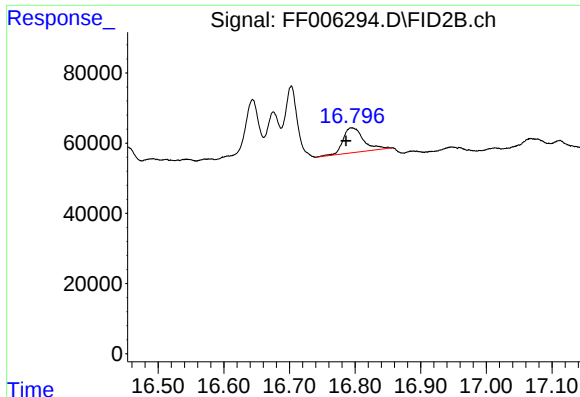

#12 N-OCTACOSANE


R.T.: 16.795 min
Delta R.T.: 0.008 min
Response: 152729
Conc: 1.26 ug/ml

Instrument :
FID_F
ClientSampleId :

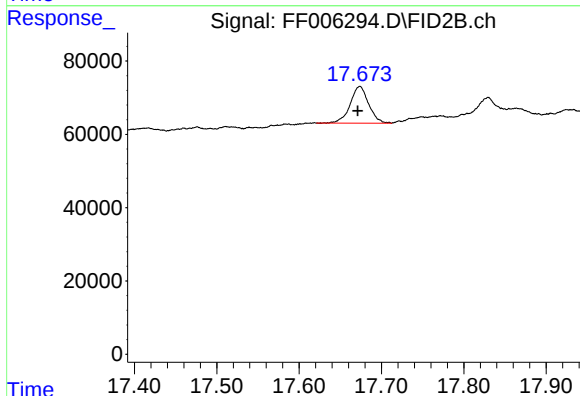


#13 N-TRIACONTANE

R.T.: 17.674 min
Delta R.T.: 0.002 min
Response: 156538
Conc: 1.31 ug/ml

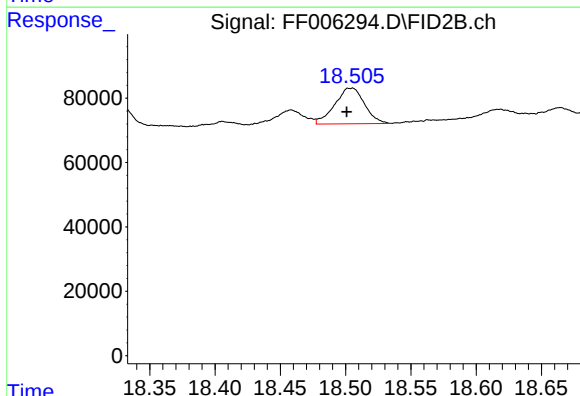


#14 N-DOTRIACONTANE

R.T.: 18.504 min
Delta R.T.: 0.003 min
Response: 175911
Conc: 1.52 ug/ml

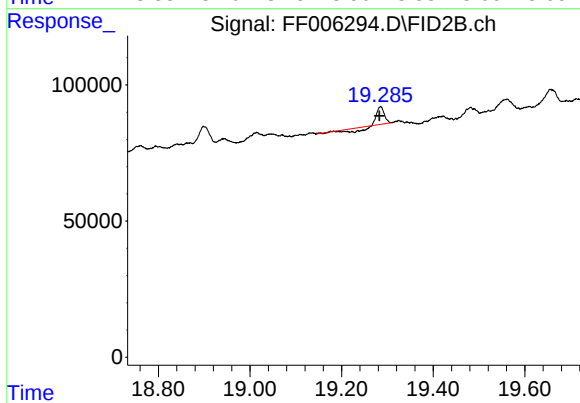

#15 N-TETRATRIACONTANE

R.T.: 19.285 min
Delta R.T.: 0.003 min
Response: 35321
Conc: 0.31 ug/ml

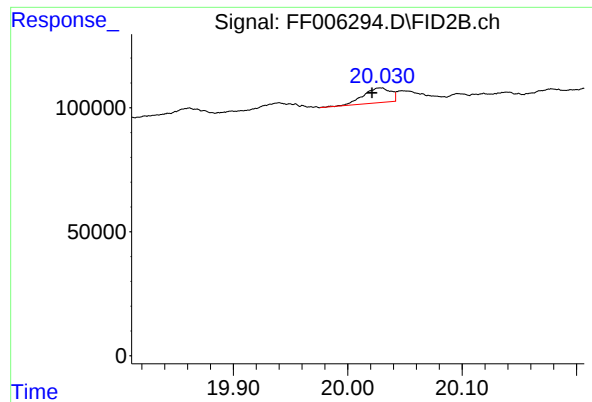

#16 N-HEXATRIACONTANE

R.T.: 20.028 min
Delta R.T.: 0.007 min
Response: 100340
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :