

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
 Data File : FF006299.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jan 2020 00:55
 Operator : DD\AJ
 Sample : L1161-09
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Integration File: autoint1.e
 Quant Time: Jan 25 04:12:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	1745667	16.110 ug/ml
Target Compounds			
2) N-DECANE	4.383	166054	1.332 ug/ml
3) N-DODECANE	6.399	151172	1.197 ug/ml
4) N-TETRADECANE	8.190	122484	0.970 ug/ml
5) N-HEXADECANE	9.787	155665	1.218 ug/ml
6) N-OCTADECANE	11.224	152934	1.206 ug/ml
7) N-EICOSANE	12.530	154624	1.210 ug/ml
8) N-DOCOSANE	13.724	152646	1.211 ug/ml
10) N-TETRACOSANE	14.824	152672	1.226 ug/ml
11) N-HEXACOSANE	15.842	160964	1.309 ug/ml
12) N-OCTACOSANE	16.788	191332	1.574 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012420\
Data File : FF006299.D
Signal(s) : FID2B.ch
Acq On : 25 Jan 2020 00:55
Operator : DD\AJ
Sample : L1161-09
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MDL-WATER-03-QT1-2020

Integration File: autoint1.e
Quant Time: Jan 25 04:12:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

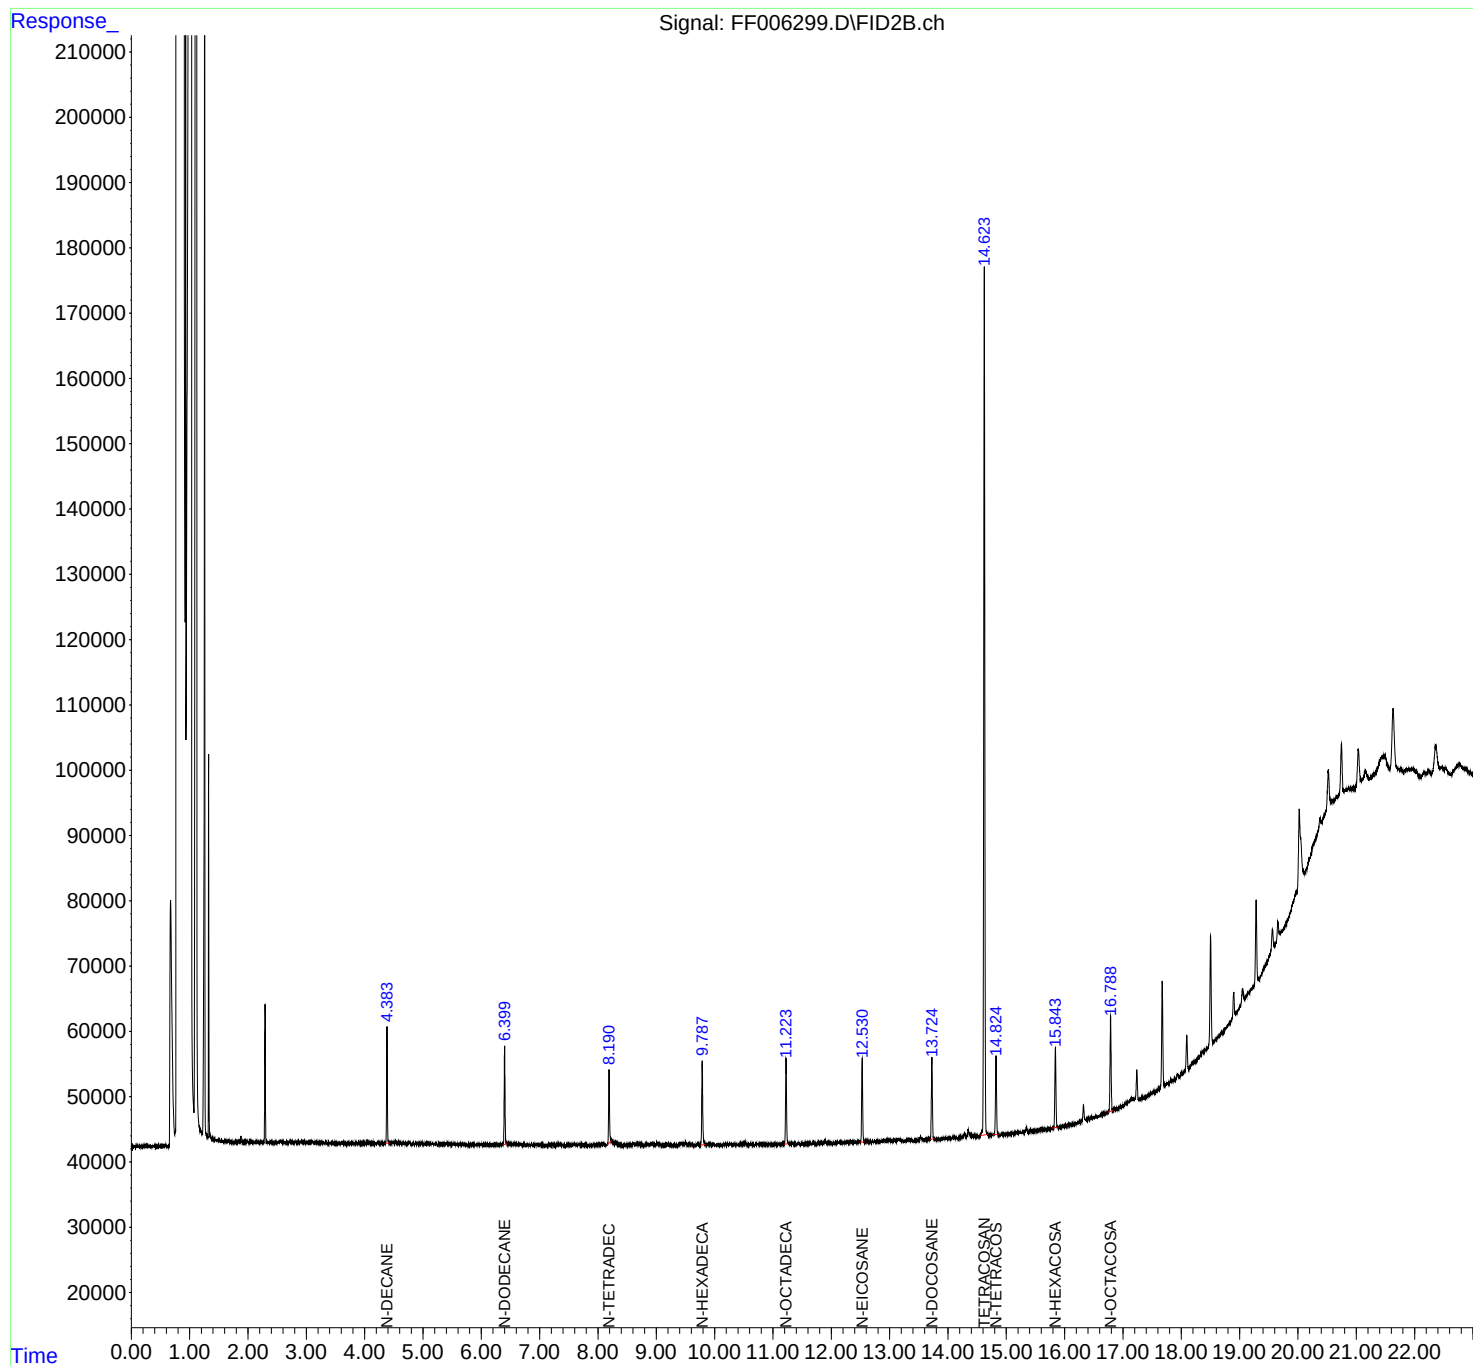


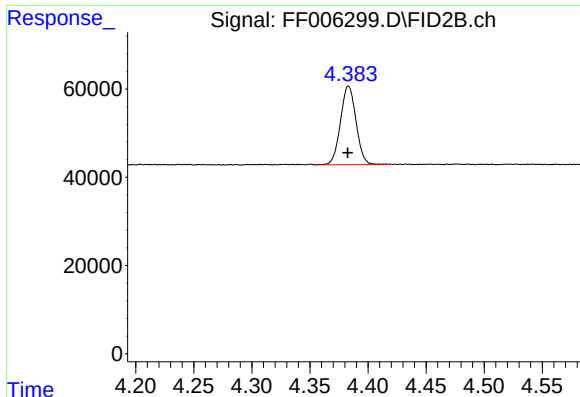

#2 N-DECANE


R.T.: 4.383 min
Delta R.T.: 0.000 min
Response: 166054
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :
MDL-WATER-03-QT1-2020

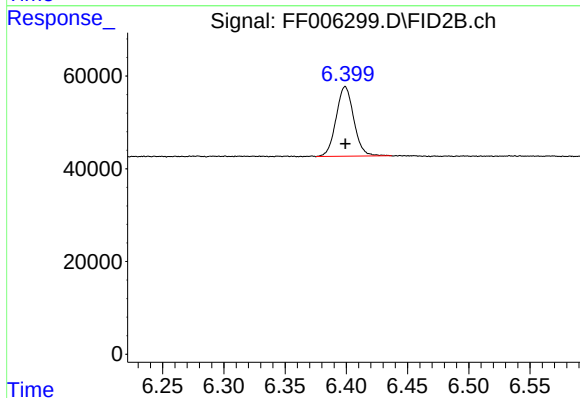


#3 N-DODECANE

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 151172
Conc: 1.20 ug/ml

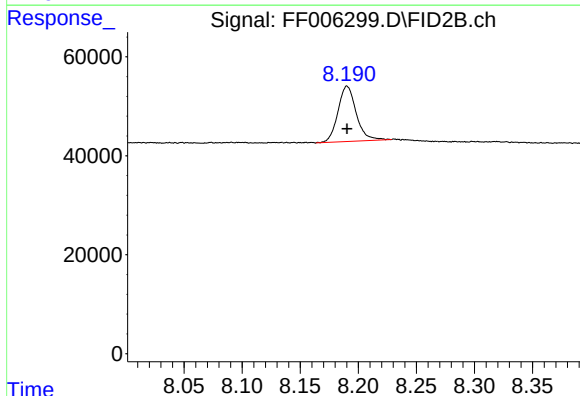


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 122484
Conc: 0.97 ug/ml

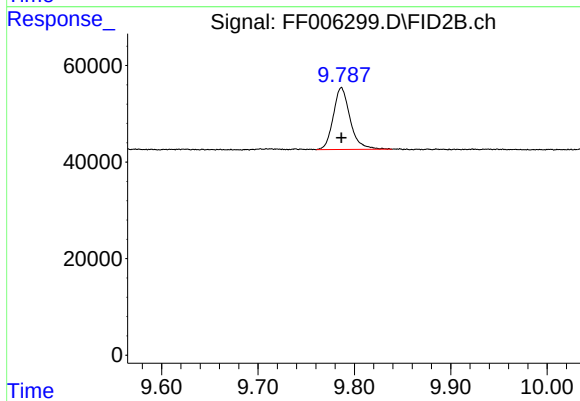

#5 N-HEXADECANE


R.T.: 9.787 min
Delta R.T.: 0.000 min
Response: 155665
Conc: 1.22 ug/ml

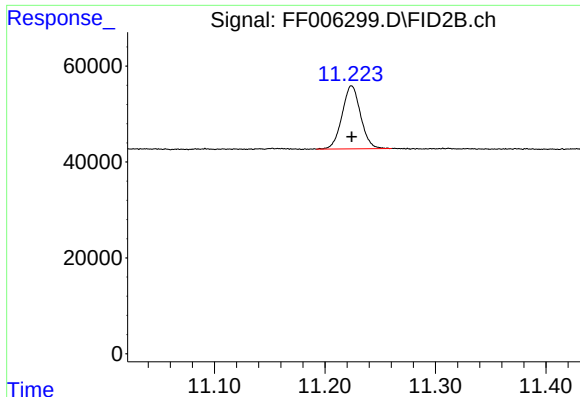

#6 N-OCTADECANE


R.T.: 11.224 min
Delta R.T.: 0.000 min
Response: 152934
Conc: 1.21 ug/ml

Instrument :
FID_F
ClientSampleId :
MDL-WATER-03-QT1-2020

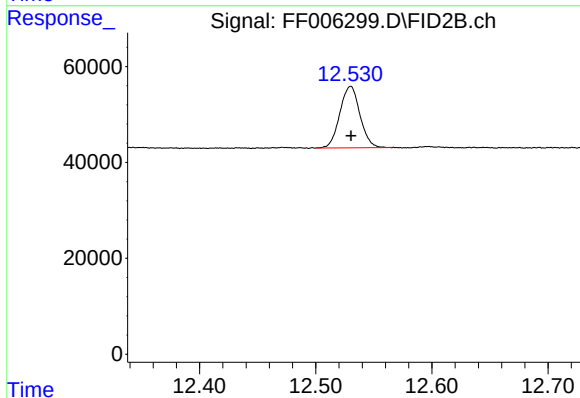


#7 N-EICOSANE

R.T.: 12.530 min
Delta R.T.: 0.000 min
Response: 154624
Conc: 1.21 ug/ml

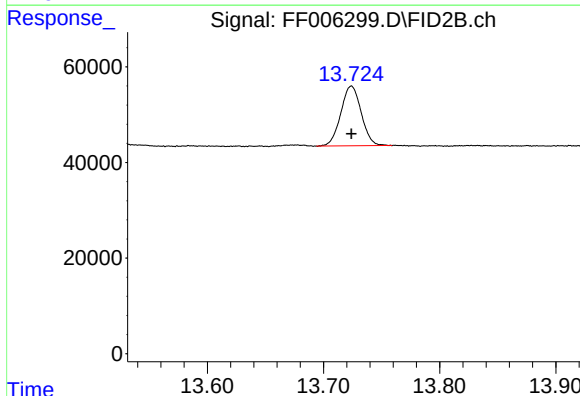


#8 N-DOCOSANE

R.T.: 13.724 min
Delta R.T.: 0.000 min
Response: 152646
Conc: 1.21 ug/ml

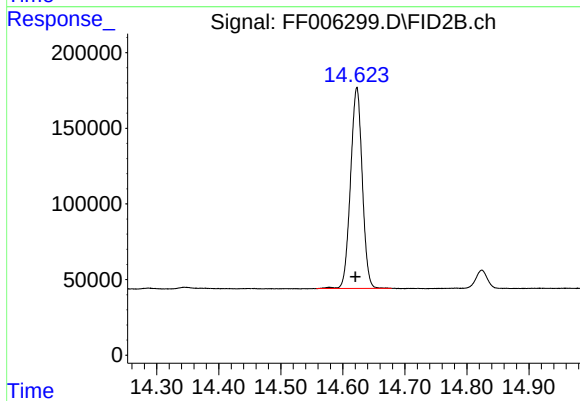

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.623 min
Delta R.T.: 0.003 min
Response: 1745667
Conc: 16.11 ug/ml

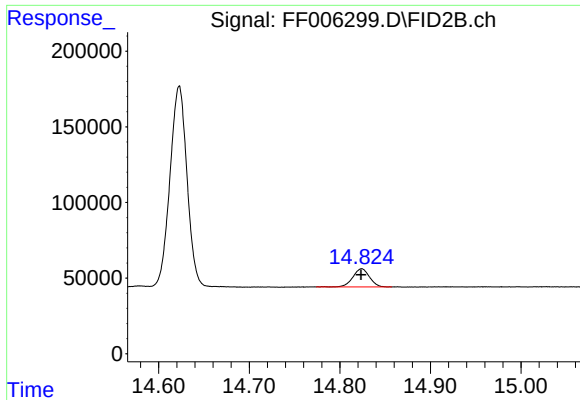

#10 N-TETRACOSANE


R.T.: 14.824 min
Delta R.T.: 0.000 min
Response: 152672
Conc: 1.23 ug/ml

Instrument :
FID_F
ClientSampleId :
MDL-WATER-03-QT1-2020

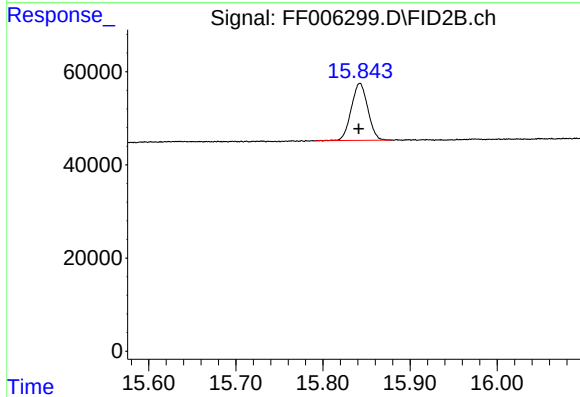

#11 N-HEXACOSANE

R.T.: 15.842 min
Delta R.T.: 0.001 min
Response: 160964
Conc: 1.31 ug/ml

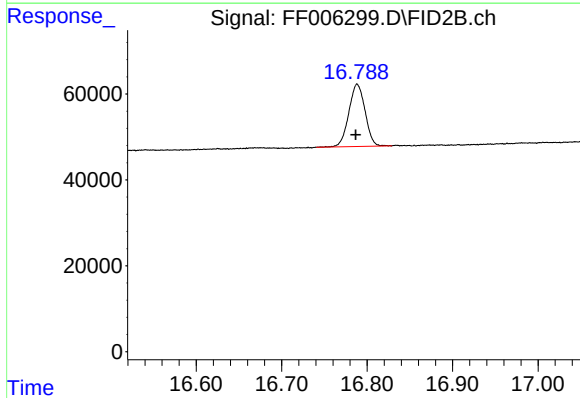

#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: 0.002 min
Response: 191332
Conc: 1.57 ug/ml