

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009771.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 11:07
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 20:39:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.336	182699	1.343 ug/ml
15)	N-TETRATRIACONTANE	19.104	118110	0.994 ug/ml
16)	N-HEXATRIACONTANE	19.883	2585439	25.076 ug/ml
18)	N-TETRACONTANE	21.394	483994	5.328 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009771.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 11:07
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 20:39:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

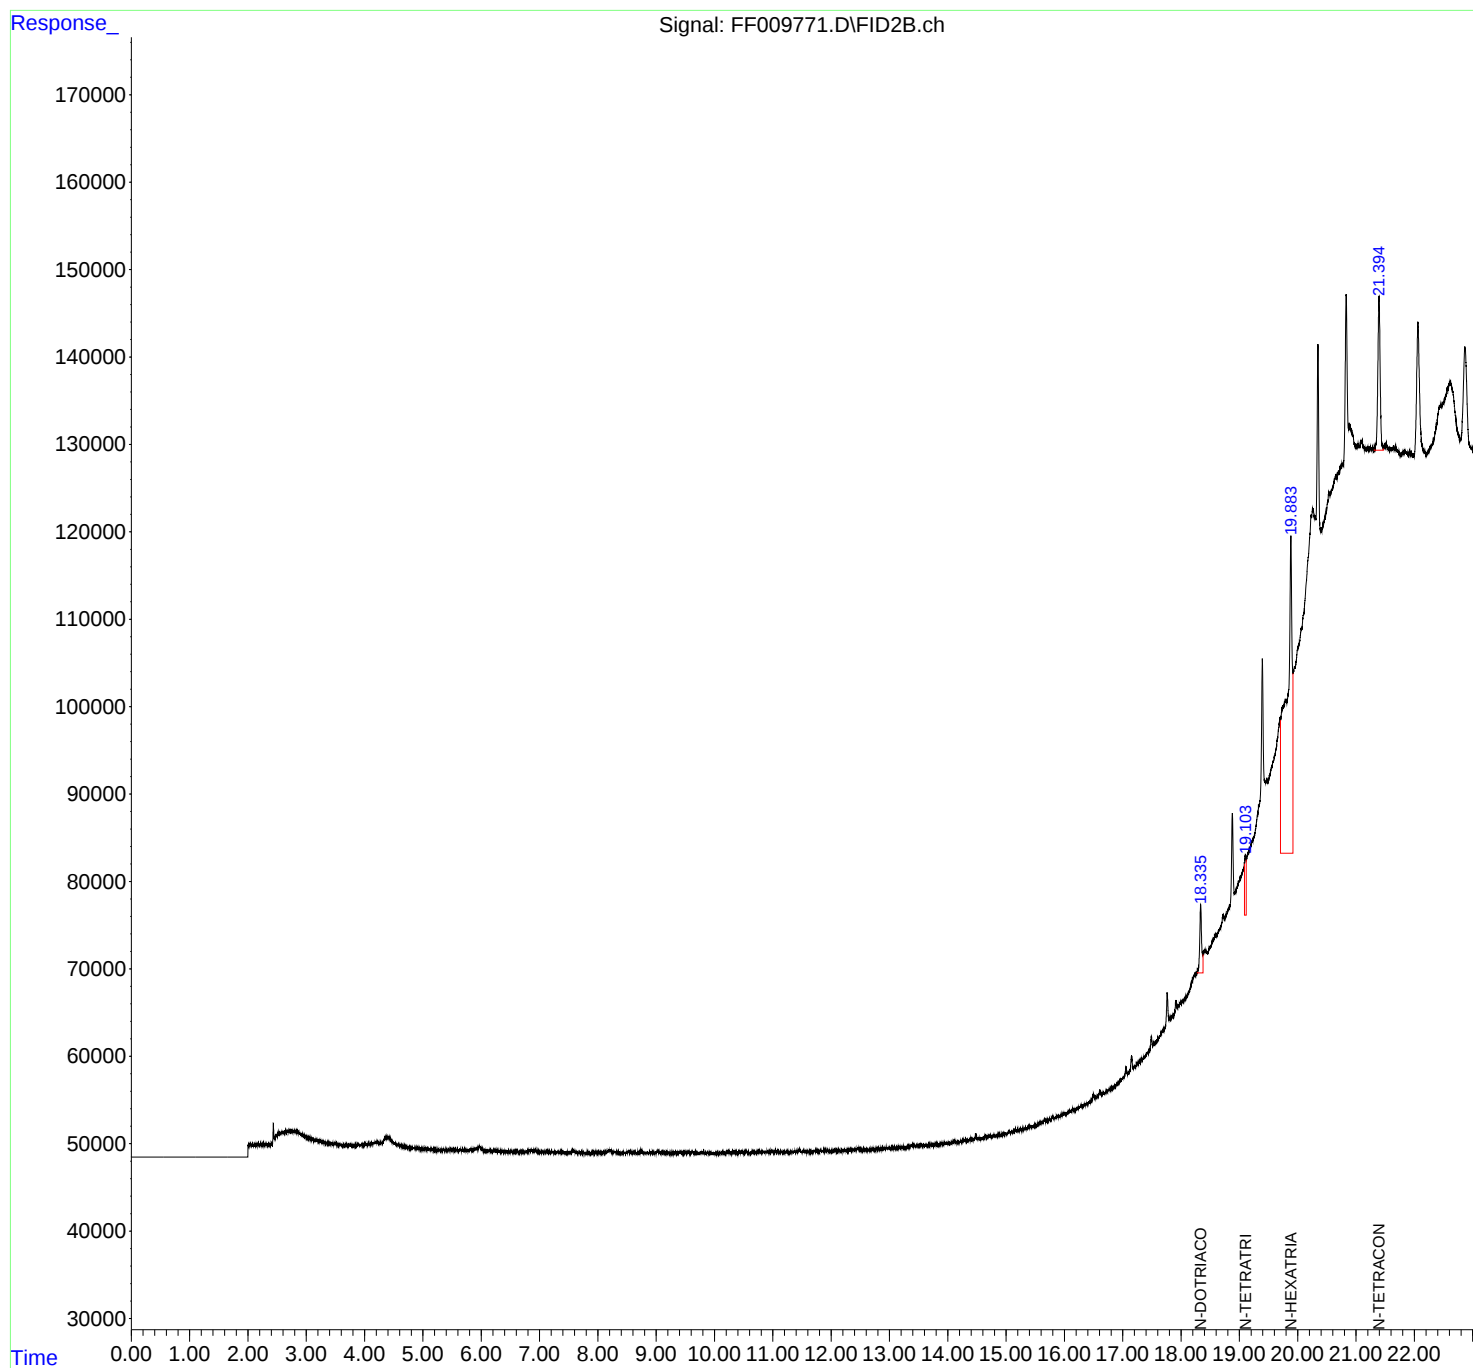


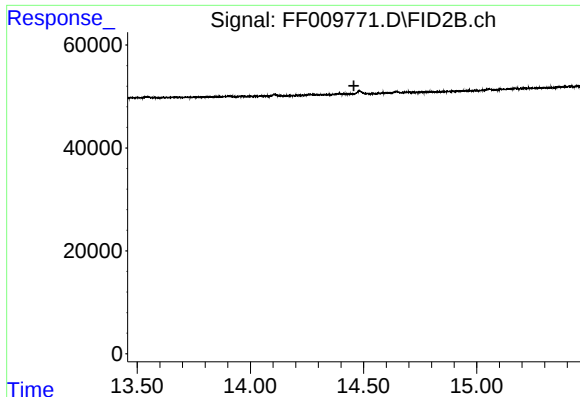

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

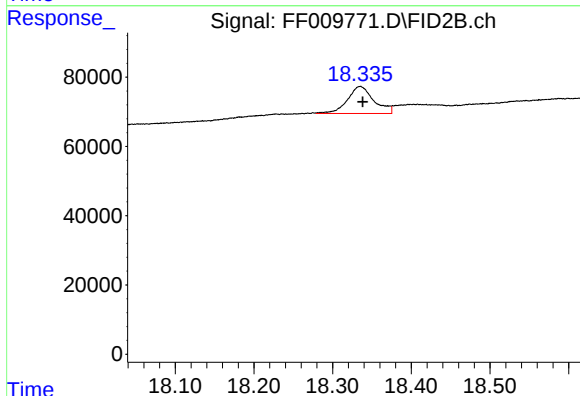


#14 N-DOTRIACONTANE

R.T.: 18.336 min
Delta R.T.: -0.003 min
Response: 182699
Conc: 1.34 ug/ml

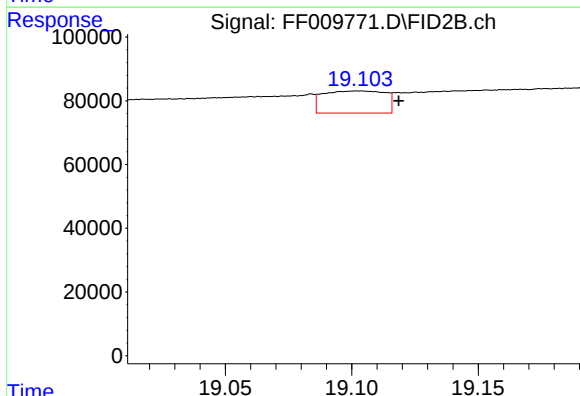


#15 N-TETRATRIACONTANE

R.T.: 19.104 min
Delta R.T.: -0.015 min
Response: 118110
Conc: 0.99 ug/ml

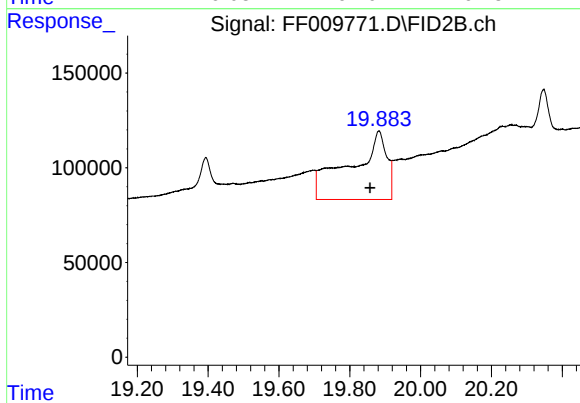

#16 N-HEXATRIACONTANE

R.T.: 19.883 min
Delta R.T.: 0.026 min
Response: 2585439
Conc: 25.08 ug/ml

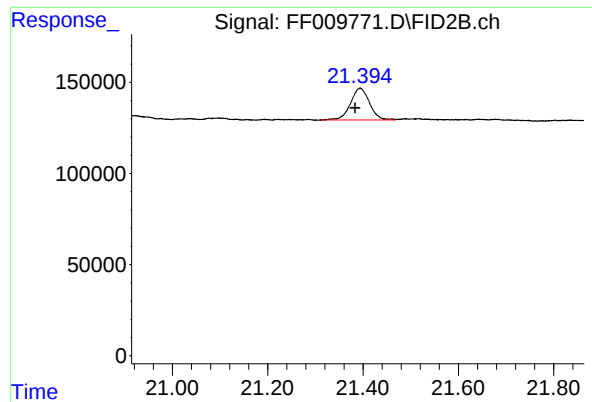

#18 N-TETRACONTANE

R.T.: 21.394 min
Delta R.T.: 0.011 min
Response: 483994
Conc: 5.33 ug/ml

Instrument :

FID_F

ClientSampleId :