

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
 Data File : FF009776.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2022 14:42
 Operator : AJ\MA
 Sample : N1224-02 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 20:40:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.439	988196	7.562 ug/ml
Target Compounds			
4) N-TETRADECANE	8.019	51523	0.351 ug/ml
6) N-OCTADECANE	11.132f	51414	0.333 ug/ml
11) N-HEXACOSANE	15.658	50387	0.345 ug/ml
12) N-OCTACOSANE	16.604	75296	0.519 ug/ml
13) N-TRIACONTANE	17.488	61821	0.432 ug/ml
14) N-DOTRIACONTANE	18.320	129177	0.949 ug/ml
15) N-TETRATRIACONTANE	19.097	140284	1.181 ug/ml
16) N-HEXATRIACONTANE	19.837	484833	4.702 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009776.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 14:42
Operator : AJ\MA
Sample : N1224-02 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 20:40:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

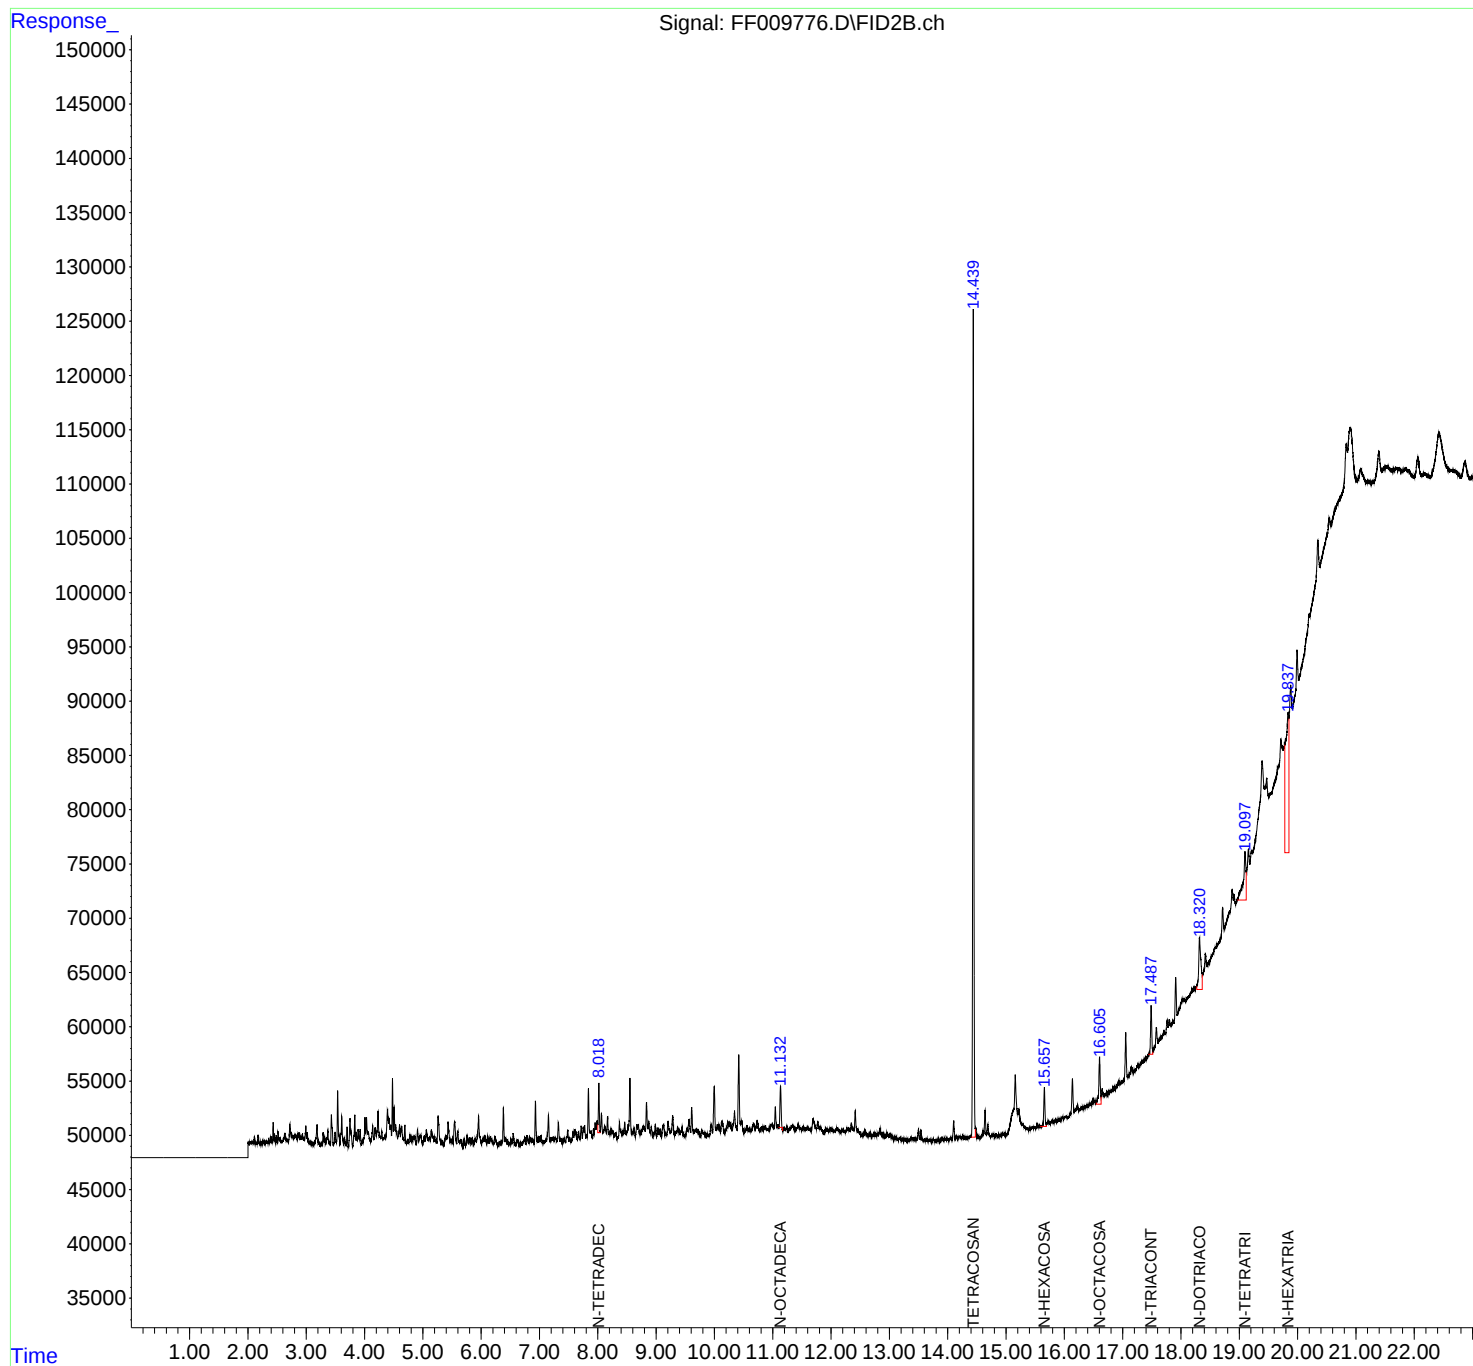


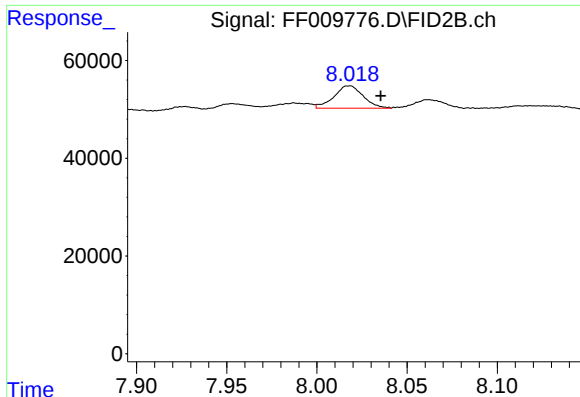

#4 N-TETRADECANE


R.T.: 8.019 min
Delta R.T.: -0.017 min
Response: 51523
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

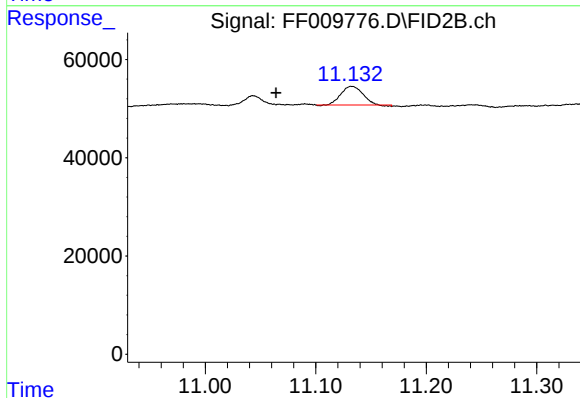


#6 N-OCTADECANE

R.T.: 11.132 min
Delta R.T.: 0.068 min
Response: 51414
Conc: 0.33 ug/ml

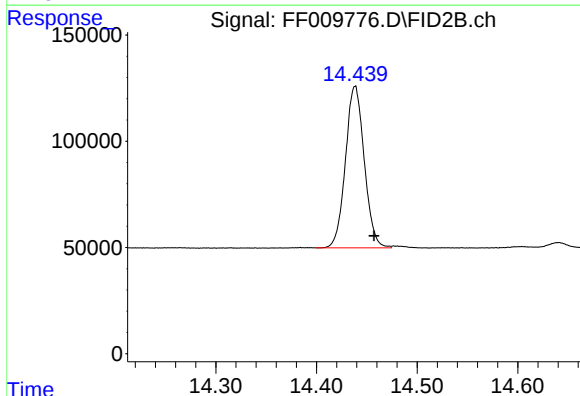


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.439 min
Delta R.T.: -0.018 min
Response: 988196
Conc: 7.56 ug/ml

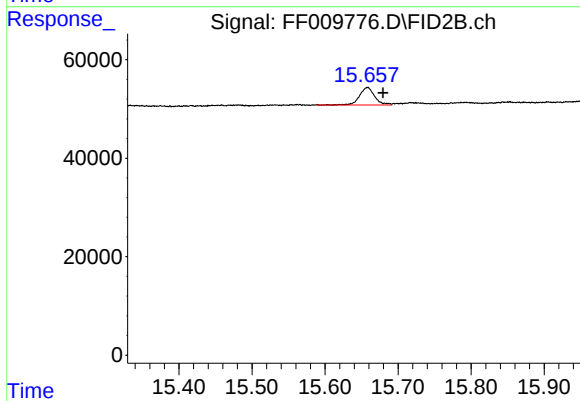

#11 N-HEXACOSANE


R.T.: 15.658 min
Delta R.T.: -0.021 min
Response: 50387
Conc: 0.34 ug/ml

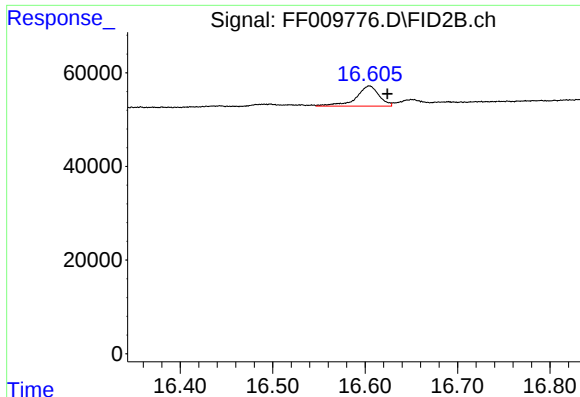

#12 N-OCTACOSANE


R.T.: 16.604 min
Delta R.T.: -0.020 min
Response: 75296
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :

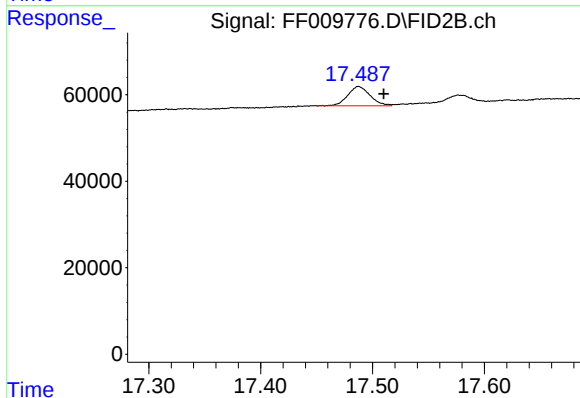


#13 N-TRIACONTANE

R.T.: 17.488 min
Delta R.T.: -0.022 min
Response: 61821
Conc: 0.43 ug/ml

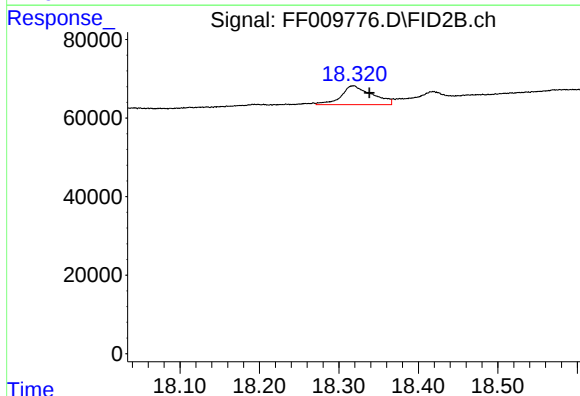


#14 N-DOTRIACONTANE

R.T.: 18.320 min
Delta R.T.: -0.019 min
Response: 129177
Conc: 0.95 ug/ml

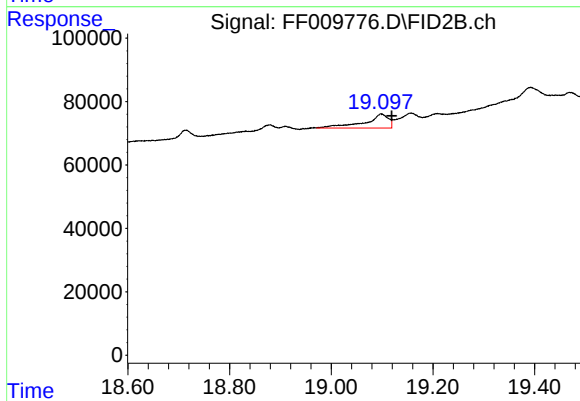

#15 N-TETRATRIACONTANE

R.T.: 19.097 min
Delta R.T.: -0.021 min
Response: 140284
Conc: 1.18 ug/ml

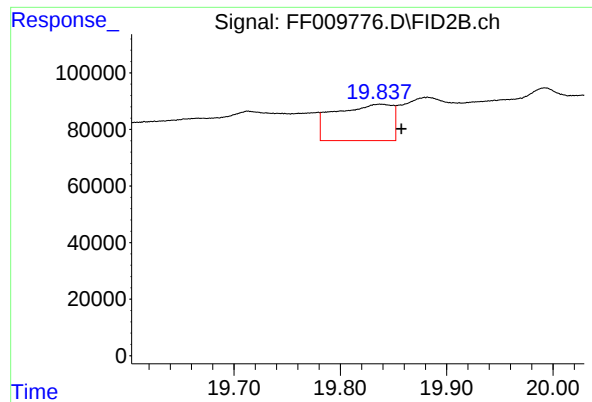

#16 N-HEXATRIACONTANE

R.T.: 19.837 min
Delta R.T.: -0.020 min
Response: 484833
Conc: 4.70 ug/ml

Instrument :

FID_F

ClientSampleId :