

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
 Data File : FF009781.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jan 2022 17:10
 Operator : AJ\MA
 Sample : N1208-04 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 20:42:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
4) N-TETRADECANE	7.974f	208835	1.421 ug/ml
5) N-HEXADECANE	9.630	281983	1.885 ug/ml
6) N-OCTADECANE	11.021	202029	1.310 ug/ml
7) N-EICOSANE	12.359	363285	2.403 ug/ml
16) N-HEXATRIACONTANE	19.843	390283	3.785 ug/ml
18) N-TETRACONTANE	21.390	57352	0.631 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009781.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 17:10
Operator : AJ\MA
Sample : N1208-04 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 20:42:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

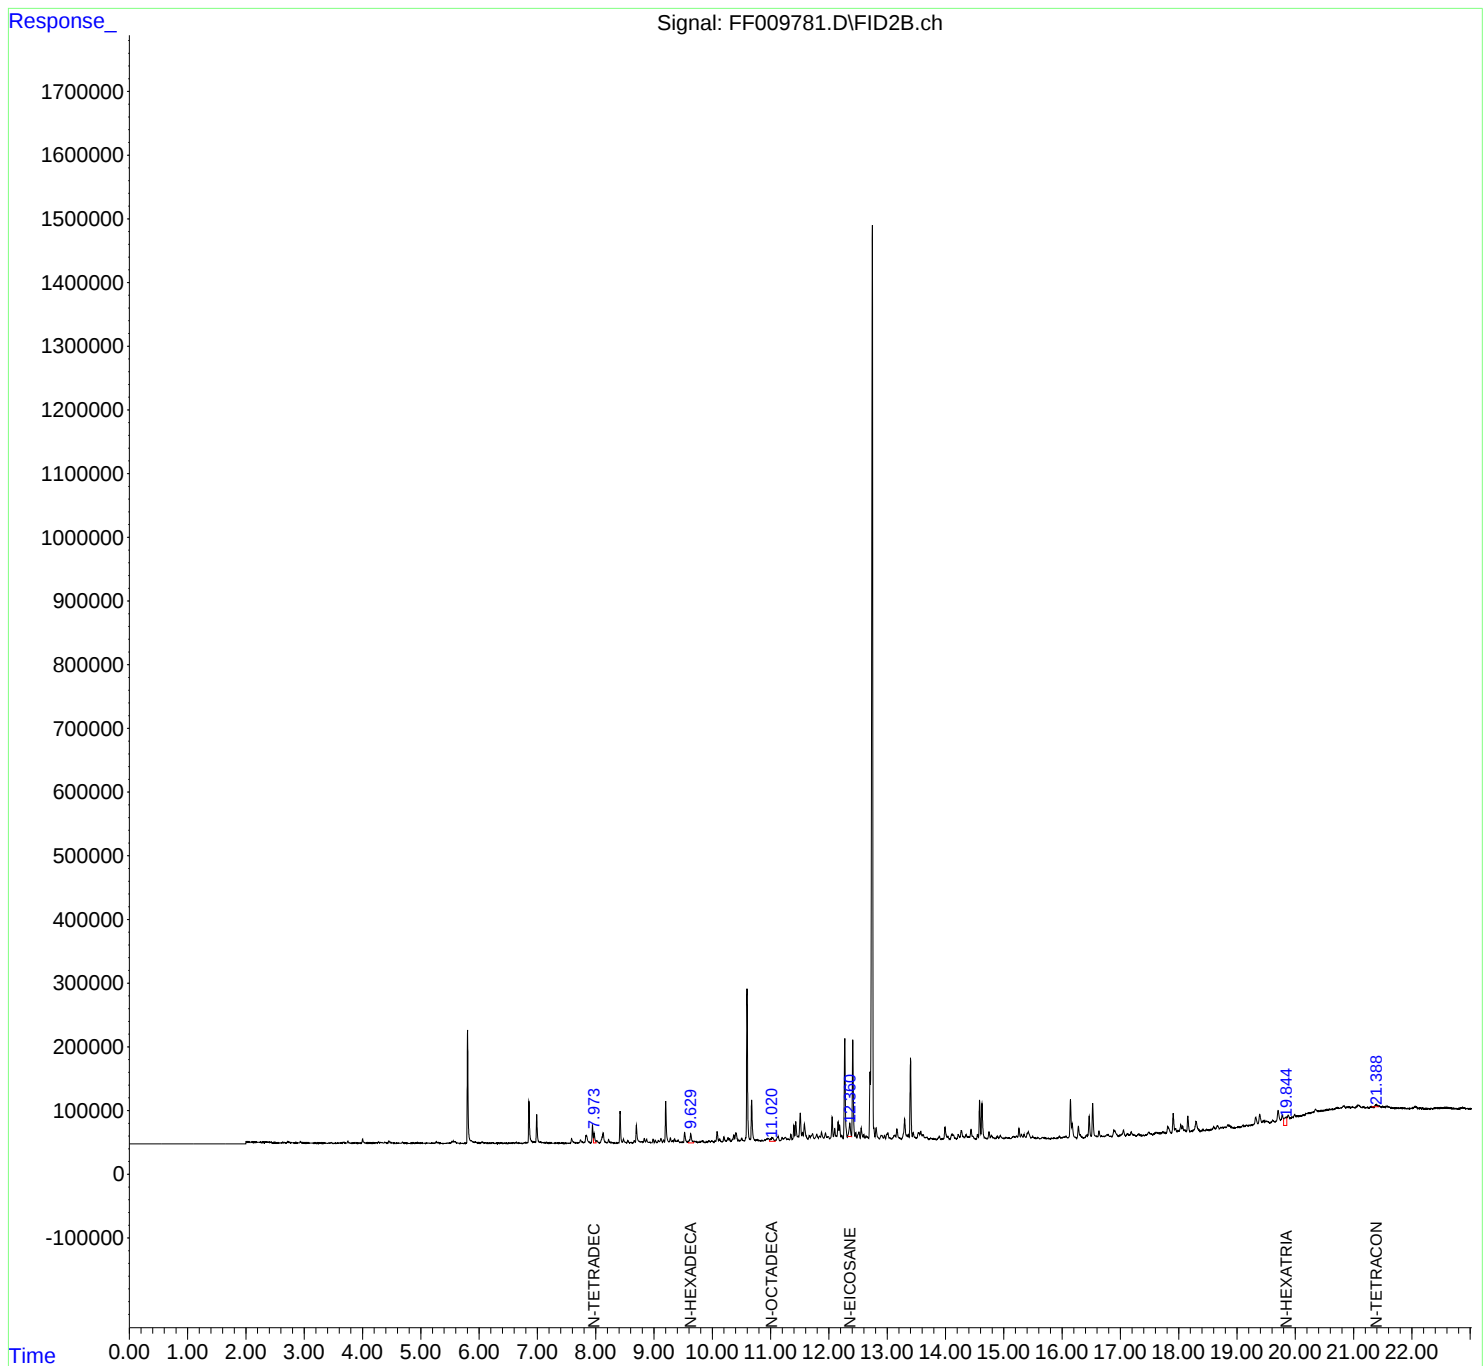


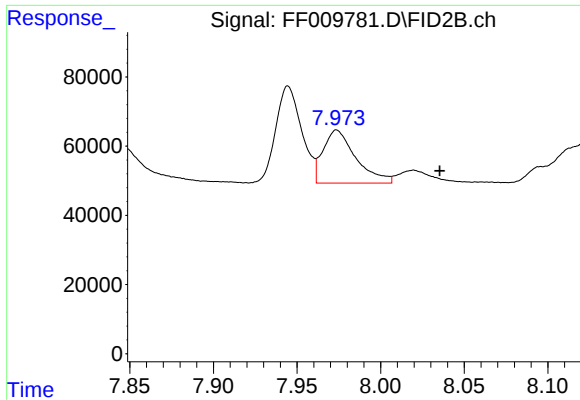

#4 N-TETRADECANE


R.T.: 7.974 min
Delta R.T.: -0.062 min
Response: 208835
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :

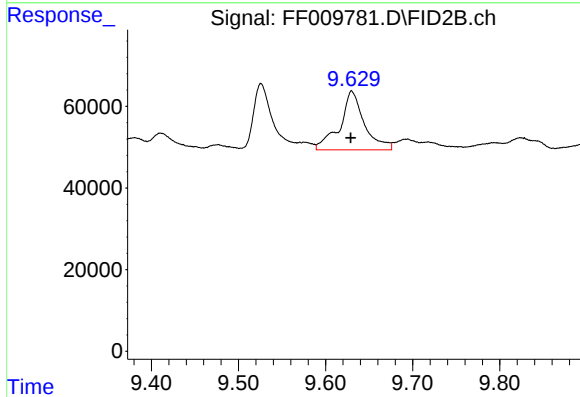


#5 N-HEXADECANE

R.T.: 9.630 min
Delta R.T.: 0.001 min
Response: 281983
Conc: 1.88 ug/ml

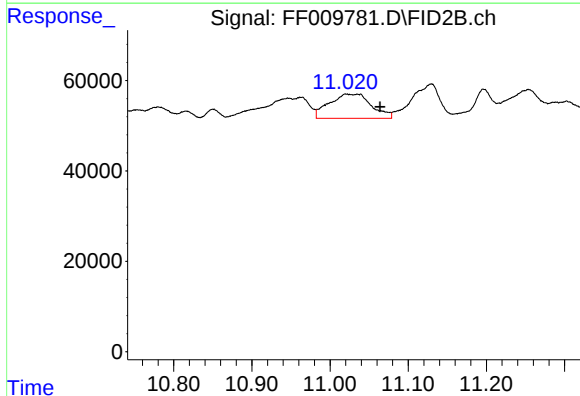


#6 N-OCTADECANE

R.T.: 11.021 min
Delta R.T.: -0.044 min
Response: 202029
Conc: 1.31 ug/ml

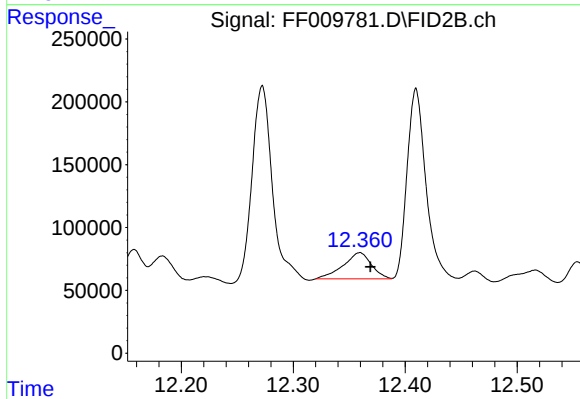

#7 N-EICOSANE


R.T.: 12.359 min
Delta R.T.: -0.010 min
Response: 363285
Conc: 2.40 ug/ml

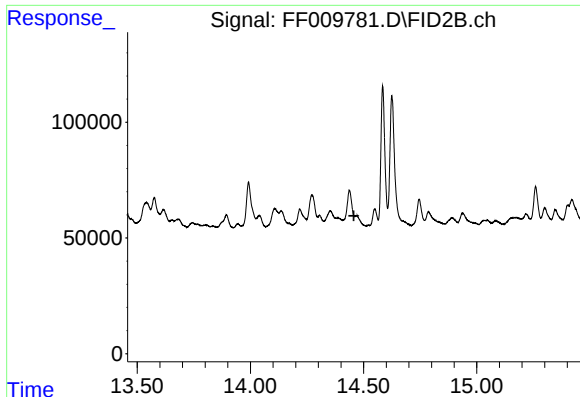

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.437 min
Delta R.T.: -0.020 min
Response: -1828483
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

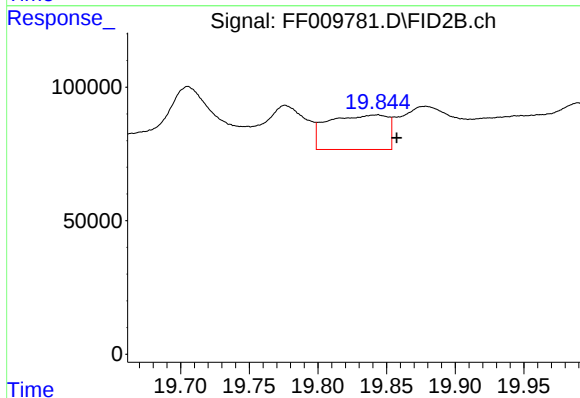

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.014 min
Response: 390283
Conc: 3.79 ug/ml

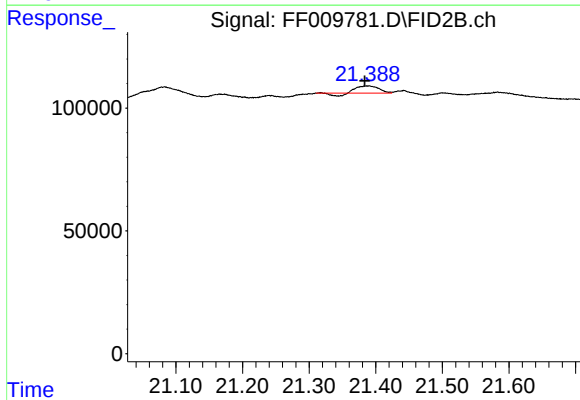

#18 N-TETRACONTANE

R.T.: 21.390 min
Delta R.T.: 0.006 min
Response: 57352
Conc: 0.63 ug/ml