

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009774.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 12:35
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Jan 24 20:40:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.236	3605234	25.194 ug/ml
12)	N-OCTACOSANE	16.608	3203875	22.071 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009774.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 12:35
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Jan 24 20:40:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

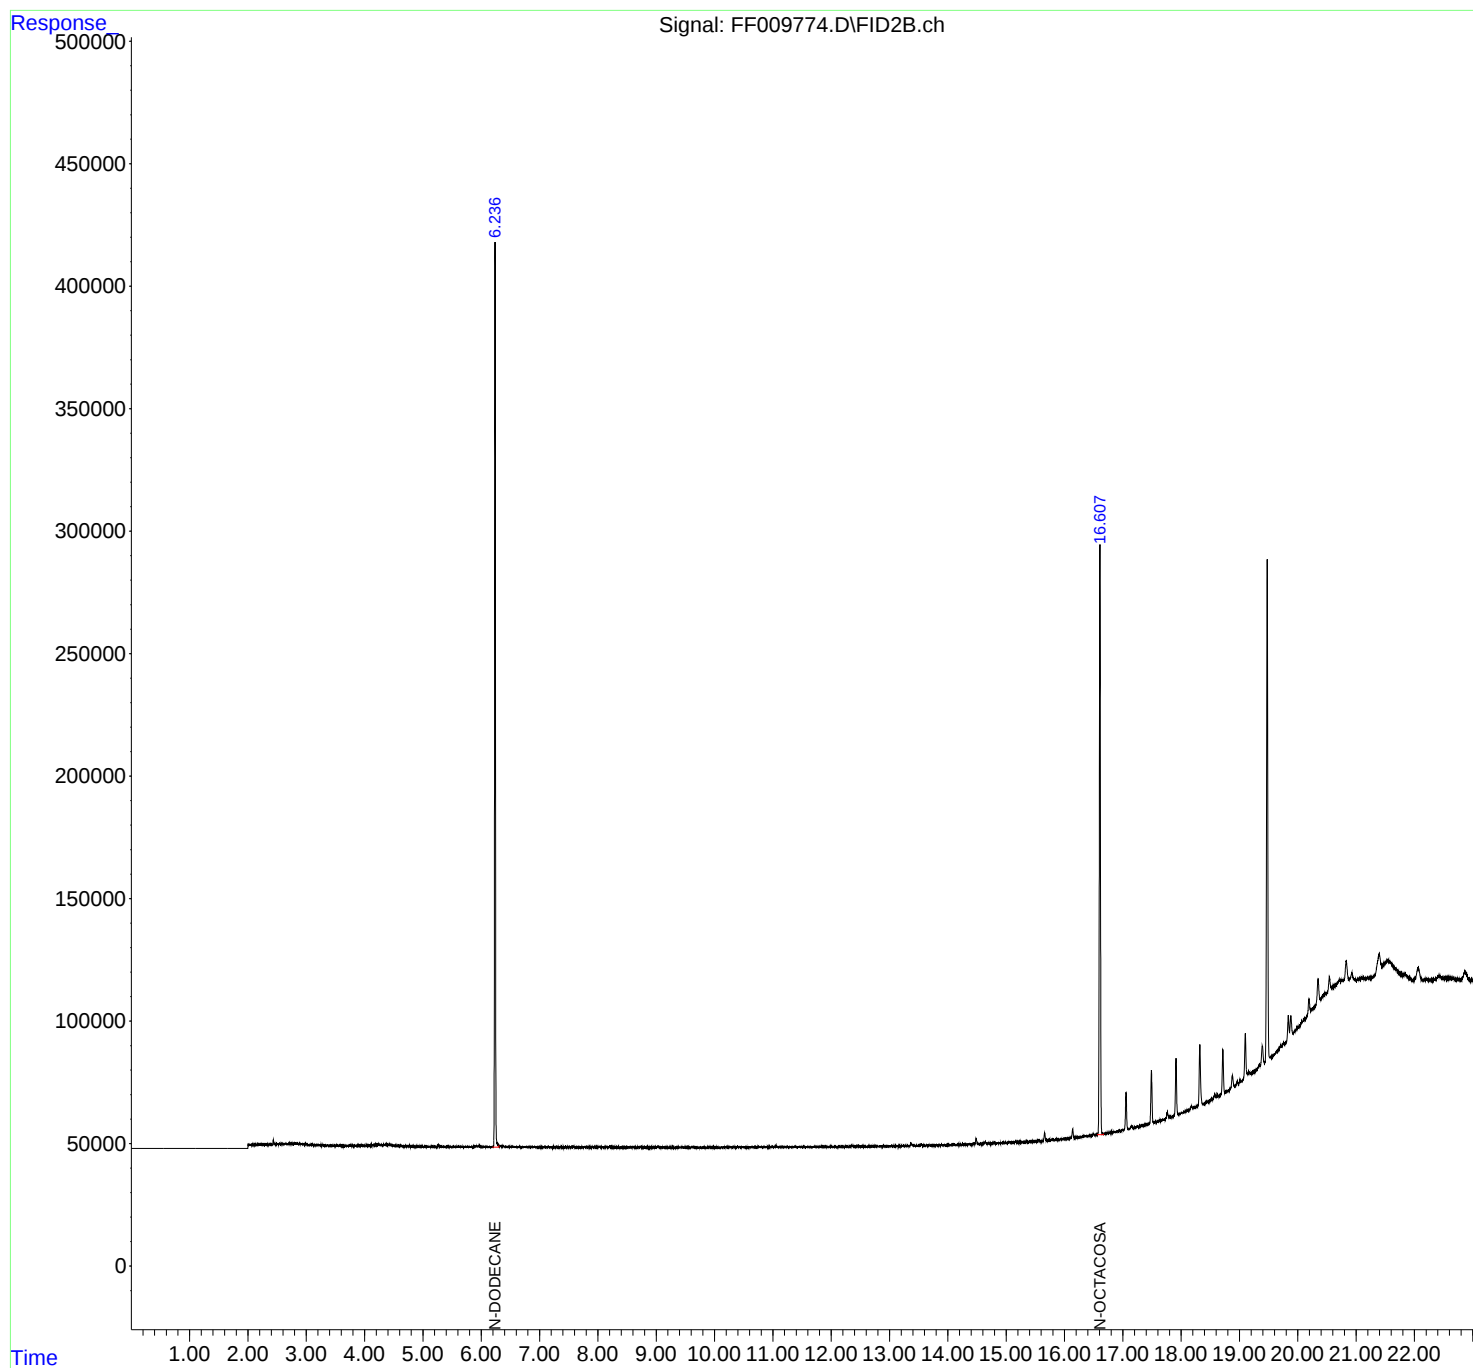


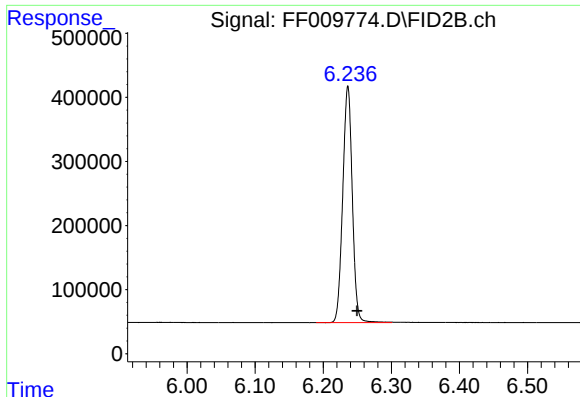

#3 N-DODECANE


R.T.: 6.236 min
Delta R.T.: -0.014 min
Response: 3605234
Conc: 25.19 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

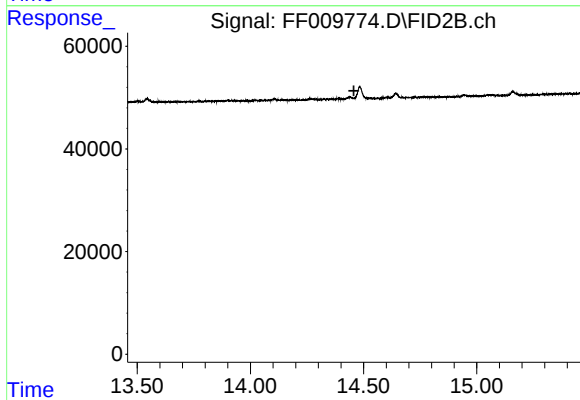

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

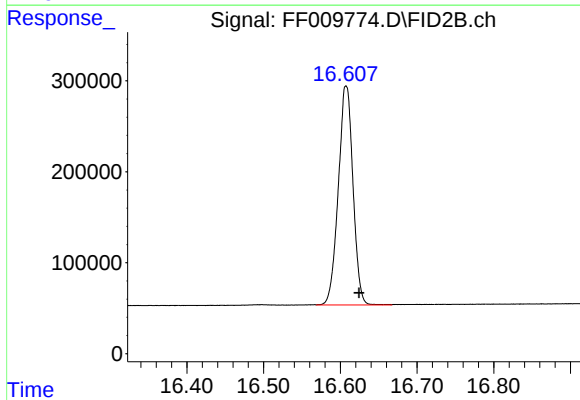

#12 N-OCTACOSANE

R.T.: 16.608 min
Delta R.T.: -0.017 min
Response: 3203875
Conc: 22.07 ug/ml