

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009775.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 14:13
Operator : AJ\MA
Sample : N1224-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-2-B-1@7-BGS

Integration File: Sample.e
Quant Time: Jan 24 20:40:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.437	1901803	14.553 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009775.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 14:13
Operator : AJ\MA
Sample : N1224-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-2-B-1@7-BGS

Integration File: Sample.e
Quant Time: Jan 24 20:40:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

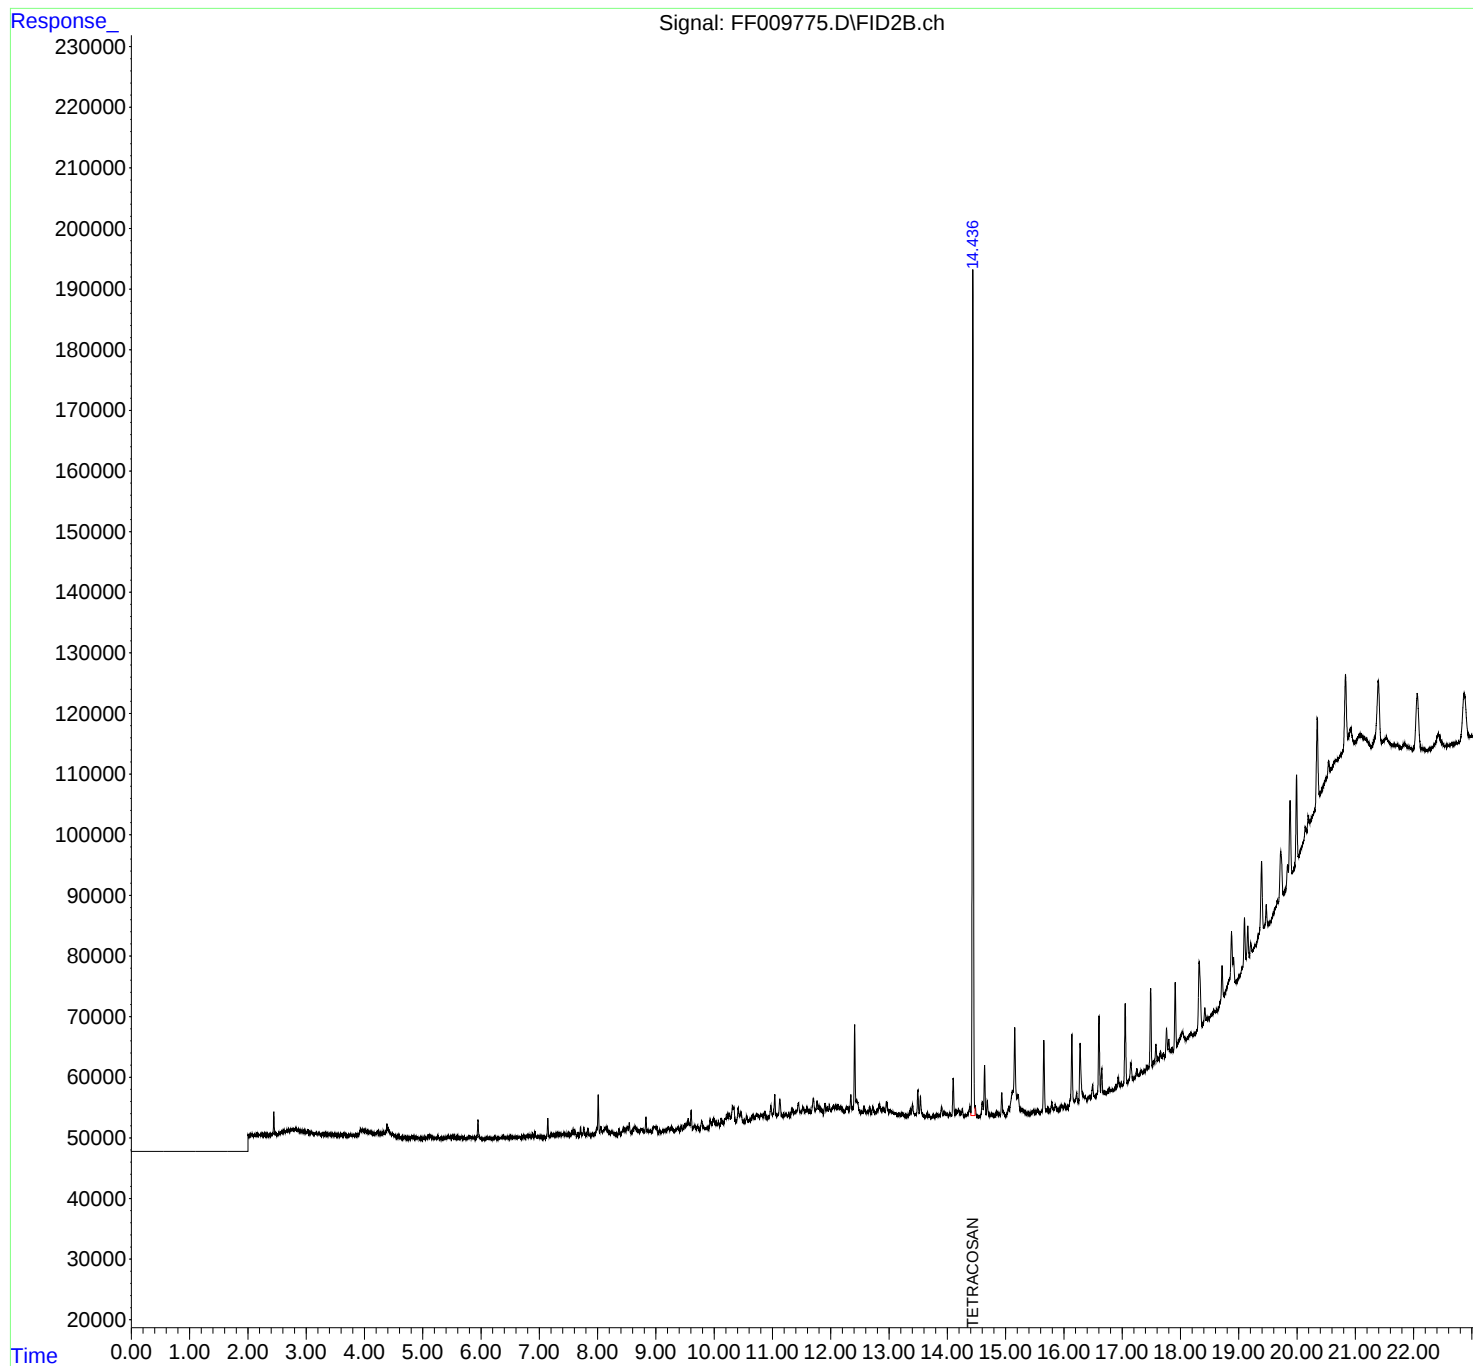

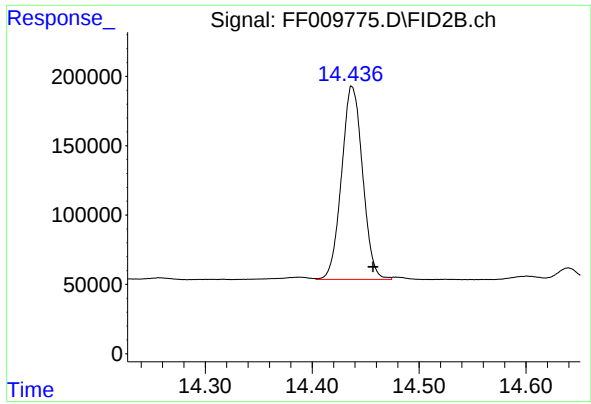

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.437 min
Delta R.T.: -0.020 min
Response: 1901803
Conc: 14.55 ug/ml

Instrument :
FID_F
ClientSampleId :
AREA-2-B-1@7-BGS