

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012422\  
 Data File : FF009779.D  
 Signal(s) : FID2B.ch  
 Acq On : 24 Jan 2022 16:11  
 Operator : AJ\MA  
 Sample : N1224-07 2X  
 Misc :  
 ALS Vial : 59 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 AREA-2-COMPOSITE

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 01/26/2022  
 Supervised By :Ankita Jodhani 01/26/2022

Integration File: Sample.e  
 Quant Time: Jan 24 20:41:52 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
 Quant Title :  
 QLast Update : Tue Jan 18 02:53:40 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.437 | 1205967  | 9.229 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012422\  
Data File : FF009779.D  
Signal(s) : FID2B.ch  
Acq On : 24 Jan 2022 16:11  
Operator : AJ\MA  
Sample : N1224-07 2X  
Misc :  
ALS Vial : 59 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
AREA-2-COMPOSITE


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/26/2022  
Supervised By :Ankita Jodhani 01/26/2022

Integration File: Sample.e  
Quant Time: Jan 24 20:41:52 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
Quant Title :  
QLast Update : Tue Jan 18 02:53:40 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

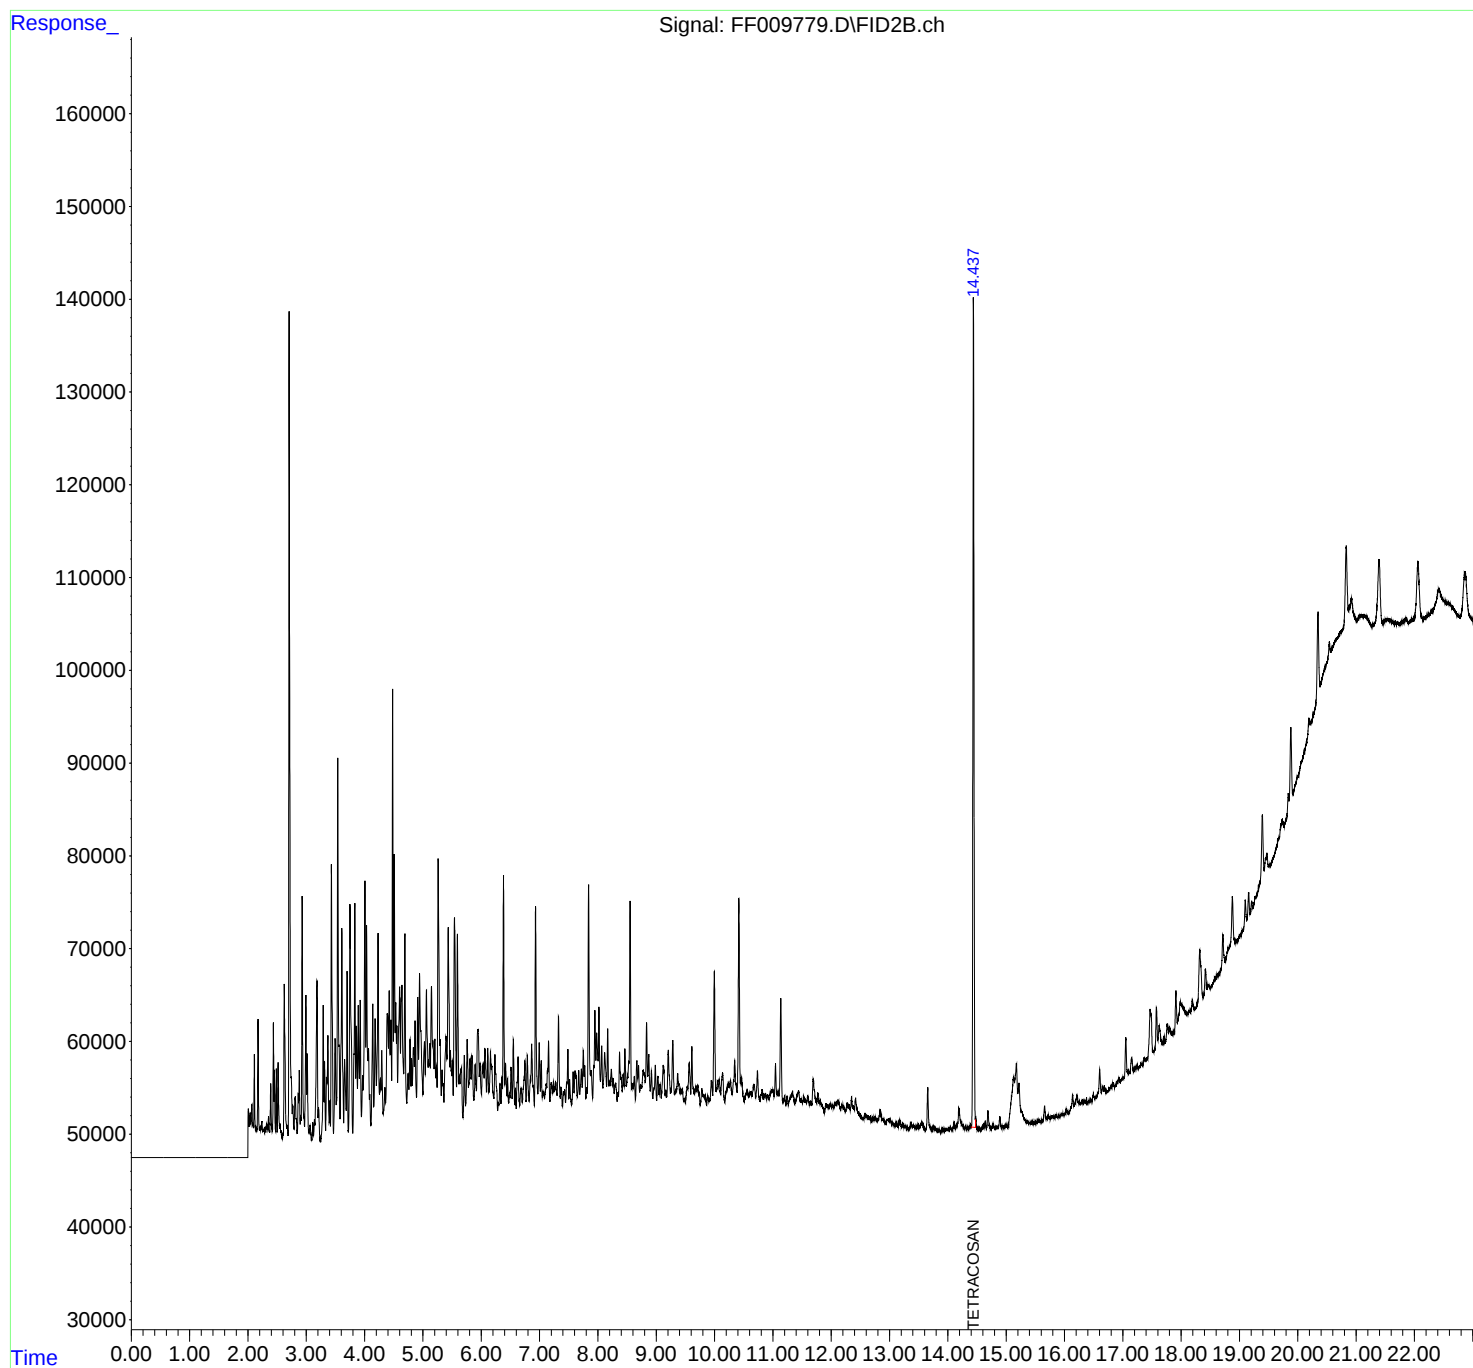

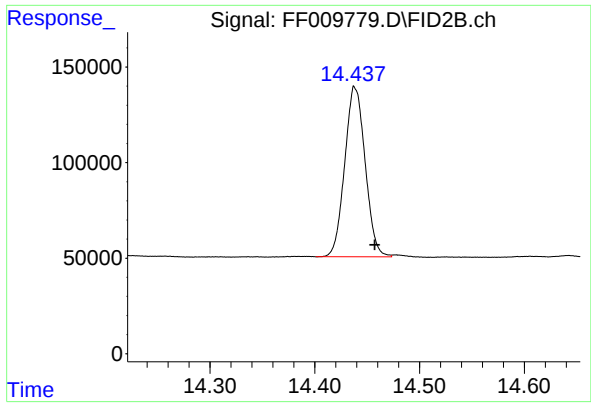

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.437 min  
Delta R.T.: -0.020 min  
Response: 1205967  
Conc: 9.23 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
AREA-2-COMPOSITE

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/26/2022  
Supervised By :Ankita Jodhani 01/26/2022