

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009780.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 16:40
Operator : AJ\MA
Sample : N1224-11 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-1-B-2@4-BGS

Integration File: Sample.e
Quant Time: Jan 24 20:42:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.438	443931	3.397 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012422\
Data File : FF009780.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2022 16:40
Operator : AJ\MA
Sample : N1224-11 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AREA-1-B-2@4-BGS

Integration File: Sample.e
Quant Time: Jan 24 20:42:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

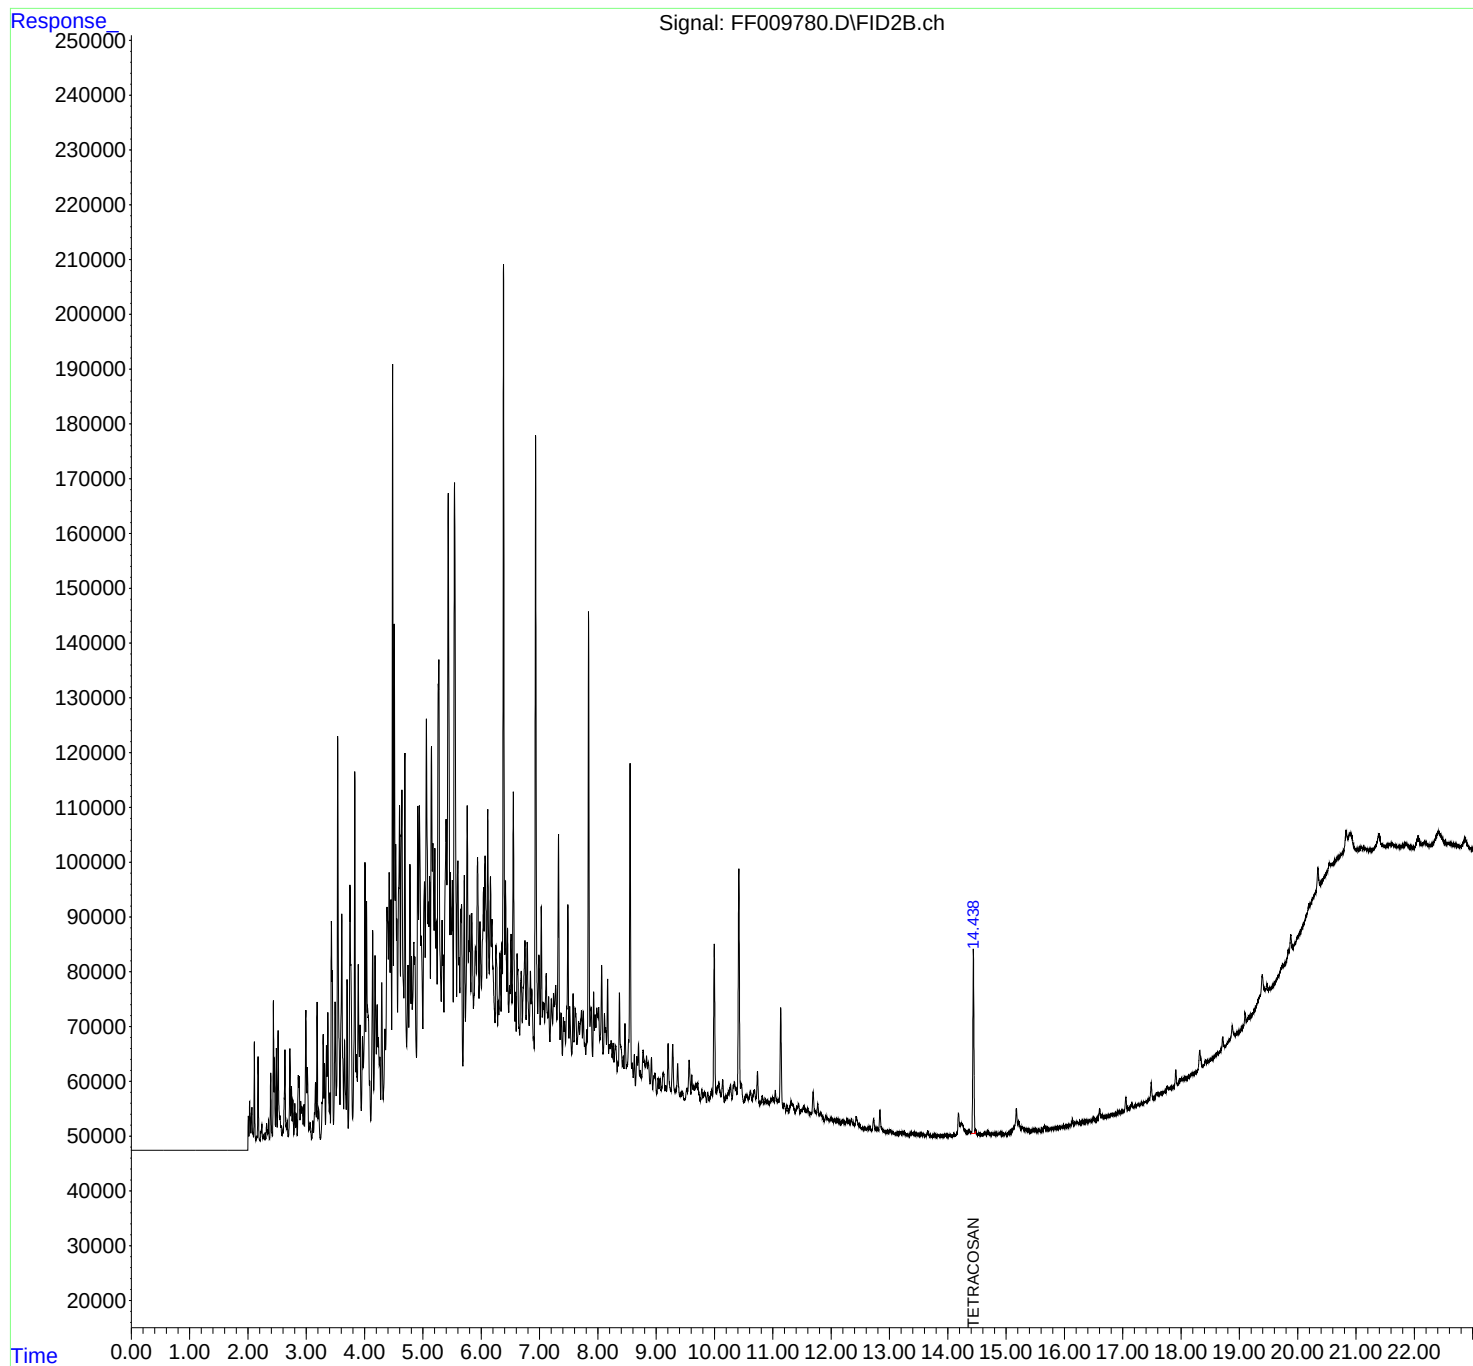

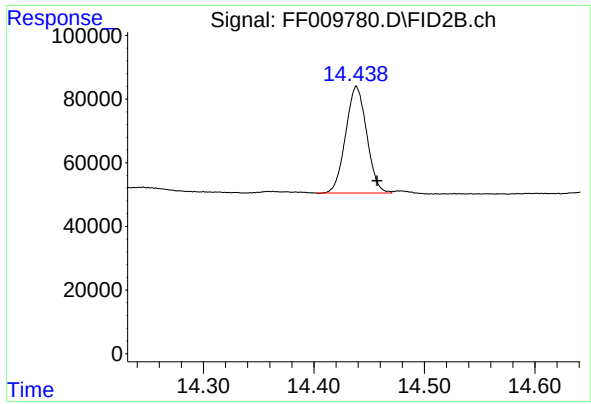

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.438 min
Delta R.T.: -0.019 min
Response: 443931
Conc: 3.40 ug/ml

Instrument :

FID_F

ClientSampleId :

AREA-1-B-2@4-BGS