

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012425\
Data File : FF015310.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 13:36
Operator : YP\AJ
Sample : PB166220BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB166220BL

Integration File: autoint1.e
Quant Time: Jan 24 23:30:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.021	2068396	15.796 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012425\
Data File : FF015310.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 13:36
Operator : YP\AJ
Sample : PB166220BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB166220BL

Integration File: autoint1.e
Quant Time: Jan 24 23:30:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

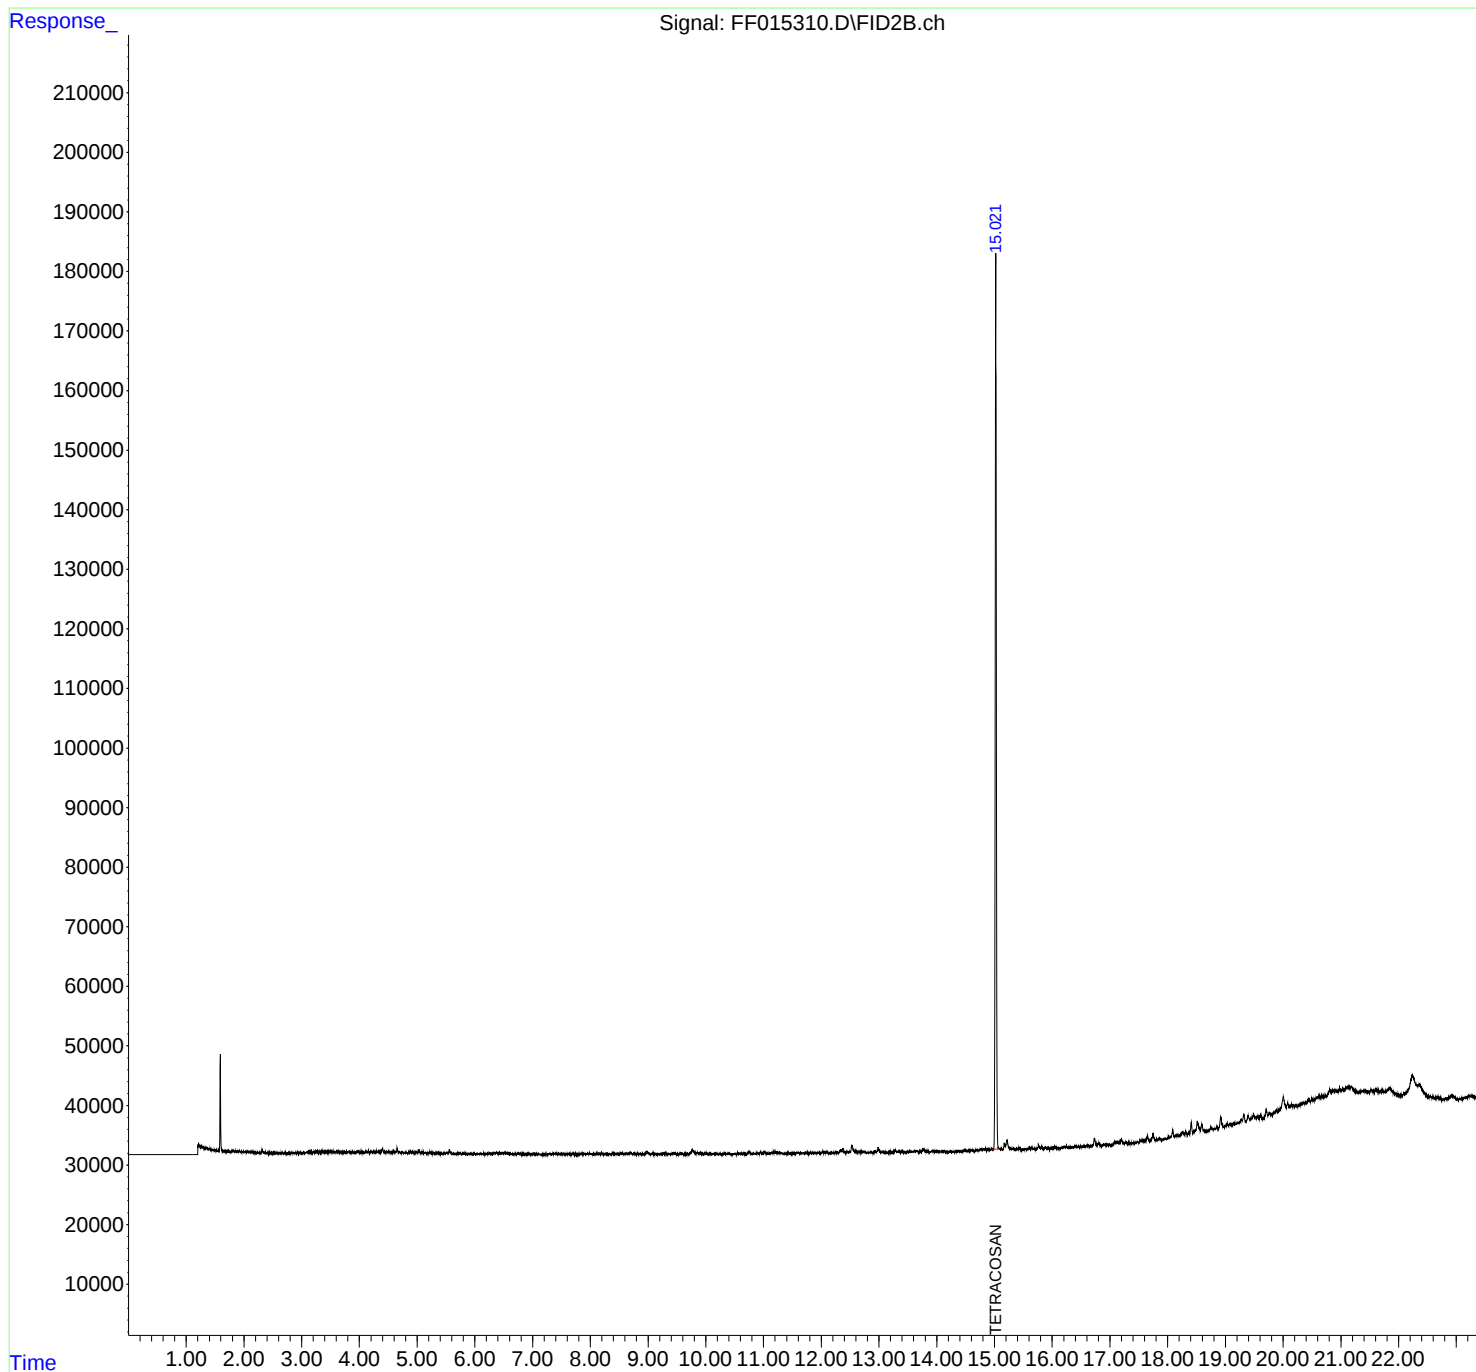

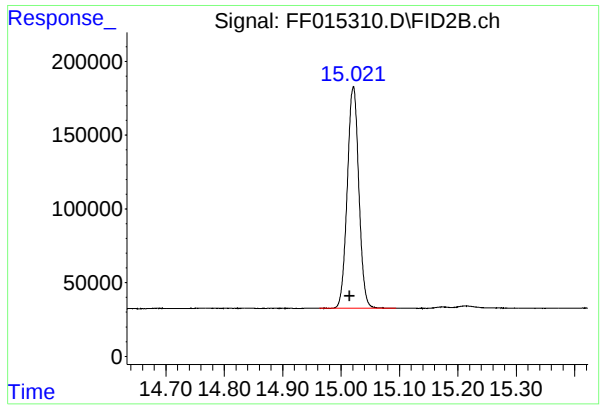

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.021 min
Delta R.T.: 0.007 min
Response: 2068396
Conc: 15.80 ug/ml

Instrument :
FID_F
ClientSampleId :
PB166220BL